


Data Path : Z:\HPCHEM1\BNA_F\Data\BF041615\
 Data File : BF078585.D
 Acq On : 17 Apr 2015 1:39
 Operator : TP/IZ
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF031115.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Tue Mar 31 14:58:34 2015

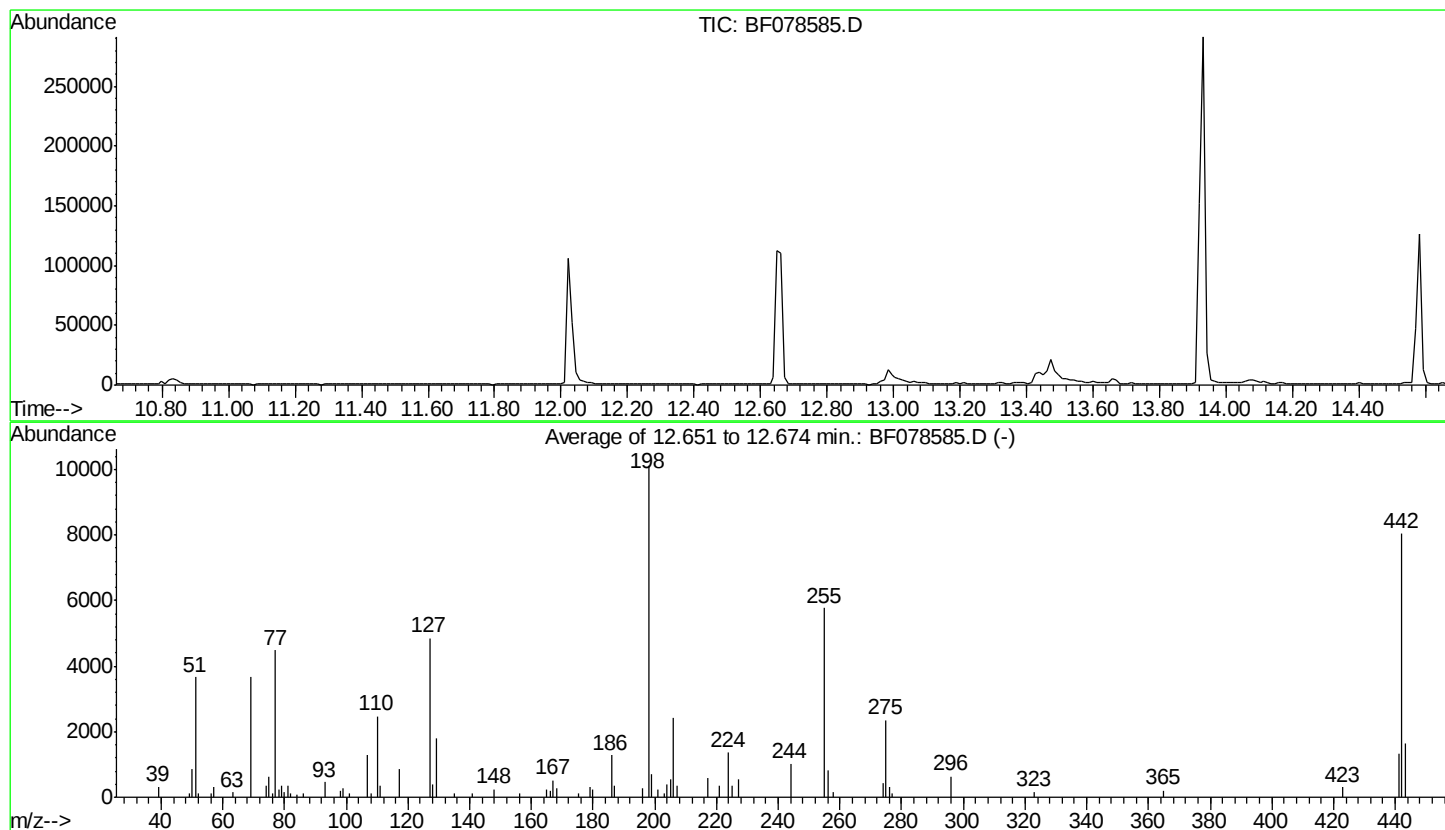

AutoFind: Scans 1003, 1004, 1005; Background Corrected with Scan 999

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	36.3	3665	PASS
68	69	0.00	2	0.0	0	PASS
69	198	0.00	100	36.4	3679	PASS
70	69	0.00	2	0.0	0	PASS
127	198	10	80	48.1	4858	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	10110	PASS
199	198	5	9	7.0	703	PASS
275	198	10	60	23.2	2349	PASS
365	198	1	100	2.1	210	PASS
441	442	0.01	24	16.6	1332	PASS
442	198	50	100	79.5	8036	PASS
443	442	15	24	20.4	1636	PASS