


Data Path : Z:\HPCHEM1\BNA F\Data\BF041618\
Data File : BF104523.D
Acq On : 16 Apr 2018 10:14
Operator : JU/SJ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF040618.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Mon Apr 16 12:15:25 2018

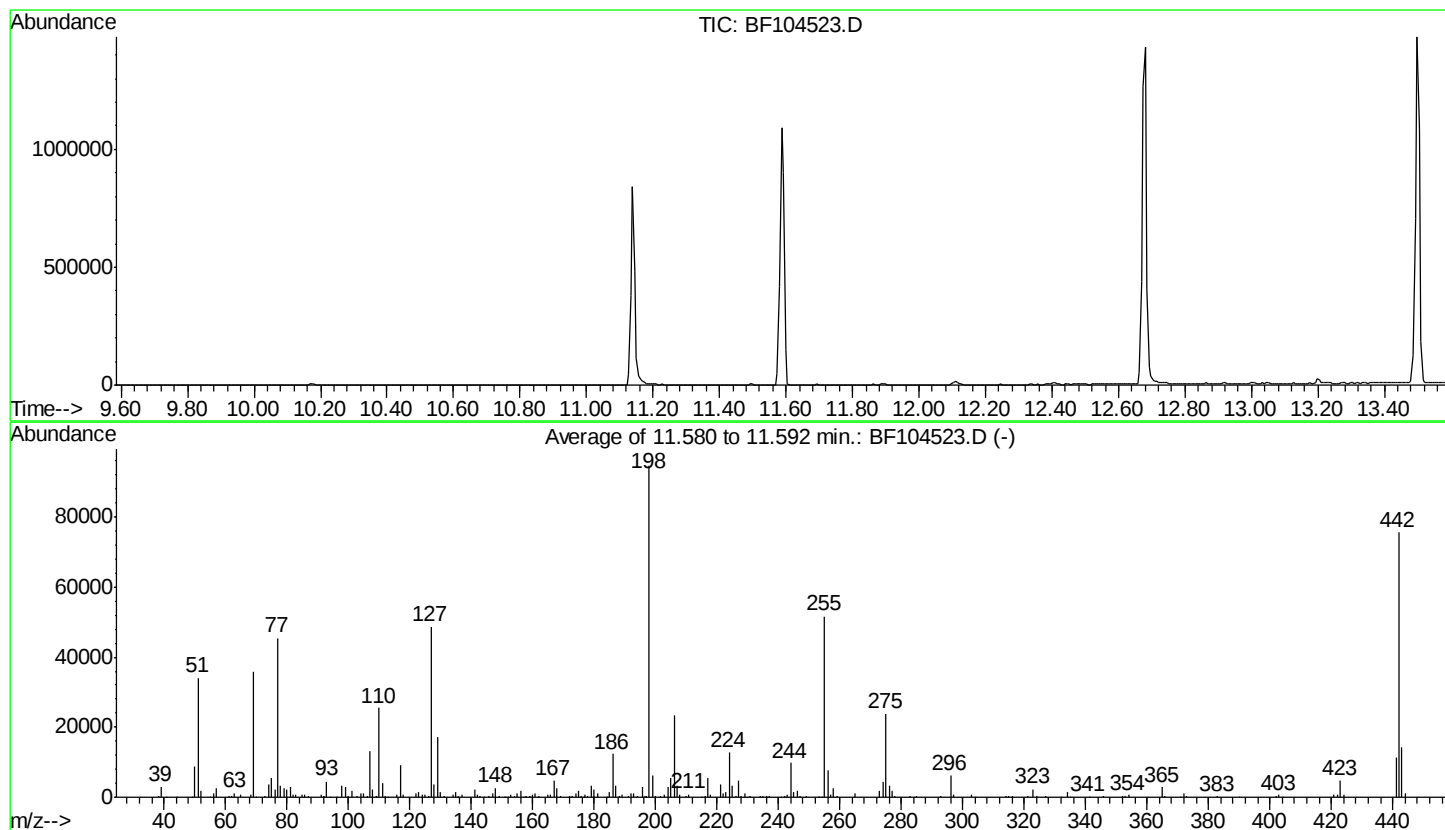

AutoFind: Scans 1614, 1615, 1616; Background Corrected with Scan 1610

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	35.9	34010	PASS
68	69	0.00	2	2.0	721	PASS
69	198	0.00	100	37.9	35856	PASS
70	69	0.00	2	0.4	132	PASS
127	198	10	80	51.4	48674	PASS
197	198	0.00	2	0.5	471	PASS
198	198	100	100	100.0	94704	PASS
199	198	5	9	6.6	6296	PASS
275	198	10	60	25.3	23938	PASS
365	198	1	100	3.0	2874	PASS
441	443	0.01	100	79.6	11356	PASS
442	198	50	100	79.8	75546	PASS
443	442	15	24	18.9	14261	PASS