


Data Path : Z:\HPCHEM1\BNA F\Data\BF041618\
 Data File : BF104536.D
 Acq On : 16 Apr 2018 16:47
 Operator : JU/SJ
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF040618.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Mon Apr 16 12:15:25 2018

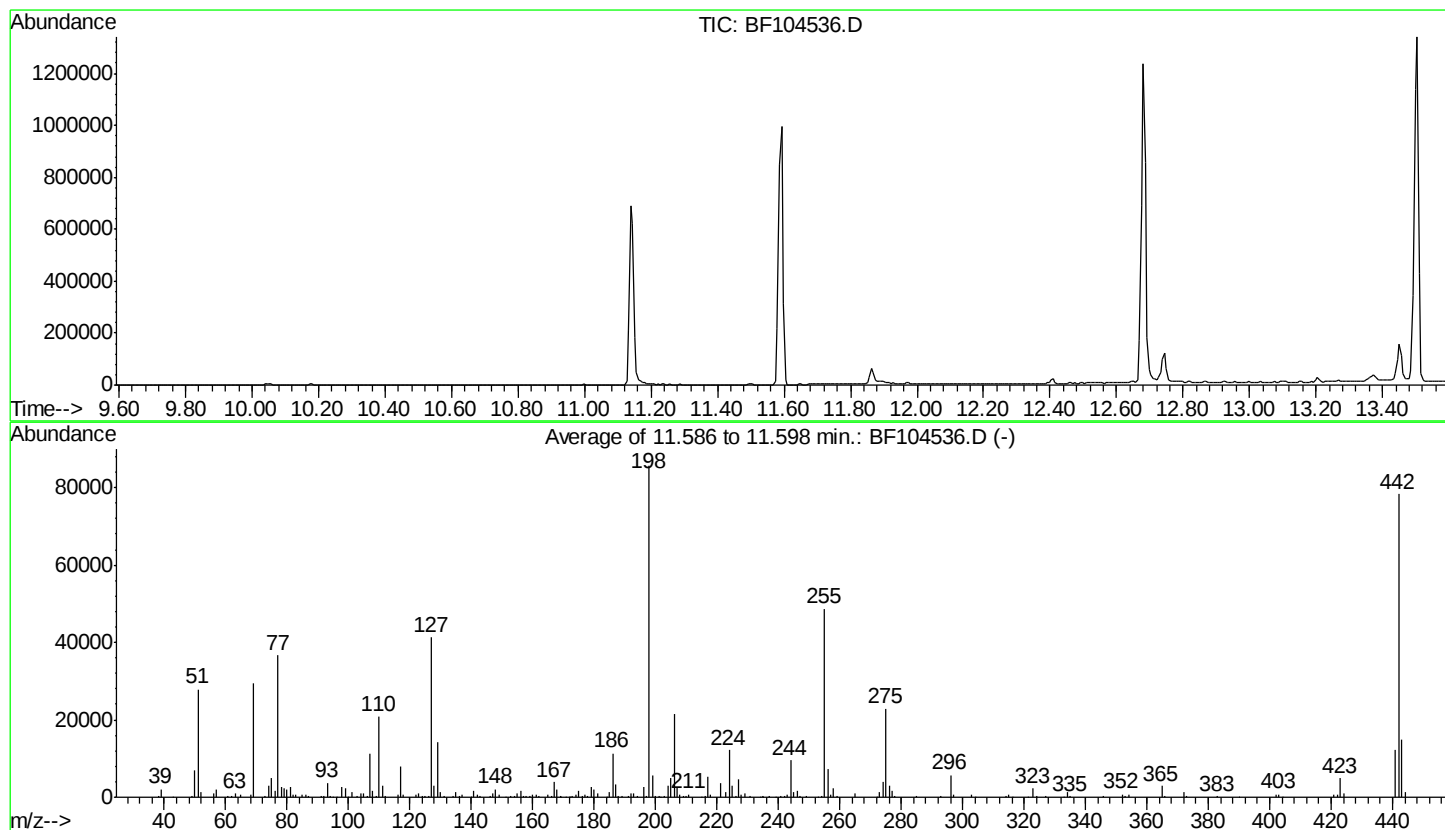

AutoFind: Scans 1615, 1616, 1617; Background Corrected with Scan 1610

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	32.6	27915	PASS
68	69	0.00	2	1.9	574	PASS
69	198	0.00	100	34.4	29496	PASS
70	69	0.00	2	0.0	0	PASS
127	198	10	80	48.1	41250	PASS
197	198	0.00	2	0.5	438	PASS
198	198	100	100	100.0	85677	PASS
199	198	5	9	6.7	5722	PASS
275	198	10	60	26.8	22972	PASS
365	198	1	100	3.4	2901	PASS
441	443	0.01	100	82.5	12307	PASS
442	198	50	100	91.4	78266	PASS
443	442	15	24	19.1	14912	PASS