

Data Path : Z:\HPCHEM1\BNA_F\DATA\BF041715\
 Data File : BF078612.D
 Acq On : 17 Apr 2015 18:29
 Operator : TP/IZ
 Sample : G1871-03
 Misc :
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 MW-47

Quant Time: Apr 17 23:44:55 2015
 Quant Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF040115.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Apr 17 23:28:12 2015
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	6.67	152	44146	20.00	ng	0.00
21) Naphthalene-d8	8.25	136	181159	20.00	ng	0.00
38) Acenaphthene-d10	10.40	164	91779	20.00	ng	-0.01
63) Phenanthrene-d10	12.22	188	186950	20.00	ng	0.00
75) Chrysene-d12	15.46	240	222785	20.00	ng	0.00
86) Perylene-d12	17.14	264	220179	20.00	ng	-0.01
System Monitoring Compounds						
5) 2-Fluorophenol	4.90	112	140654	52.53	ng	0.00
7) Phenol-d6	6.27	99	110723	33.00	ng	-0.01
23) Nitrobenzene-d5	7.38	82	242289	81.07	ng	0.00
41) 2,4,6-Tribromophenol	11.38	330	113985	149.75	ng	0.00
44) 2-Fluorobiphenyl	9.60	172	486785	75.81	ng	0.00
78) Terphenyl-d14	14.21	244	633377	64.24	ng	0.00


Target Compounds	Qvalue
------------------	--------


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\HPCHEM1\BNA_F\DATA\BF041715\
Data File : BF078612.D
Acq On : 17 Apr 2015 18:29
Operator : TP/IZ
Sample : G1871-03
Misc :
ALS Vial : 12 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
MW-47

Quant Time: Apr 17 23:44:55 2015
Quant Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF040115.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Apr 17 23:28:12 2015
Response via : Initial Calibration

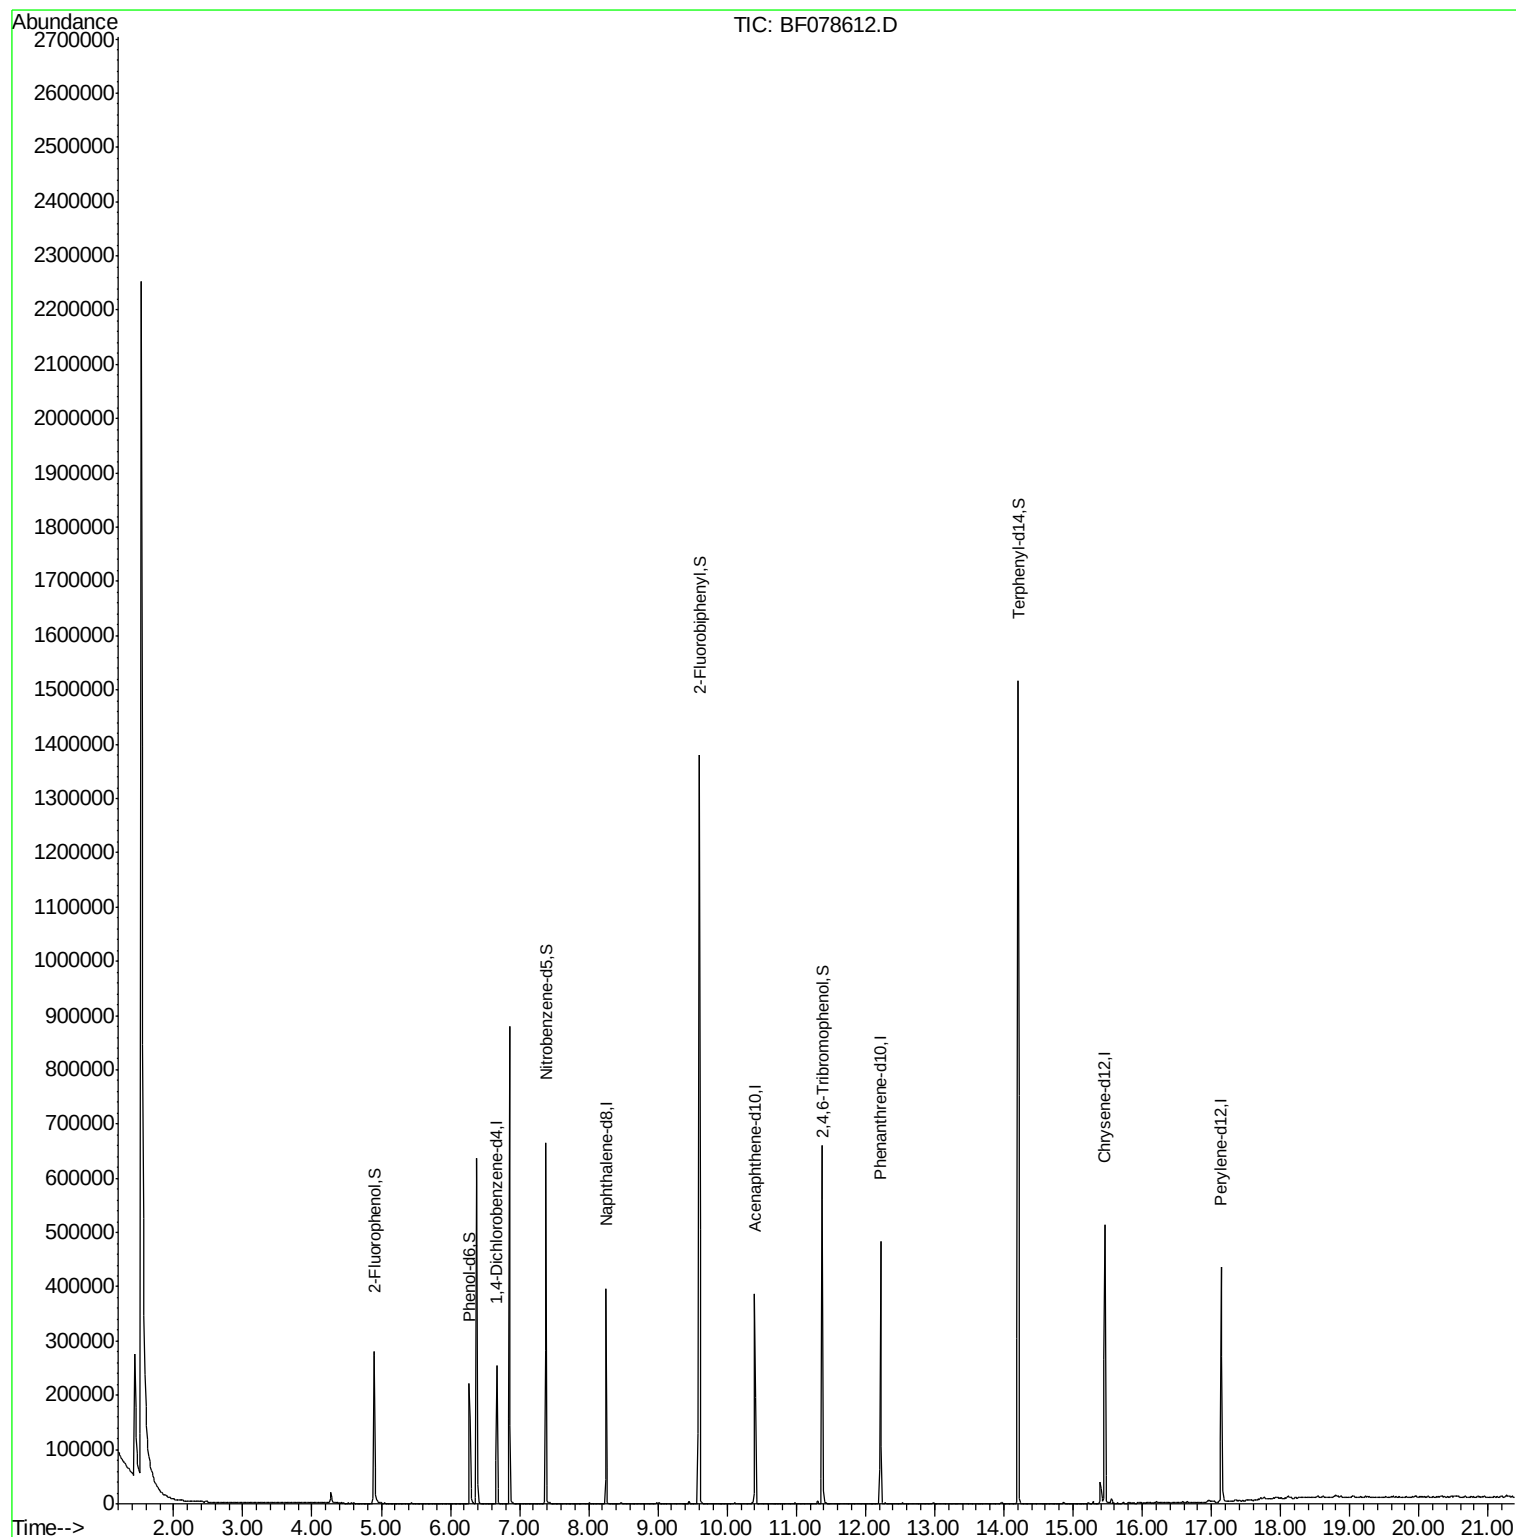




#1




1,4-Dichlorobenzene-d4
Concen: 20.00 ng
RT: 6.67 min Scan# 480
Delta R.T. 0.00 min
Lab File: BF078612.D
Acq: 17 Apr 2015 18:29

Instrument :
BNA_F
ClientSampleId :
MW-47

Tgt Ion:152 Resp: 44146
Ion Ratio Lower Upper
152 100
150 153.1 125.9 188.9
115 55.5 52.7 79.1

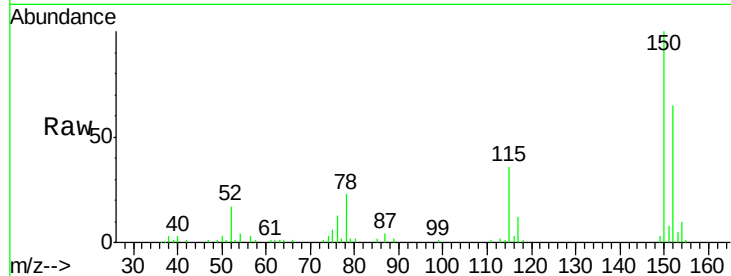


Abundance Ion 152.00 (151.70 to 152.70): E
Ion 150.00 (149.70 to 150.70): E
Ion 115.00 (114.70 to 115.70): E

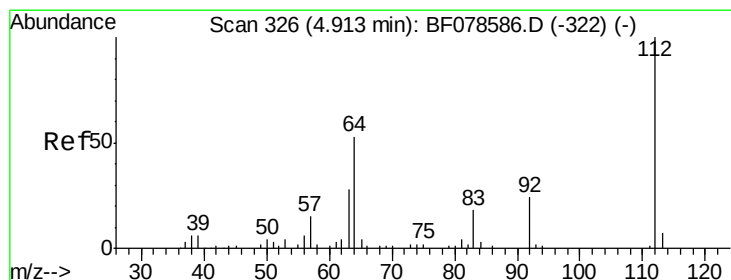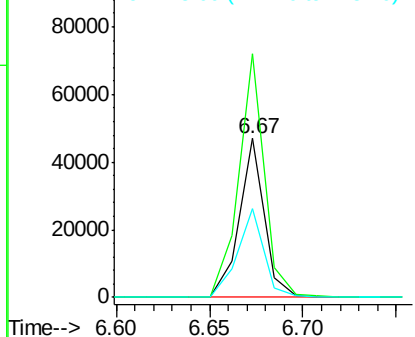



#5


2-Fluorophenol
Concen: 52.53 ng
RT: 4.90 min Scan# 325
Delta R.T. 0.00 min
Lab File: BF078612.D
Acq: 17 Apr 2015 18:29

Tgt Ion:112 Resp: 140654
Ion Ratio Lower Upper
112 100
64 48.7 39.9 59.9
63 24.8 20.2 30.4

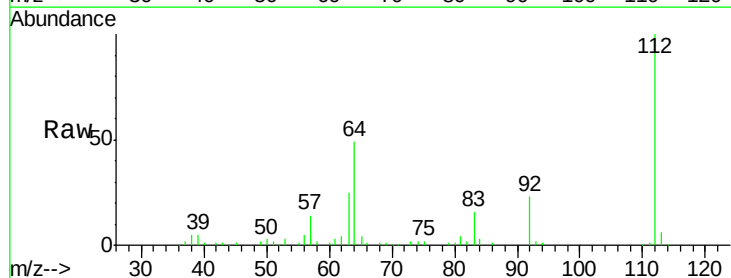

Abundance Ion 112.00 (111.70 to 112.70): E
Ion 64.00 (63.70 to 64.70): BF0
Ion 63.00 (62.70 to 63.70): BF0

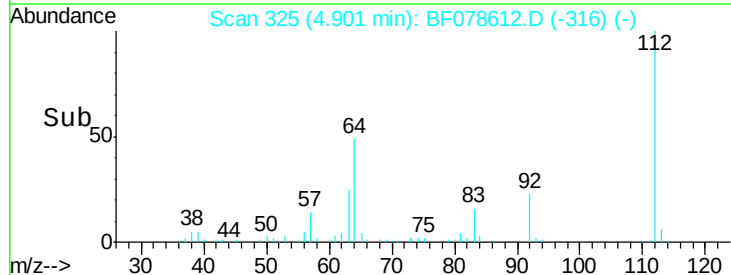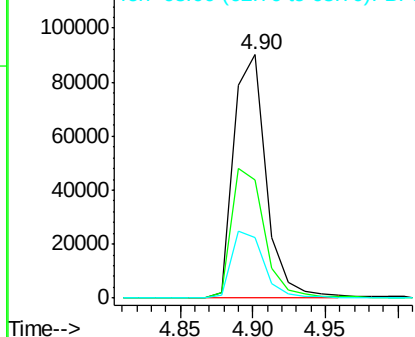



#7

Phenol-d6

Concen: 33.00 ng

RT: 6.27 min Scan# 445

Delta R.T. -0.01 min

Lab File: BF078612.D

Acq: 17 Apr 2015 18:29

Instrument :

BNA_F

ClientSampleId :

MW-47


Tgt Ion: 99 Resp: 110723

Ion Ratio Lower Upper

99 100

42 19.4 14.8 22.2




71 34.2 26.6 39.8

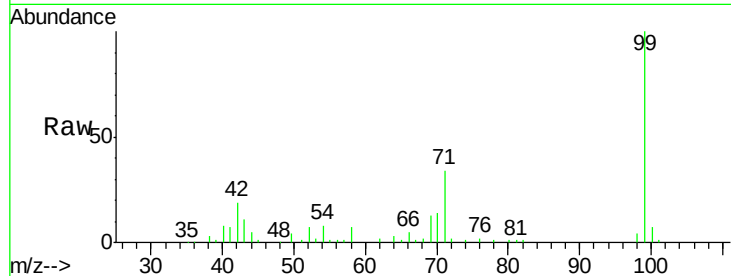

Abundance Ion 99.00 (98.70 to 99.70): BF0

Ion 42.00 (41.70 to 42.70): BF0

Ion 71.00 (70.70 to 71.70): BF0

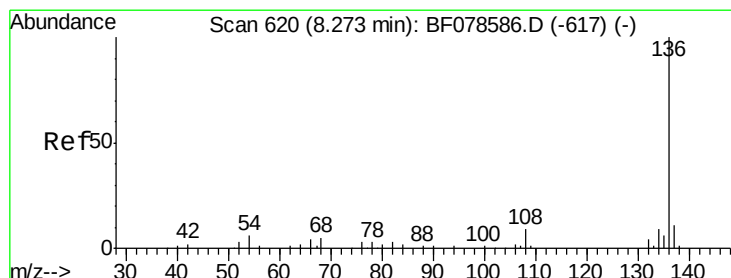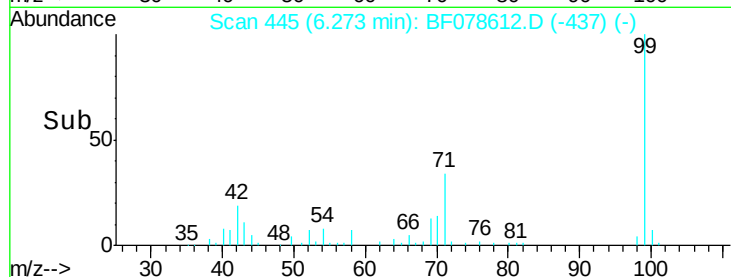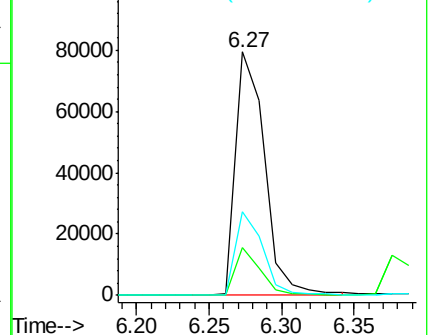

#21

Naphthalene-d8

Concen: 20.00 ng

RT: 8.25 min Scan# 618

Delta R.T. 0.00 min

Lab File: BF078612.D

Acq: 17 Apr 2015 18:29

Tgt Ion: 136 Resp: 181159


Ion Ratio Lower Upper

136 100

137 10.9 9.0 13.4

54 7.5 7.0 10.6

68 5.5 5.4 8.2


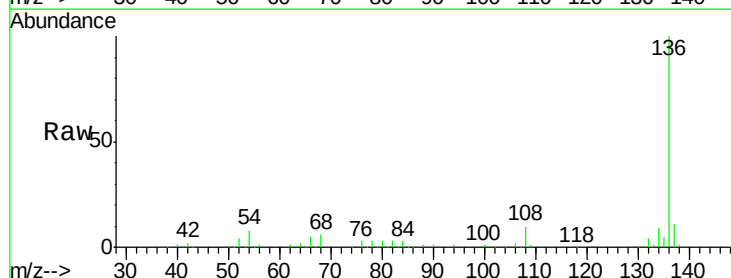



Abundance Ion 136.00 (135.70 to 136.70): E

Ion 137.00 (136.70 to 137.70): E

Ion 54.00 (53.70 to 54.70): BF0

Ion 68.00 (67.70 to 68.70): BF0

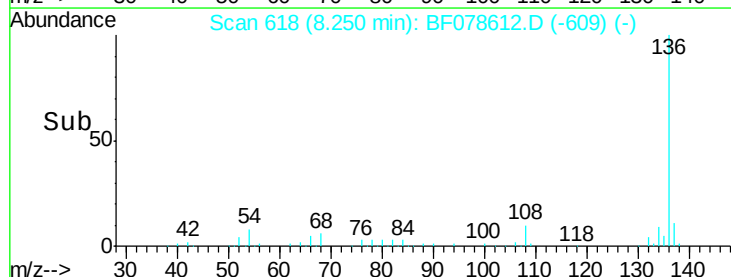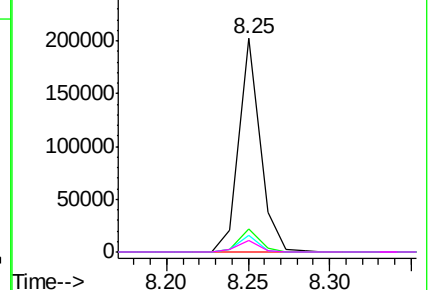

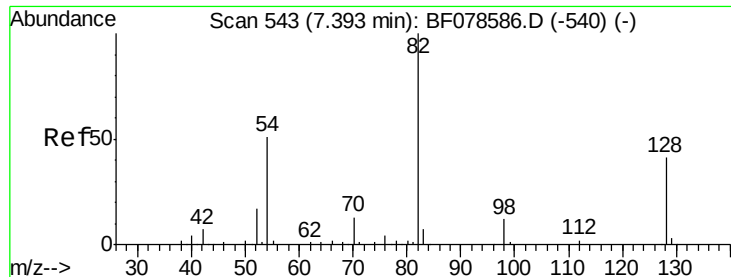

#23

Nitrobenzene-d5

Concen: 81.07 ng

RT: 7.38 min Scan# 542

Delta R.T. 0.00 min

Lab File: BF078612.D

Acq: 17 Apr 2015 18:29

Instrument :

BNA_F

ClientSampleId :

MW-47


Tgt Ion: 82 Resp: 242289

Ion Ratio Lower Upper

82 100

128 46.9 31.8 47.8




54 45.4 41.5 62.3

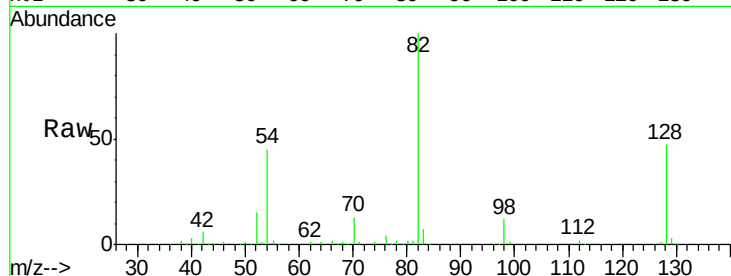

Abundance Ion 82.00 (81.70 to 82.70): BF0

Ion 128.00 (127.70 to 128.70): BF0

Ion 54.00 (53.70 to 54.70): BF0

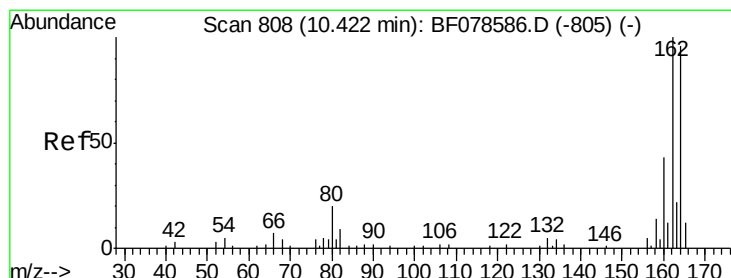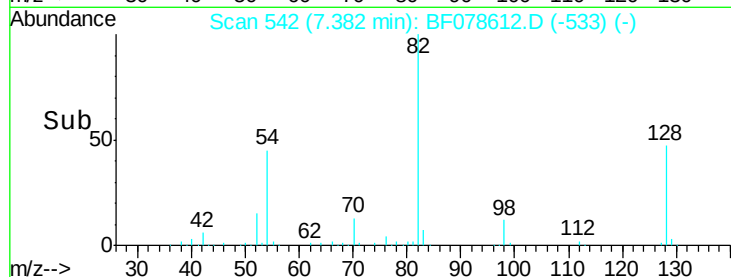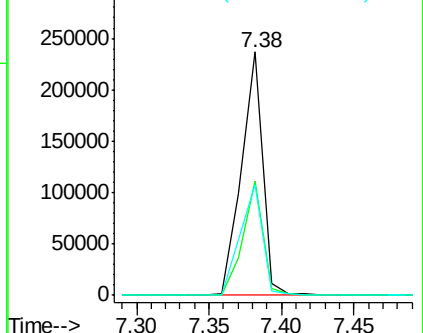

#38

Acenaphthene-d10

Concen: 20.00 ng

RT: 10.40 min Scan# 806

Delta R.T. -0.01 min

Lab File: BF078612.D

Acq: 17 Apr 2015 18:29


Tgt Ion: 164 Resp: 91779

Ion Ratio Lower Upper

164 100

162 103.8 82.2 123.2



160 45.2 34.7 52.1

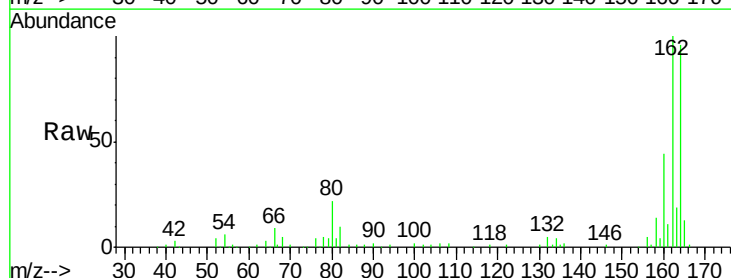


Abundance Ion 164.00 (163.70 to 164.70): E

Ion 162.00 (161.70 to 162.70): E

Ion 160.00 (159.70 to 160.70): E

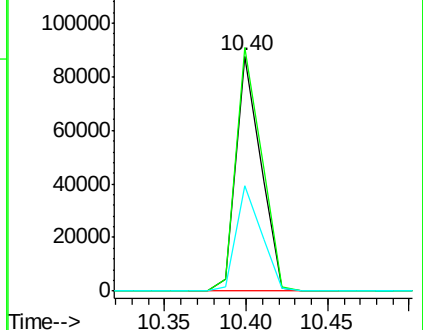







#41
 2,4,6-Tribromophenol
 Concen: 149.75 ng
 RT: 11.38 min Scan# 892
 Delta R.T. 0.00 min
 Lab File: BF078612.D
 Acq: 17 Apr 2015 18:29

Instrument :
 BNA_F
 ClientSampleId :
 MW-47

Tgt Ion:330 Resp: 113985
 Ion Ratio Lower Upper
 330 100
 332 96.5 78.6 117.8
 141 35.3 31.2 46.8

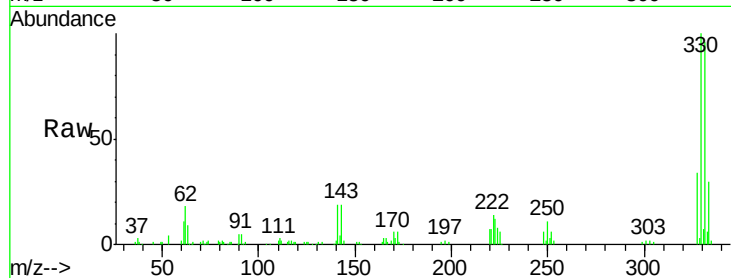


Abundance Ion 329.80 (329.50 to 330.50): E
 Ion 331.80 (331.50 to 332.50): E
 Ion 141.00 (140.70 to 141.70): E

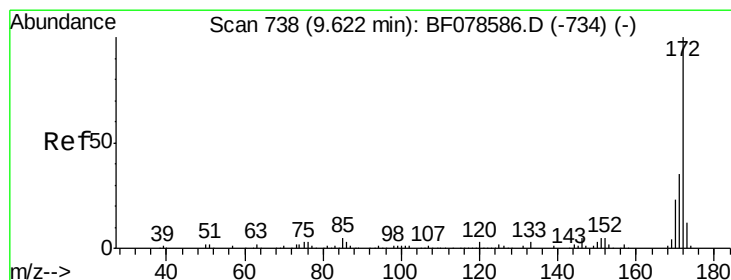
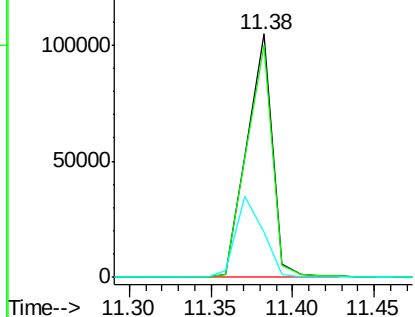



#44
 2-Fluorobiphenyl
 Concen: 75.81 ng
 RT: 9.60 min Scan# 736
 Delta R.T. 0.00 min
 Lab File: BF078612.D
 Acq: 17 Apr 2015 18:29

Tgt Ion:172 Resp: 486785
 Ion Ratio Lower Upper
 172 100
 171 35.7 28.6 42.8
 170 23.4 18.5 27.7

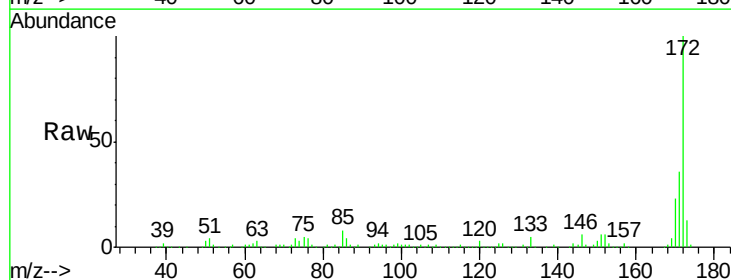

Abundance Ion 172.00 (171.70 to 172.70): E
 Ion 171.00 (170.70 to 171.70): E
 Ion 170.00 (169.70 to 170.70): E




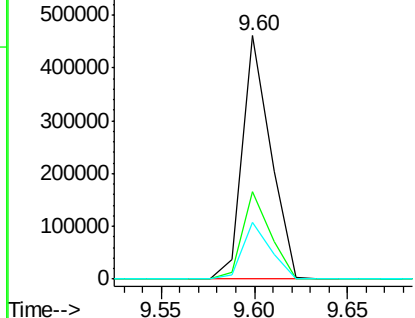




#63
 Phenanthrene-d10
 Concen: 20.00 ng
 RT: 12.22 min Scan# 965
 Delta R.T. 0.00 min
 Lab File: BF078612.D
 Acq: 17 Apr 2015 18:29




Instrument :
 BNA_F
 ClientSampleId :
 MW-47


Tgt Ion:188 Resp: 186950
 Ion Ratio Lower Upper
 188 100
 94 10.2 9.0 13.4
 80 11.4 9.5 14.3

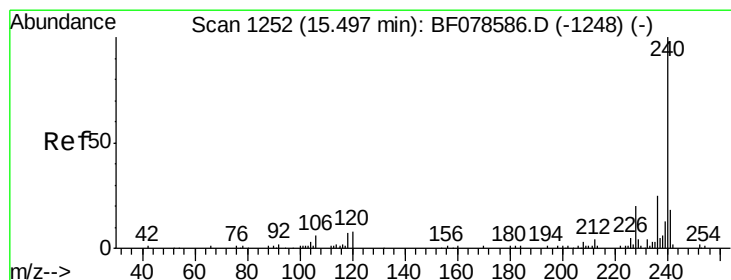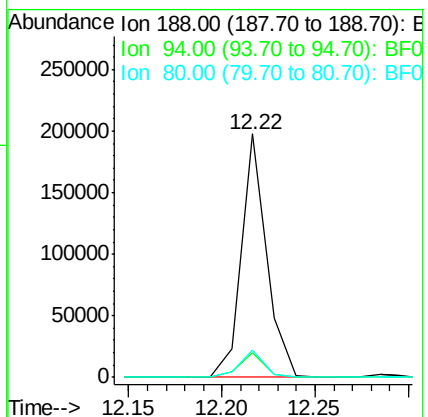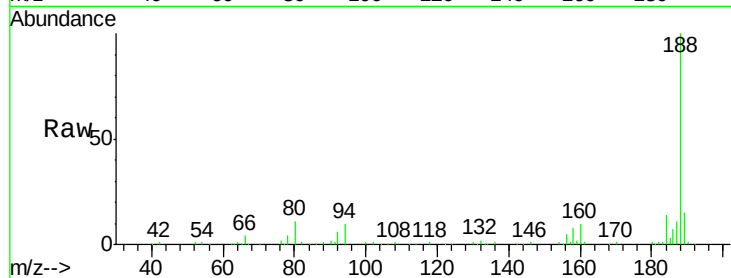

#75
 Chrysene-d12
 Concen: 20.00 ng
 RT: 15.46 min Scan# 1249
 Delta R.T. 0.00 min
 Lab File: BF078612.D
 Acq: 17 Apr 2015 18:29

Tgt Ion:240 Resp: 222785
 Ion Ratio Lower Upper
 240 100
 120 9.9 7.1 10.7
 236 25.5 21.4 32.2

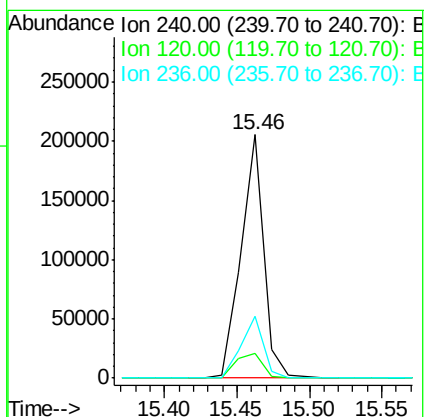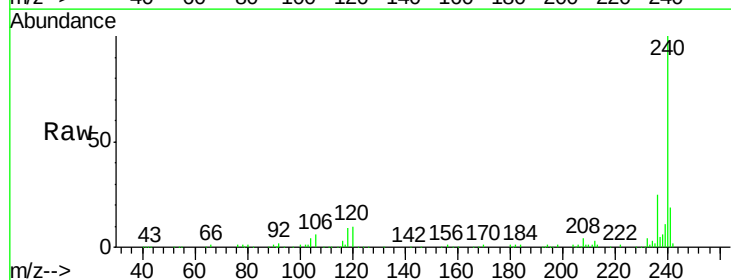



#78

Terphenyl-d14

Concen: 64.24 ng

RT: 14.21 min Scan# 1139

Delta R.T. 0.00 min

Lab File: BF078612.D

Acq: 17 Apr 2015 18:29

Instrument :

BNA_F

ClientSampleId :

MW-47


Tgt Ion:244 Resp: 633377

Ion Ratio Lower Upper

244 100

212 7.1 5.0 7.4




122 13.5 7.1 10.7#

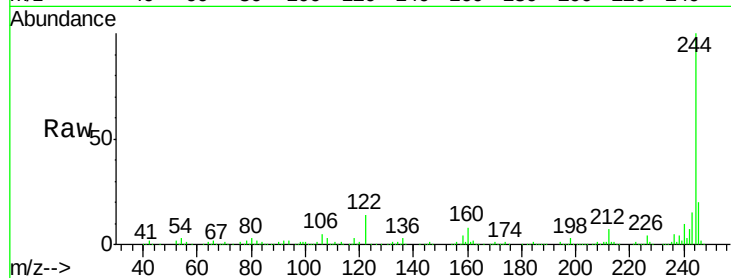

Abundance Ion 244.00 (243.70 to 244.70): E

Ion 212.00 (211.70 to 212.70): E

Ion 122.00 (121.70 to 122.70): E

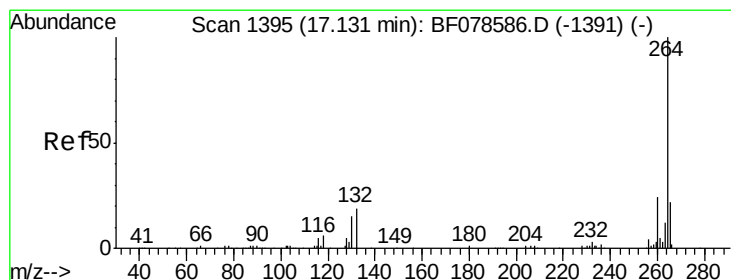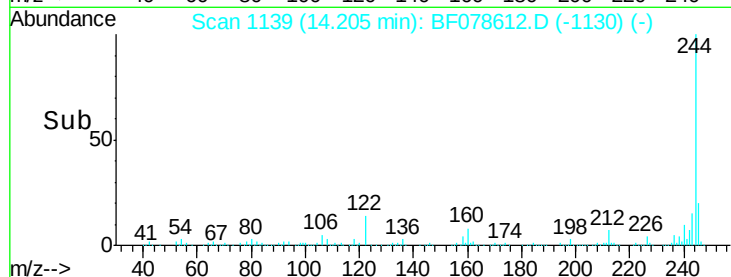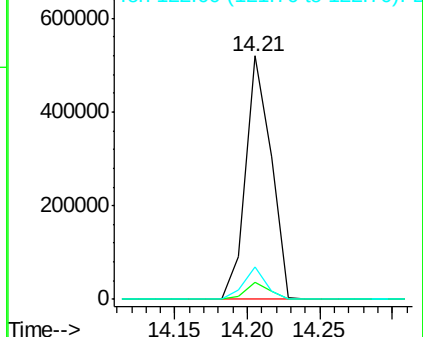

#86

Perylene-d12

Concen: 20.00 ng

RT: 17.14 min Scan# 1396

Delta R.T. -0.01 min

Lab File: BF078612.D

Acq: 17 Apr 2015 18:29


Tgt Ion:264 Resp: 220179

Ion Ratio Lower Upper

264 100

260 23.4 18.6 27.8

265 21.6 17.0 25.6

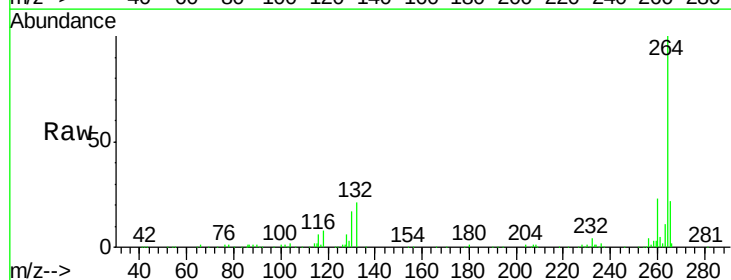

Abundance Ion 264.00 (263.70 to 264.70): E

Ion 260.00 (259.70 to 260.70): E

Ion 265.00 (264.70 to 265.70): E

