

Data Path : Z:\HPCHEM1\BNA_F\DATA\BF041715\
 Data File : BF078625.D
 Acq On : 18 Apr 2015 5:41
 Operator : TP/IZ
 Sample : G1872-06
 Misc :
 ALS Vial : 22 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 MW-23

Quant Time: Apr 18 07:13:47 2015
 Quant Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF040115.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Sat Apr 18 05:24:48 2015
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	6.67	152	37283	20.00	ng	0.00
21) Naphthalene-d8	8.25	136	156303	20.00	ng	0.00
38) Acenaphthene-d10	10.40	164	83611	20.00	ng	0.00
63) Phenanthrene-d10	12.22	188	171015	20.00	ng	0.00
75) Chrysene-d12	15.46	240	203951	20.00	ng	0.00
86) Perylene-d12	17.11	264	197501	20.00	ng	0.01
System Monitoring Compounds						
5) 2-Fluorophenol	4.90	112	122153	54.02	ng	0.01
7) Phenol-d6	6.28	99	103297	36.45	ng	0.00
23) Nitrobenzene-d5	7.38	82	205801	79.81	ng	0.00
41) 2,4,6-Tribromophenol	11.38	330	92284	133.08	ng	0.00
44) 2-Fluorobiphenyl	9.60	172	425223	72.70	ng	0.00
78) Terphenyl-d14	14.21	244	569684	63.12	ng	0.00


Target Compounds	Qvalue
------------------	--------


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\HPCHEM1\BNA_F\DATA\BF041715\
Data File : BF078625.D
Acq On : 18 Apr 2015 5:41
Operator : TP/IZ
Sample : G1872-06
Misc :
ALS Vial : 22 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
MW-23

Quant Time: Apr 18 07:13:47 2015
Quant Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF040115.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Sat Apr 18 05:24:48 2015
Response via : Initial Calibration

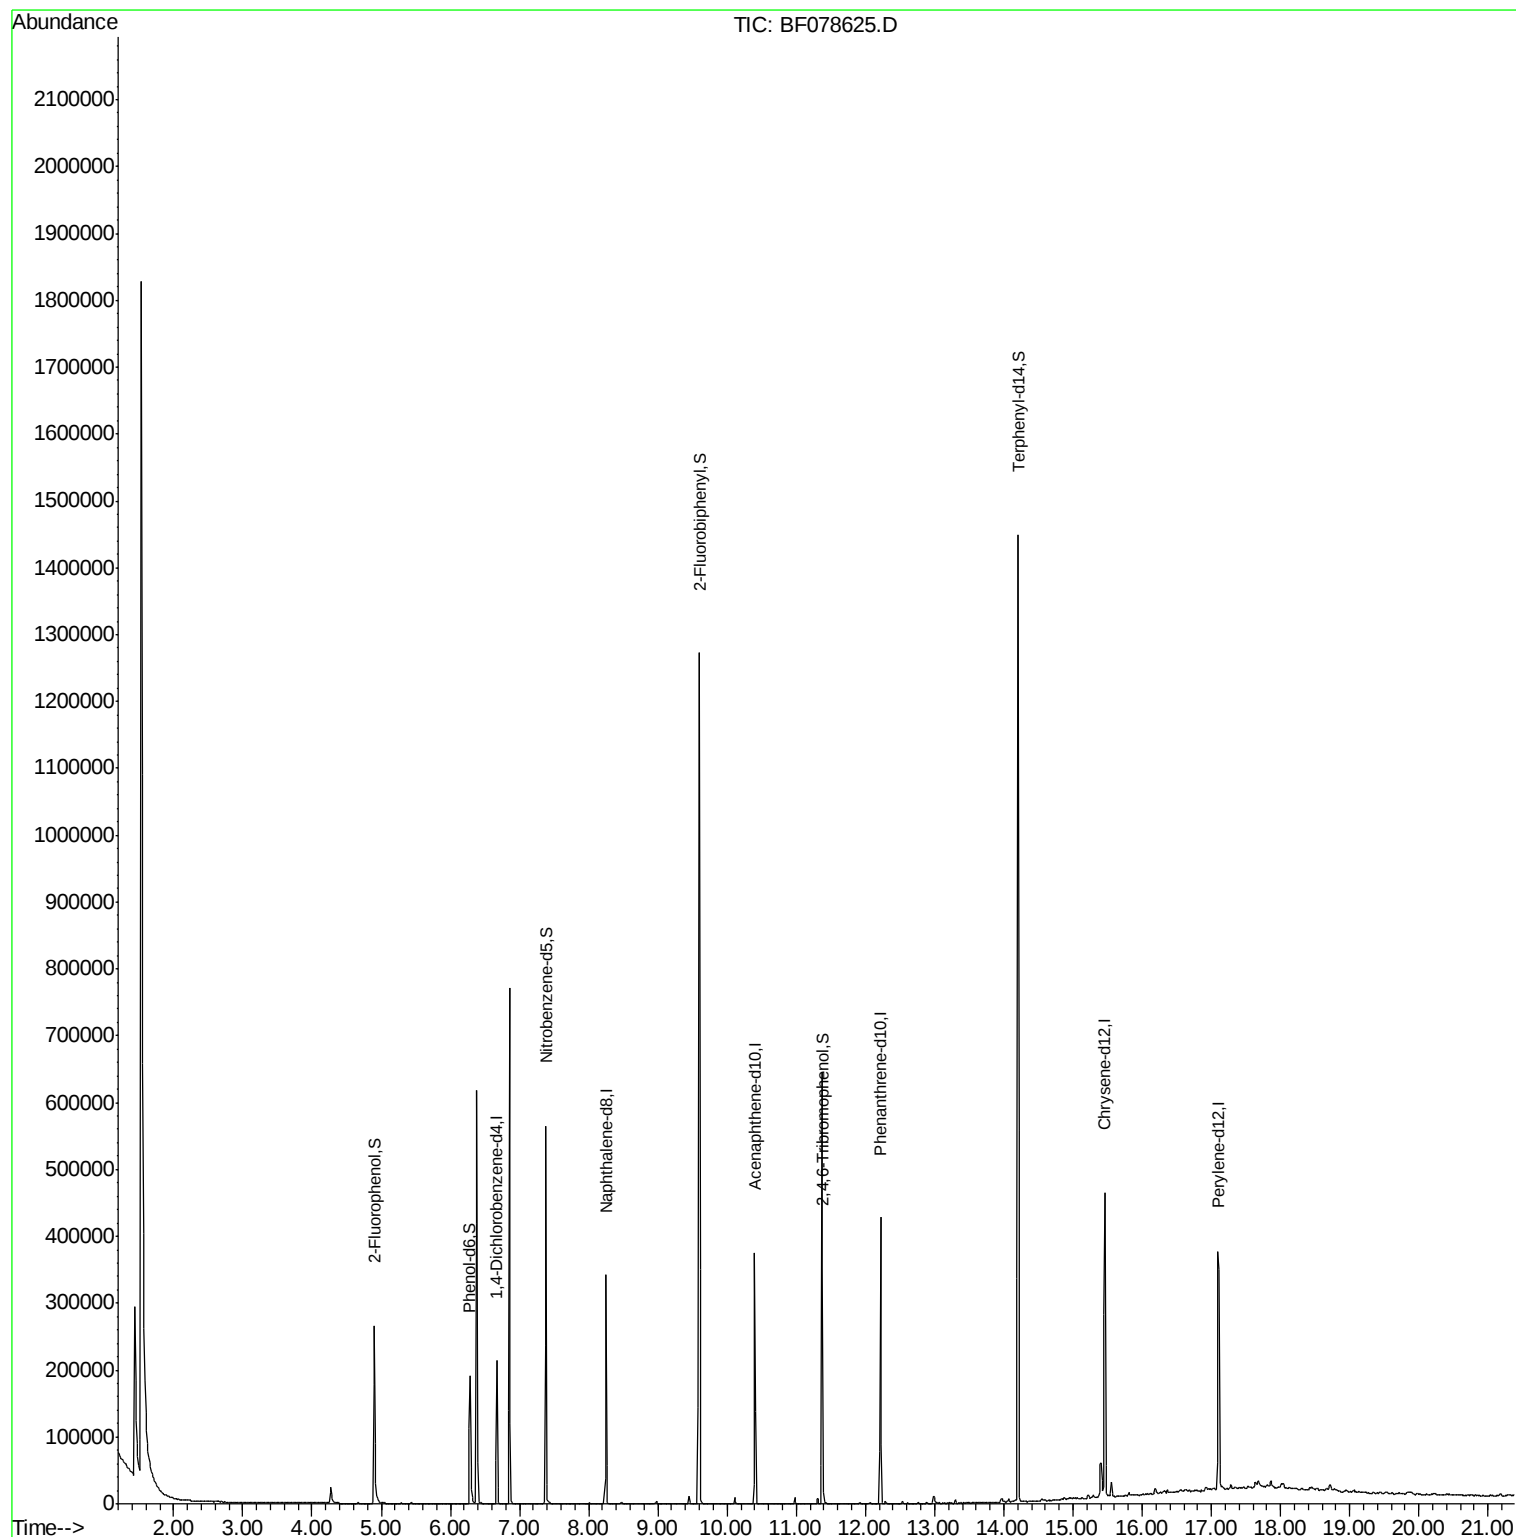



#1

1,4-Dichlorobenzene-d4

Concen: 20.00 ng

RT: 6.67 min Scan# 480

Delta R.T. 0.00 min

Lab File: BF078625.D

Acq: 18 Apr 2015 5:41

Instrument :

BNA_F

ClientSampleId :

MW-23


Tgt Ion:152 Resp: 37283

Ion Ratio Lower Upper

152 100

150 155.3 125.9 188.9




115 57.6 52.7 79.1



Abundance Ion 152.00 (151.70 to 152.70): E

Ion 150.00 (149.70 to 150.70): E

Ion 115.00 (114.70 to 115.70): E

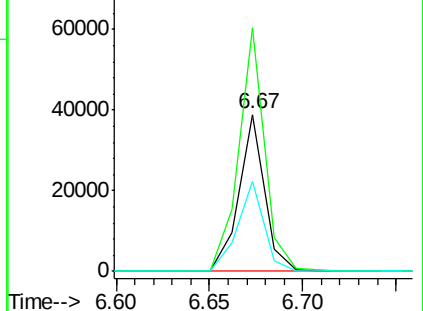

#5

2-Fluorophenol

Concen: 54.02 ng

RT: 4.90 min Scan# 325

Delta R.T. 0.01 min

Lab File: BF078625.D

Acq: 18 Apr 2015 5:41


Tgt Ion:112 Resp: 122153

Ion Ratio Lower Upper

112 100

64 53.6 39.9 59.9



63 27.1 20.2 30.4



Abundance Ion 112.00 (111.70 to 112.70): E

Ion 64.00 (63.70 to 64.70): BF0

Ion 63.00 (62.70 to 63.70): BF0

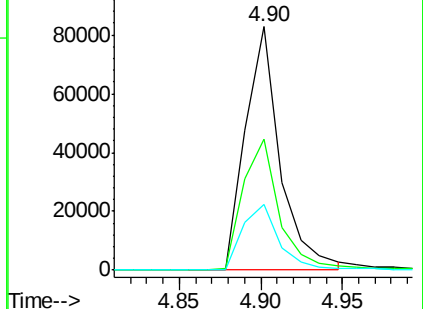



#7

Phenol-d6

Concen: 36.45 ng

RT: 6.28 min Scan# 446

Delta R.T. 0.00 min

Lab File: BF078625.D

Acq: 18 Apr 2015 5:41

Instrument :

BNA_F

ClientSampled :

MW-23


Tgt Ion: 99 Resp: 103297

Ion Ratio Lower Upper

99 100

42 14.8 14.8 22.2#



71 29.4 26.6 39.8

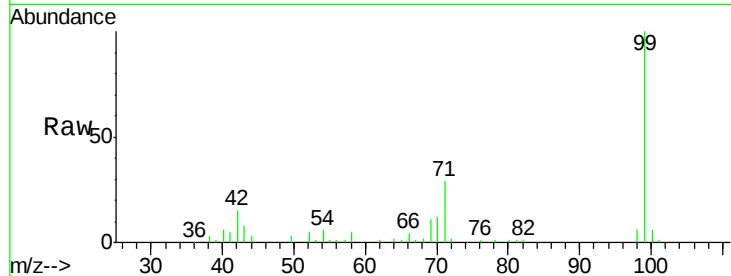

Abundance Ion 99.00 (98.70 to 99.70): BF0

Ion 42.00 (41.70 to 42.70): BF0

Ion 71.00 (70.70 to 71.70): BF0

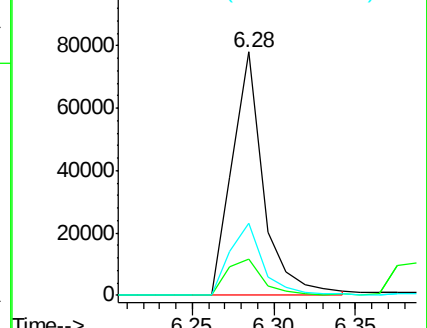

#21

Naphthalene-d8

Concen: 20.00 ng

RT: 8.25 min Scan# 618

Delta R.T. 0.00 min

Lab File: BF078625.D

Acq: 18 Apr 2015 5:41

Tgt Ion: 136 Resp: 156303


Ion Ratio Lower Upper

136 100

137 11.2 9.0 13.4

54 7.3 7.0 10.6

68 5.7 5.4 8.2






Abundance Ion 136.00 (135.70 to 136.70): E

Ion 137.00 (136.70 to 137.70): E

Ion 54.00 (53.70 to 54.70): BF0

Ion 68.00 (67.70 to 68.70): BF0



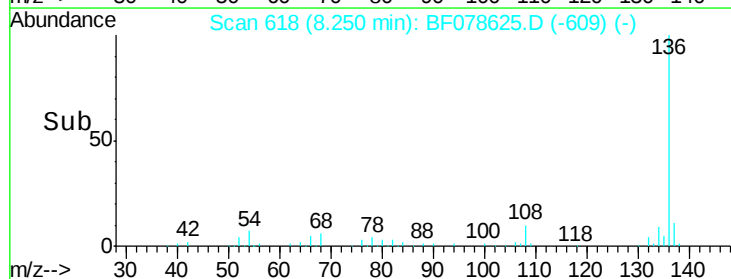
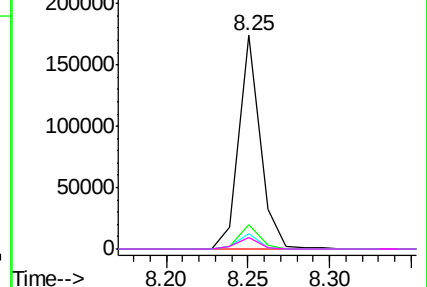


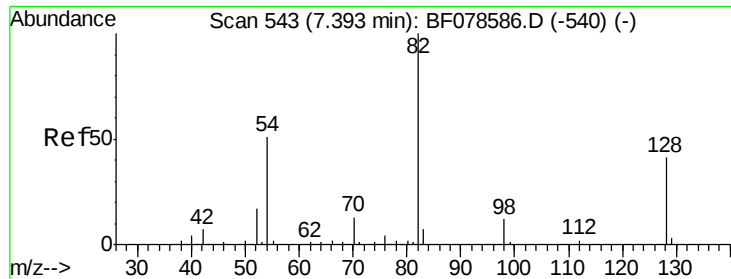

#23
 Nitrobenzene-d5
 Concen: 79.81 ng
 RT: 7.38 min Scan# 542
 Delta R.T. 0.00 min
 Lab File: BF078625.D
 Acq: 18 Apr 2015 5:41




Instrument :
 BNA_F
 ClientSampleId :
 MW-23

Tgt Ion	Ratio	Lower	Upper
82	100		
128	48.1	31.8	47.8#
54	45.5	41.5	62.3

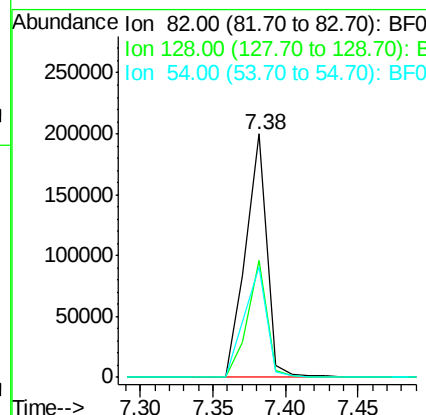

#38
 Acenaphthene-d10
 Concen: 20.00 ng
 RT: 10.40 min Scan# 806
 Delta R.T. 0.00 min
 Lab File: BF078625.D
 Acq: 18 Apr 2015 5:41

Tgt Ion	Ratio	Lower	Upper
164	100		
162	101.5	82.2	123.2
160	44.6	34.7	52.1

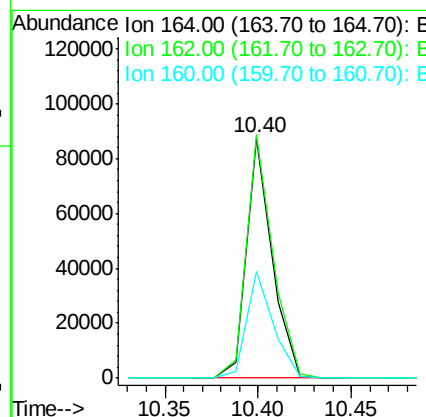







#41
 2,4,6-Tribromophenol
 Concen: 133.08 ng
 RT: 11.38 min Scan# 892
 Delta R.T. 0.00 min
 Lab File: BF078625.D
 Acq: 18 Apr 2015 5:41

Instrument :
 BNA_F
 ClientSampleId :
 MW-23

Tgt Ion:330 Resp: 92284
 Ion Ratio Lower Upper
 330 100
 332 98.1 78.6 117.8
 141 37.0 31.2 46.8




Abundance Ion 329.80 (329.50 to 330.50): E
 Ion 331.80 (331.50 to 332.50): E
 Ion 141.00 (140.70 to 141.70): E


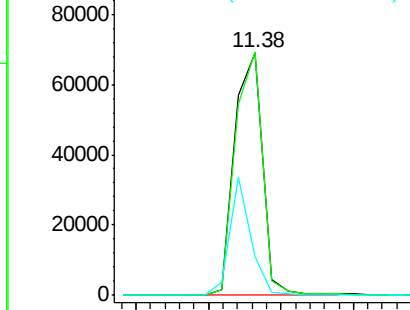



#44
 2-Fluorobiphenyl
 Concen: 72.70 ng
 RT: 9.60 min Scan# 736
 Delta R.T. 0.00 min
 Lab File: BF078625.D
 Acq: 18 Apr 2015 5:41

Tgt Ion:172 Resp: 425223
 Ion Ratio Lower Upper
 172 100
 171 35.0 28.6 42.8
 170 23.5 18.5 27.7



Abundance Ion 172.00 (171.70 to 172.70): E
 Ion 171.00 (170.70 to 171.70): E
 Ion 170.00 (169.70 to 170.70): E




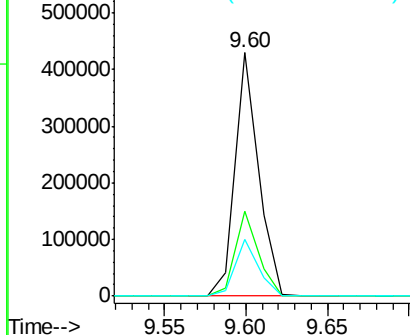


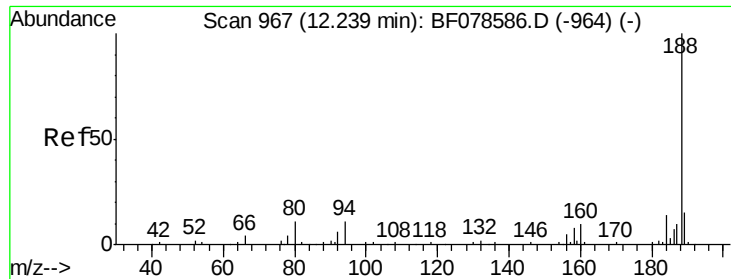

#63
 Phenanthrene-d10
 Concen: 20.00 ng
 RT: 12.22 min Scan# 965
 Delta R.T. 0.00 min
 Lab File: BF078625.D
 Acq: 18 Apr 2015 5:41




Instrument :
 BNA_F
 ClientSampleId :
 MW-23


Tgt Ion	Ratio	Lower	Upper
188	100		
94	9.4	9.0	13.4
80	10.1	9.5	14.3

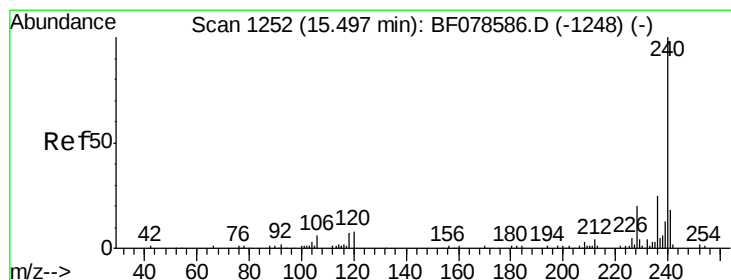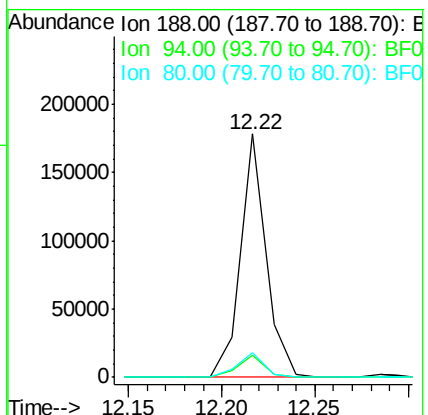

#75
 Chrysene-d12
 Concen: 20.00 ng
 RT: 15.46 min Scan# 1249
 Delta R.T. 0.00 min
 Lab File: BF078625.D
 Acq: 18 Apr 2015 5:41

Tgt Ion	Ratio	Lower	Upper
240	100		
120	9.2	7.1	10.7
236	25.6	21.4	32.2


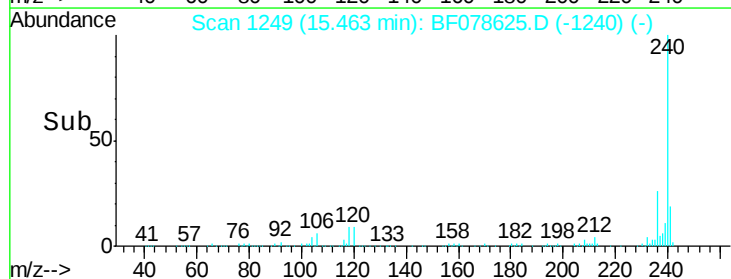
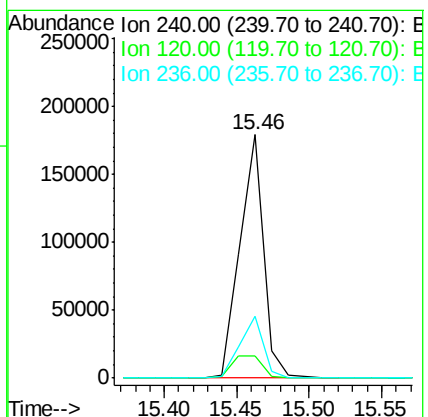
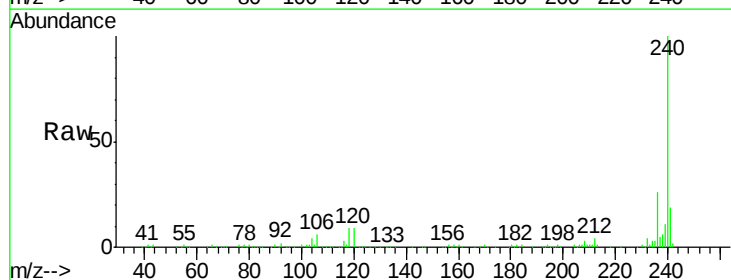


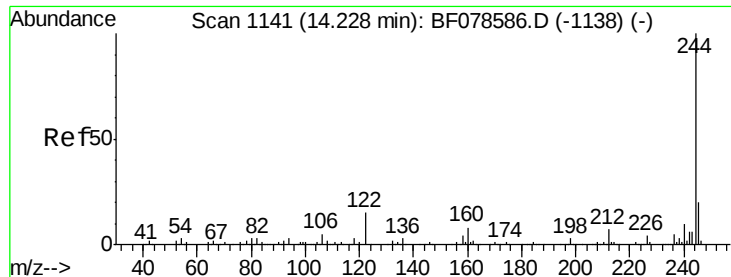

#78
 Terphenyl-d14
 Concen: 63.12 ng
 RT: 14.21 min Scan# 1139
 Delta R.T. 0.00 min
 Lab File: BF078625.D
 Acq: 18 Apr 2015 5:41

Instrument :
 BNA_F
 ClientSampleId :
 MW-23

Tgt Ion: 244 Resp: 569684
 Ion Ratio Lower Upper
 244 100
 212 7.1 5.0 7.4
 122 13.2 7.1 10.7#

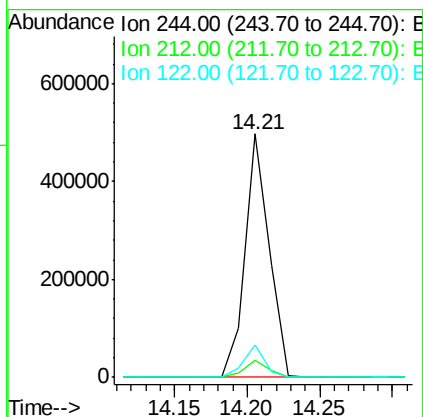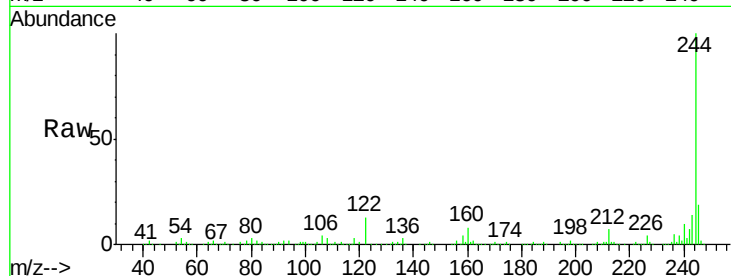

#86
 Perylene-d12
 Concen: 20.00 ng
 RT: 17.11 min Scan# 1393
 Delta R.T. 0.01 min
 Lab File: BF078625.D
 Acq: 18 Apr 2015 5:41

Tgt Ion: 264 Resp: 197501
 Ion Ratio Lower Upper
 264 100
 260 23.2 18.6 27.8
 265 21.1 17.0 25.6

