
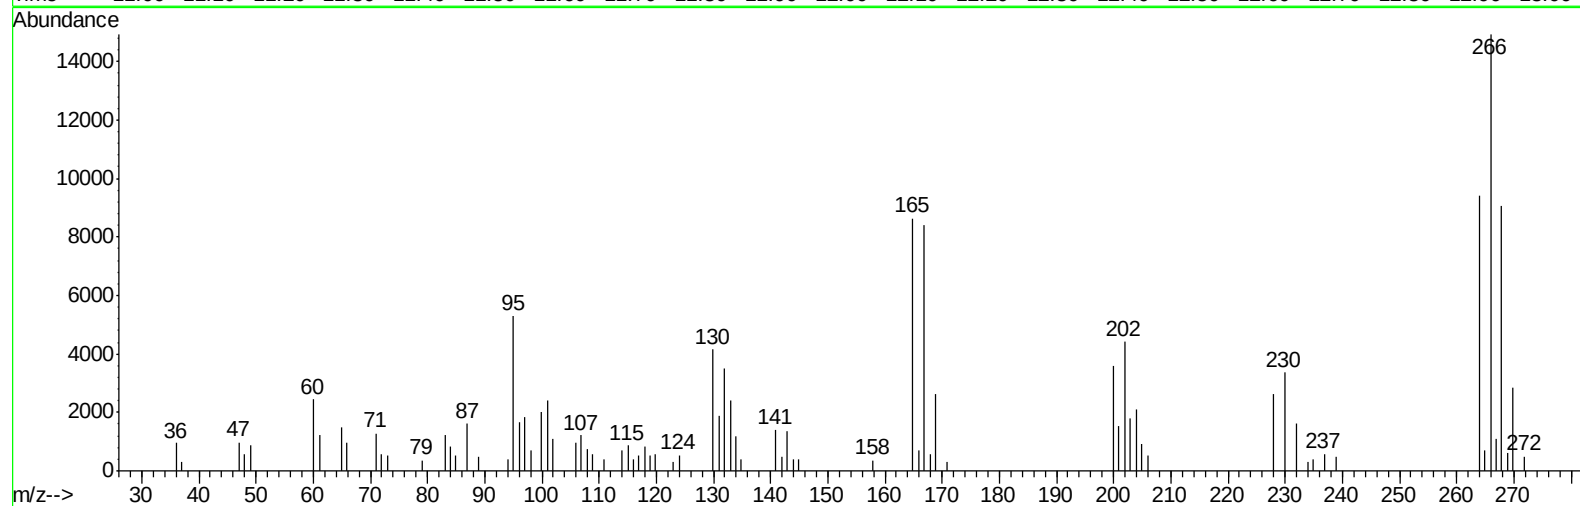


Data Path : Z:\HPCHEM1\BNA_F\DATA\BF041715\
Data File : BF078601.D
Acq On : 17 Apr 2015 12:11
Operator : TP/IZ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Apr 20 06:55:40 2015
Quant Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF040115.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Sat Apr 18 05:04:14 2015
Response via : Initial Calibration

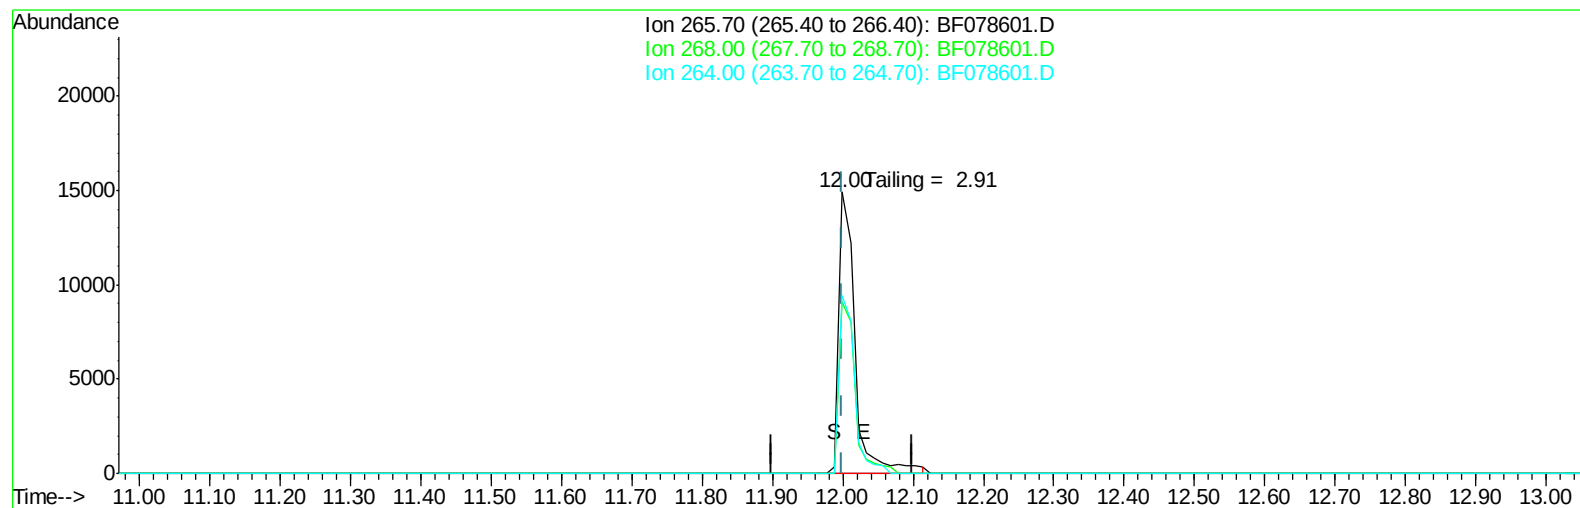

TIC: BF078601.D

(69) Pentachlorophenol (C)


11.999min (+0.000) 0.00ng

response 22122

Ion	Exp%	Act%
265.70	100	100
268.00	62.60	60.72
264.00	62.50	63.17
0.00	0.00	0.00

Data Path : Z:\HPCHEM1\BNA_F\DATA\BF041715\
Data File : BF078601.D
Acq On : 17 Apr 2015 12:11
Operator : TP/IZ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Apr 20 06:55:40 2015
Quant Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF040115.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Sat Apr 18 05:04:14 2015
Response via : Initial Calibration

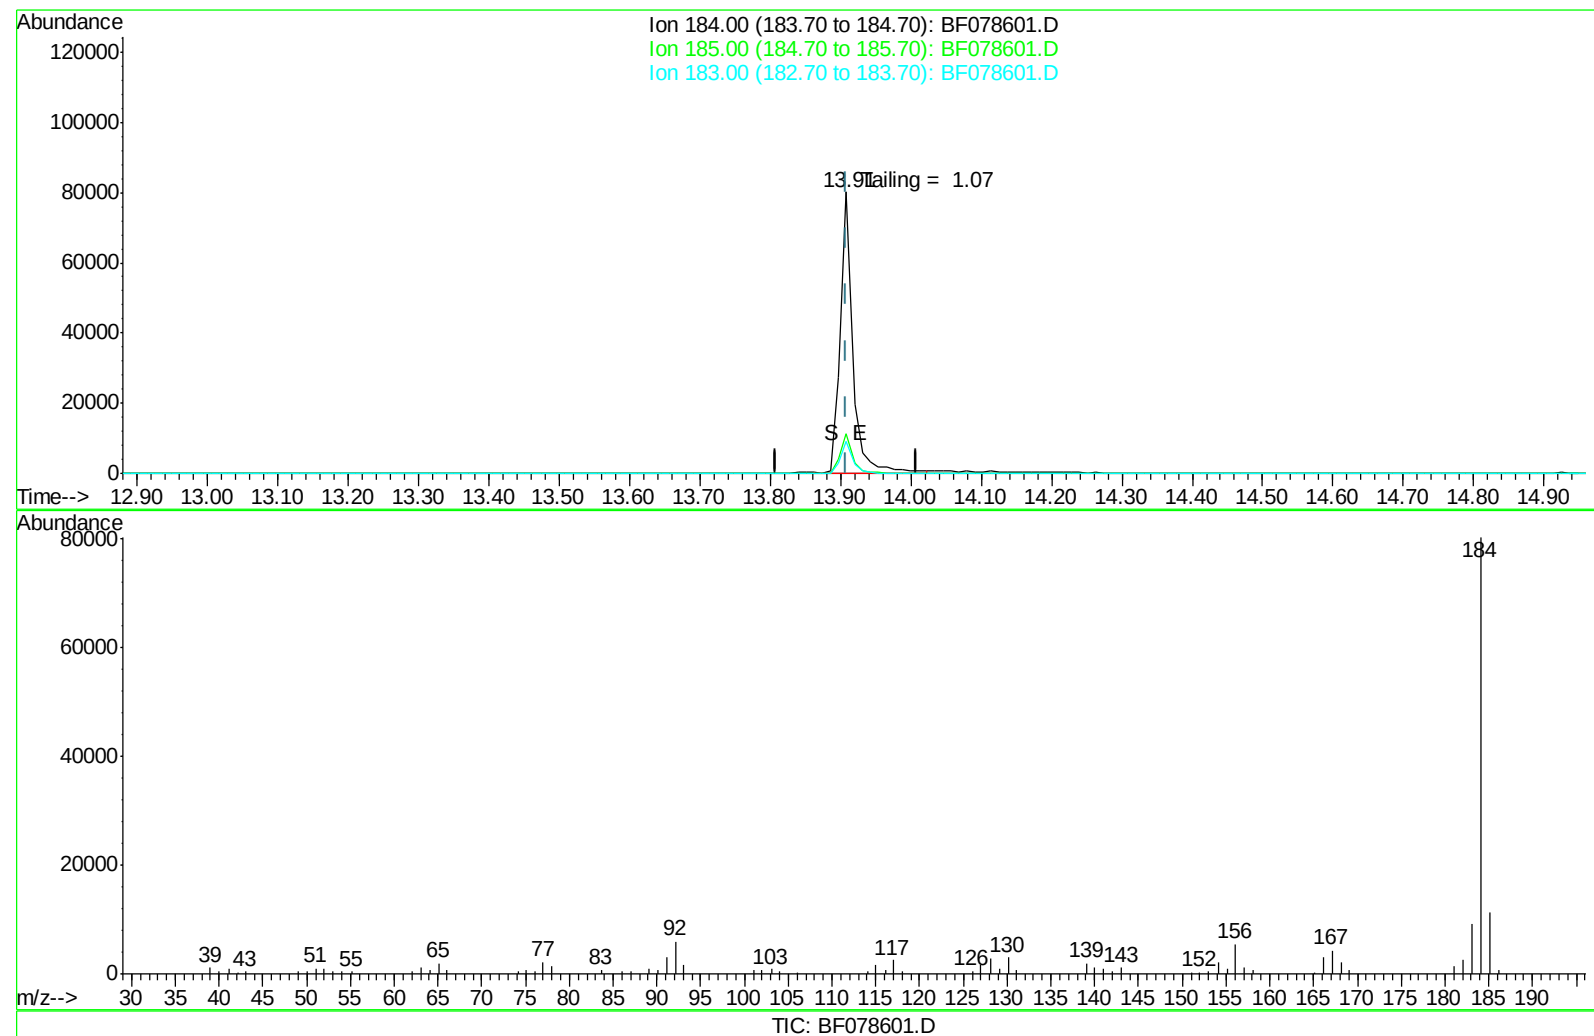

(76) Benzidine

13.908min (+0.000) 0.00ng

response 96303

Ion	Exp%	Act%
184.00	100	100
185.00	15.20	14.18
183.00	11.90	11.36
0.00	0.00	0.00