

Data Path : Z:\HPCHEM1\BNA F\DATA\BF041715\
 Data File : BF078616.D
 Acq On : 17 Apr 2015 21:04
 Operator : TP/IZ
 Sample : G1871-07
 Misc :
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 MW-29

Quant Time: Apr 17 23:45:41 2015
 Quant Method : Z:\HPCHEM1\BNA F\METHODS\8270-BF040115.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Apr 17 23:28:12 2015
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	6.67	152	44164	20.00	ng	0.00
21) Naphthalene-d8	8.25	136	184127	20.00	ng	0.00
38) Acenaphthene-d10	10.40	164	94293	20.00	ng	-0.01
63) Phenanthrene-d10	12.22	188	195039	20.00	ng	0.00
75) Chrysene-d12	15.46	240	226678	20.00	ng	0.00
86) Perylene-d12	17.21	264	223435	20.00	ng	0.06
System Monitoring Compounds						
5) 2-Fluorophenol	4.90	112	117722	43.95	ng	0.00
7) Phenol-d6	6.28	99	91747	27.33	ng	0.00
23) Nitrobenzene-d5	7.38	82	225497	74.23	ng	0.00
41) 2,4,6-Tribromophenol	11.38	330	108885	139.23	ng	0.00
44) 2-Fluorobiphenyl	9.60	172	474125	71.87	ng	0.00
78) Terphenyl-d14	14.21	244	634165	63.22	ng	0.00


Target Compounds Qvalue


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\HPCHEM1\BNA F\DATA\BF041715\
Data File : BF078616.D
Acq On : 17 Apr 2015 21:04
Operator : TP/IZ
Sample : G1871-07
Misc :
ALS Vial : 16 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
MW-29

Quant Time: Apr 17 23:45:41 2015
Quant Method : Z:\HPCHEM1\BNA F\METHODS\8270-BF040115.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Apr 17 23:28:12 2015
Response via : Initial Calibration

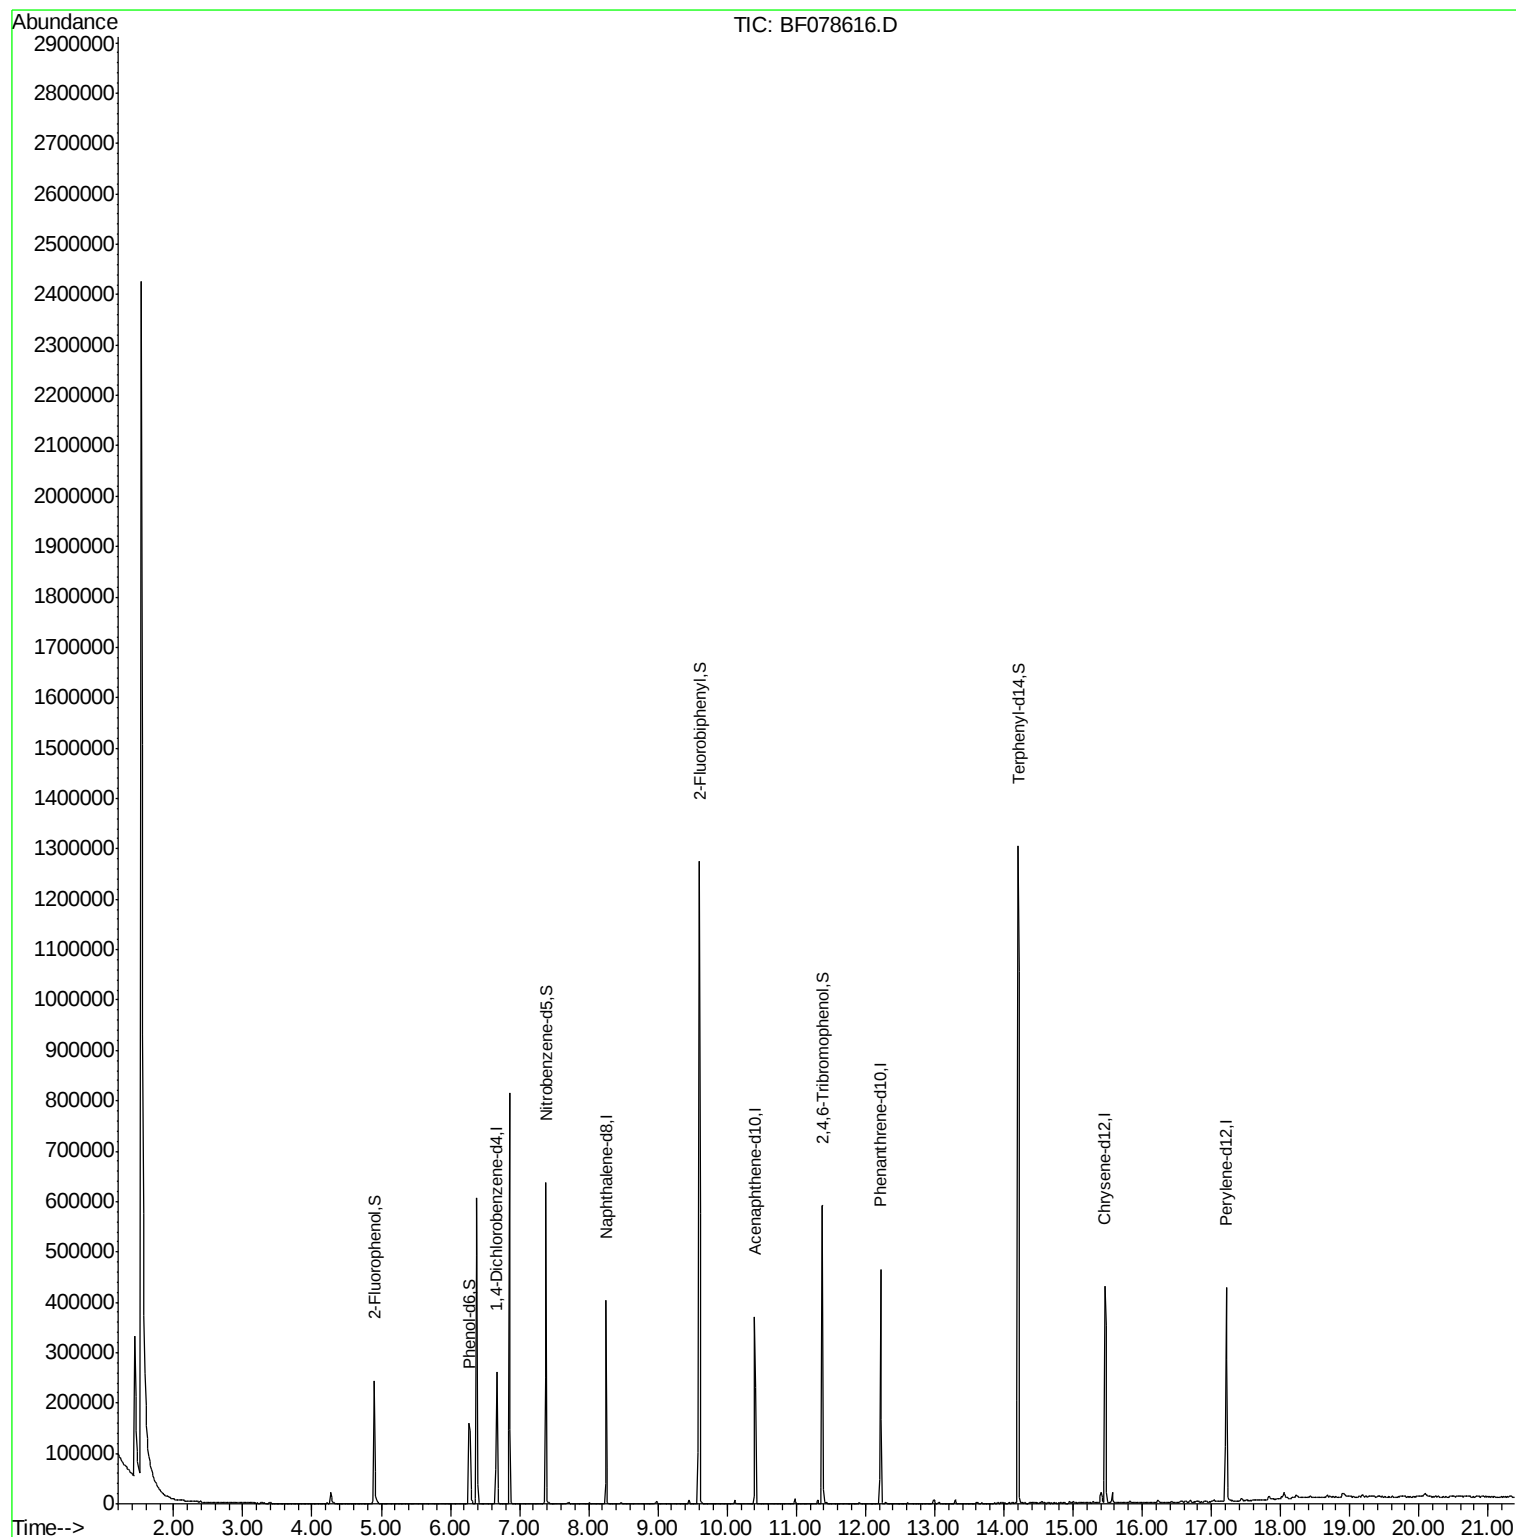

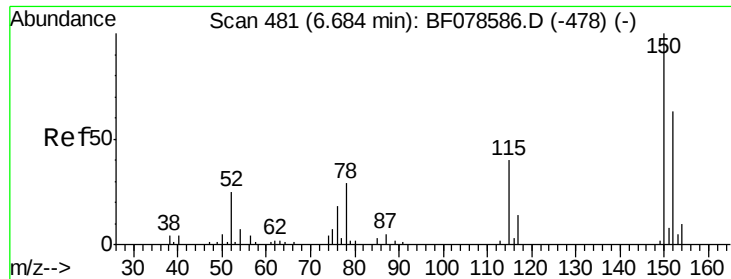

#1

1,4-Dichlorobenzene-d4

Concen: 20.00 ng

RT: 6.67 min Scan# 480

Delta R.T. 0.00 min

Lab File: BF078616.D

Acq: 17 Apr 2015 21:04

Instrument :

BNA_F

ClientSampleId :

MW-29


Tot Ion:152 Resp: 44164

Ion Ratio Lower Upper

152 100

150 156.6 125.9 188.9




115 57.8 52.7 79.1

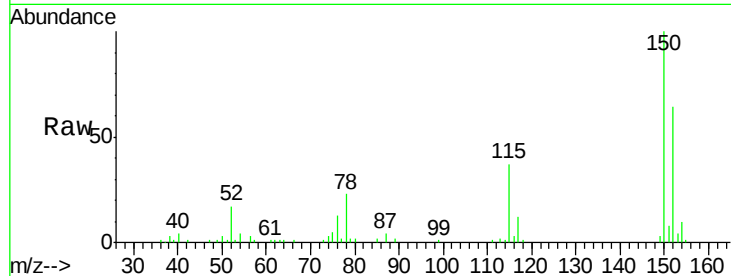

Abundance Ion 152.00 (151.70 to 152.70): E

Ion 150.00 (149.70 to 150.70): E

Ion 115.00 (114.70 to 115.70): E

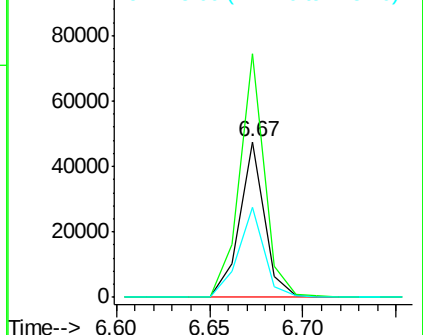

#5

2-Fluorophenol

Concen: 43.95 ng

RT: 4.90 min Scan# 325

Delta R.T. 0.00 min

Lab File: BF078616.D

Acq: 17 Apr 2015 21:04


Tgt Ion:112 Resp: 117722

Ion Ratio Lower Upper

112 100

64 51.0 39.9 59.9



63 25.5 20.2 30.4




Abundance Ion 112.00 (111.70 to 112.70): E

Ion 64.00 (63.70 to 64.70): BF0

Ion 63.00 (62.70 to 63.70): BF0

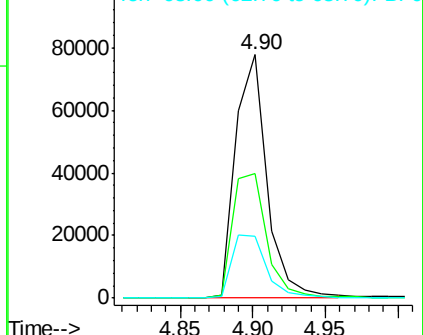

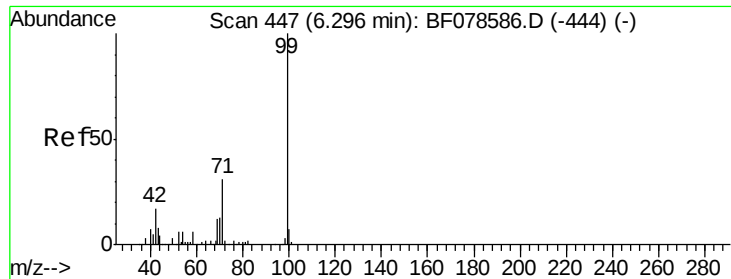

#7

Phenol-d6

Concen: 27.33 ng

RT: 6.28 min Scan# 446

Delta R.T. 0.00 min

Lab File: BF078616.D

Acq: 17 Apr 2015 21:04

Instrument :

BNA_F

ClientSampleId :

MW-29





Tot Ion: 99 Resp: 91747

Ion Ratio Lower Upper

99 100

42 14.5 14.8 22.2#

71 28.7 26.6 39.8

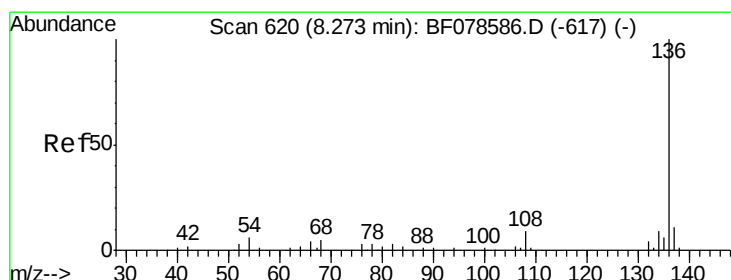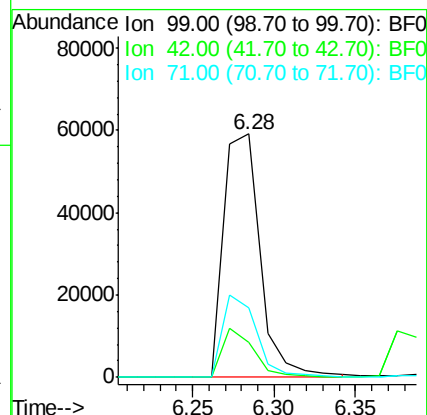

#21

Naphthalene-d8

Concen: 20.00 ng

RT: 8.25 min Scan# 618

Delta R.T. 0.00 min

Lab File: BF078616.D

Acq: 17 Apr 2015 21:04

Tgt Ion: 136 Resp: 184127




Ion Ratio Lower Upper


136 100

137 10.6 9.0 13.4

54 7.0 7.0 10.6#

68 5.8 5.4 8.2

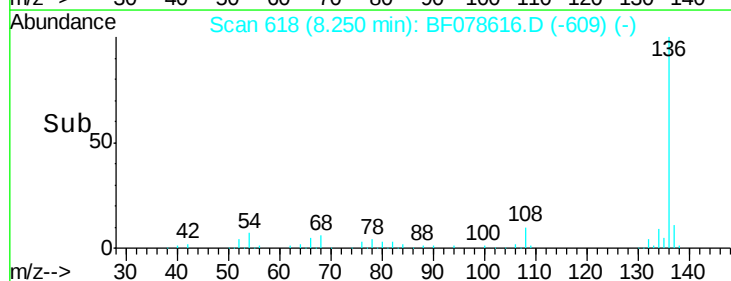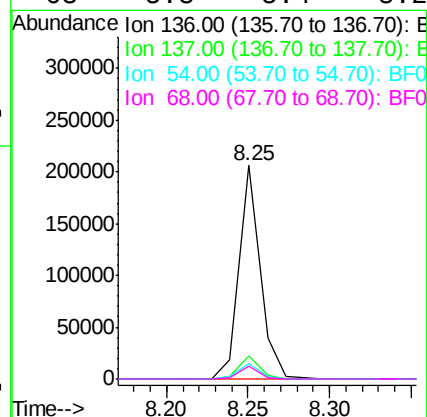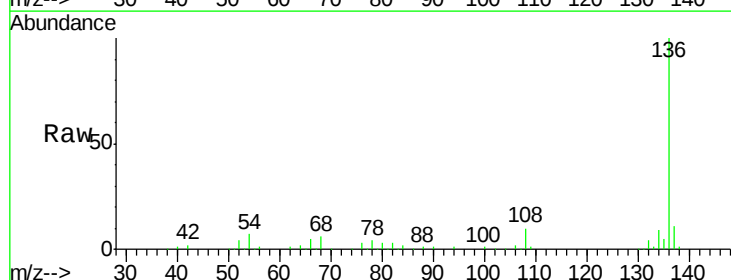







#23
Nitrobenzene-d5
Concen: 74.23 ng
RT: 7.38 min Scan# 542
Delta R.T. 0.00 min
Lab File: BF078616.D
Acq: 17 Apr 2015 21:04

Instrument :
BNA_F
ClientSampleId :
MW-29

Tot Ion: 82 Resp: 225497
Ion Ratio Lower Upper
82 100
128 48.3 31.8 47.8#
54 46.6 41.5 62.3

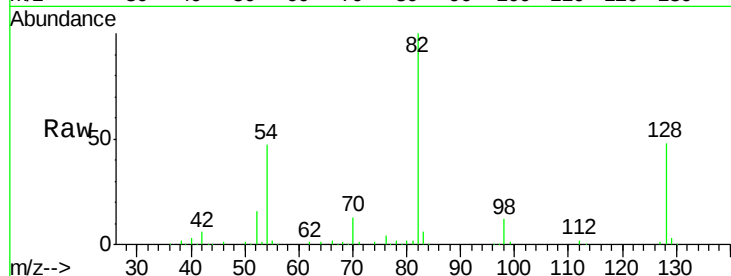


Abundance Ion 82.00 (81.70 to 82.70): BF0
Ion 128.00 (127.70 to 128.70): B
Ion 54.00 (53.70 to 54.70): BF0


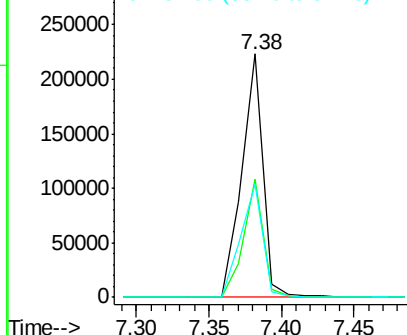


#38
Acenaphthene-d10
Concen: 20.00 ng
RT: 10.40 min Scan# 806
Delta R.T. -0.01 min
Lab File: BF078616.D
Acq: 17 Apr 2015 21:04

Tgt Ion:164 Resp: 94293
Ion Ratio Lower Upper
164 100
162 104.3 82.2 123.2
160 44.3 34.7 52.1



Abundance Ion 164.00 (163.70 to 164.70): E
Ion 162.00 (161.70 to 162.70): E
Ion 160.00 (159.70 to 160.70): E

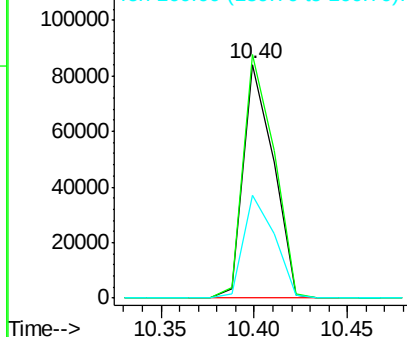







#41
 2,4,6-Tribromophenol
 Concen: 139.23 ng
 RT: 11.38 min Scan# 892
 Delta R.T. 0.00 min
 Lab File: BF078616.D
 Acq: 17 Apr 2015 21:04

Instrument :
 BNA_F
 ClientSampleId :
 MW-29

Tot Ion	Ratio	Lower	Upper
330	100		
332	96.2	78.6	117.8
141	35.5	31.2	46.8




Abundance Ion 329.80 (329.50 to 330.50): E
 Ion 331.80 (331.50 to 332.50): E
 Ion 141.00 (140.70 to 141.70): E


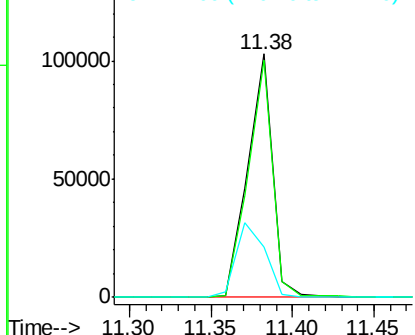



#44
 2-Fluorobiphenyl
 Concen: 71.87 ng
 RT: 9.60 min Scan# 736
 Delta R.T. 0.00 min
 Lab File: BF078616.D
 Acq: 17 Apr 2015 21:04

Tgt Ion	Ratio	Lower	Upper
172	100		
171	35.9	28.6	42.8
170	23.7	18.5	27.7



Abundance Ion 172.00 (171.70 to 172.70): E
 Ion 171.00 (170.70 to 171.70): E
 Ion 170.00 (169.70 to 170.70): E

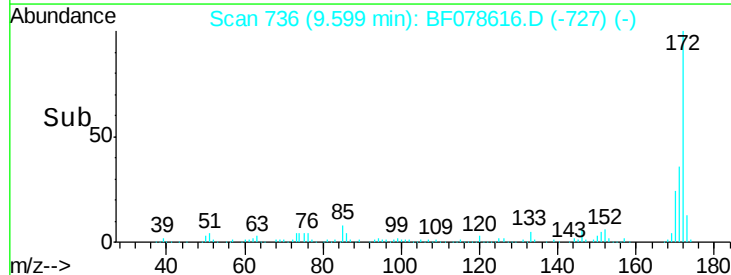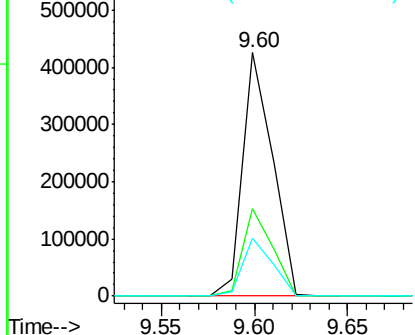


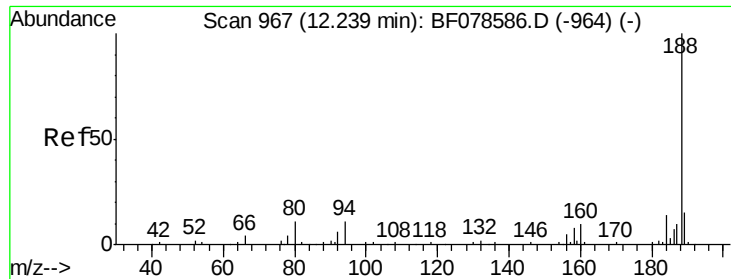




#63
Phenanthrene-d10
Concen: 20.00 ng
RT: 12.22 min Scan# 965
Delta R.T. 0.00 min
Lab File: BF078616.D
Acq: 17 Apr 2015 21:04

Instrument :
BNA_F
ClientSampleId :
MW-29

Tot Ion:188 Resp: 195039
Ion Ratio Lower Upper
188 100
94 10.7 9.0 13.4
80 11.5 9.5 14.3




Abundance Ion 188.00 (187.70 to 188.70): E
Ion 94.00 (93.70 to 94.70): BF0
Ion 80.00 (79.70 to 80.70): BF0


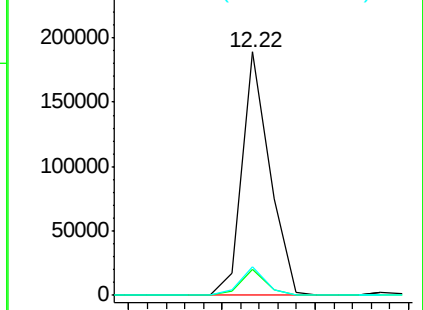


#75
Chrysene-d12
Concen: 20.00 ng
RT: 15.46 min Scan# 1249
Delta R.T. 0.00 min
Lab File: BF078616.D
Acq: 17 Apr 2015 21:04

Tgt Ion:240 Resp: 226678
Ion Ratio Lower Upper
240 100
120 14.1 7.1 10.7#
236 25.5 21.4 32.2



Abundance Ion 240.00 (239.70 to 240.70): E
Ion 120.00 (119.70 to 120.70): E
Ion 236.00 (235.70 to 236.70): E




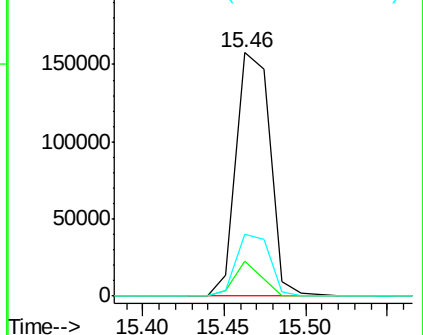




#78
 Terphenyl-d14
 Concen: 63.22 ng
 RT: 14.21 min Scan# 1139
 Delta R.T. 0.00 min
 Lab File: BF078616.D
 Acq: 17 Apr 2015 21:04

Instrument :
 BNA_F
 ClientSampleId :
 MW-29

Tot Ion:244 Resp: 634165
 Ion Ratio Lower Upper
 244 100
 212 7.0 5.0 7.4
 122 14.6 7.1 10.7#

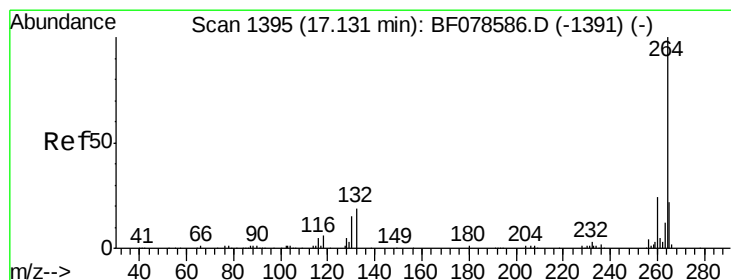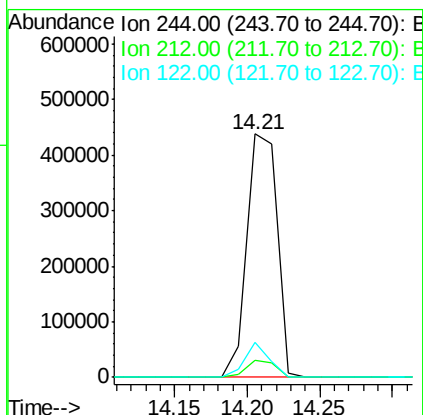

#86
 Perylene-d12
 Concen: 20.00 ng
 RT: 17.21 min Scan# 1402
 Delta R.T. 0.06 min
 Lab File: BF078616.D
 Acq: 17 Apr 2015 21:04

Tgt Ion:264 Resp: 223435
 Ion Ratio Lower Upper
 264 100
 260 23.0 18.6 27.8
 265 21.1 17.0 25.6

