
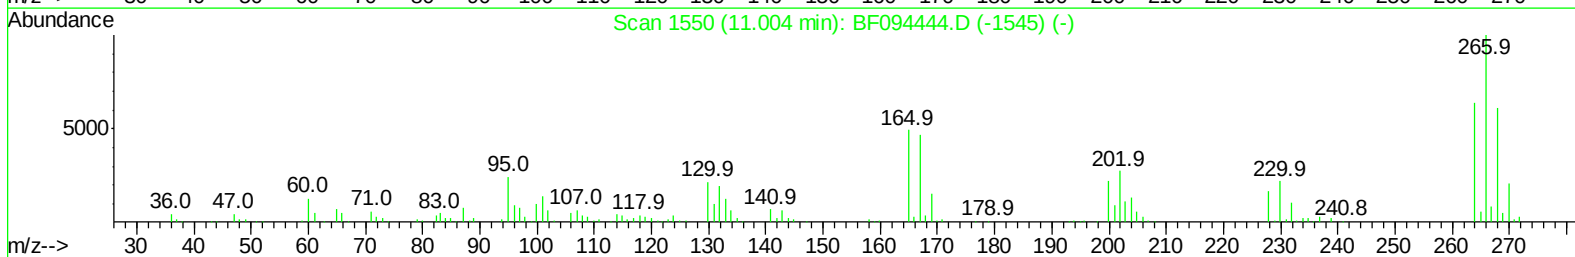
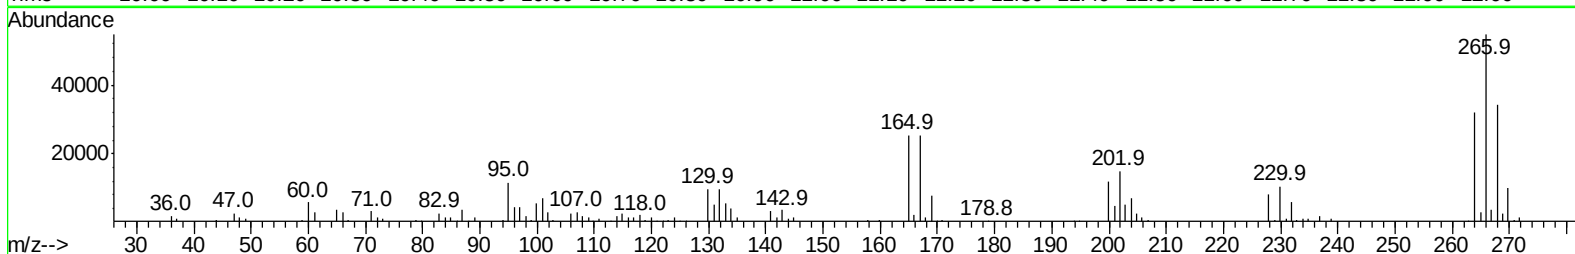


Data Path : Z:\HPCHEM1\BNA F\DATA\BF041717\
Data File : BF094440.D
Acq On : 17 Apr 2017 10:53
Operator : SJ/MA
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Apr 17 17:40:35 2017
Quant Method : Z:\HPCHEM1\BNA F\METHODS\8270-BF041717.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Apr 17 14:59:23 2017
Response via : Initial Calibration

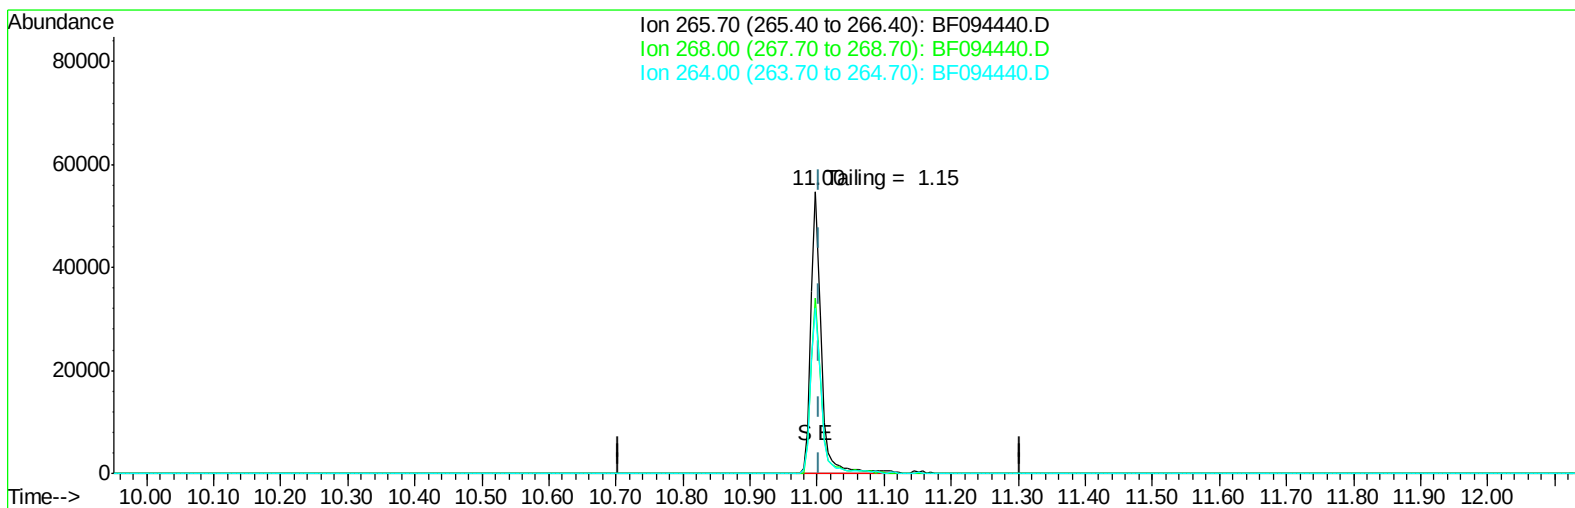

TIC: BF094440.D

(69) Pentachlorophenol (C)




10.998min (-0.006) 0.00ng

response 55986

Ion	Exp%	Act%
265.70	100	100
268.00	63.90	62.47
264.00	64.60	58.59
0.00	0.00	0.00

```
Data Path : Z:\HPCHEM1\BNA F\DATA\BF041717\  
Data File : BF094440.D  
Acq On    : 17 Apr 2017  10:53  
Operator  : SJ/MA  
Sample    : DFTPP  
Misc      :  
ALS Vial  : 1      Sample Multiplier: 1
```

Quant Time: Apr 17 17:40:35 2017
Quant Method : Z:\HPCHEM1\BNA F\METHODS\8270-BF041717.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Apr 17 14:59:23 2017
Response via : Initial Calibration

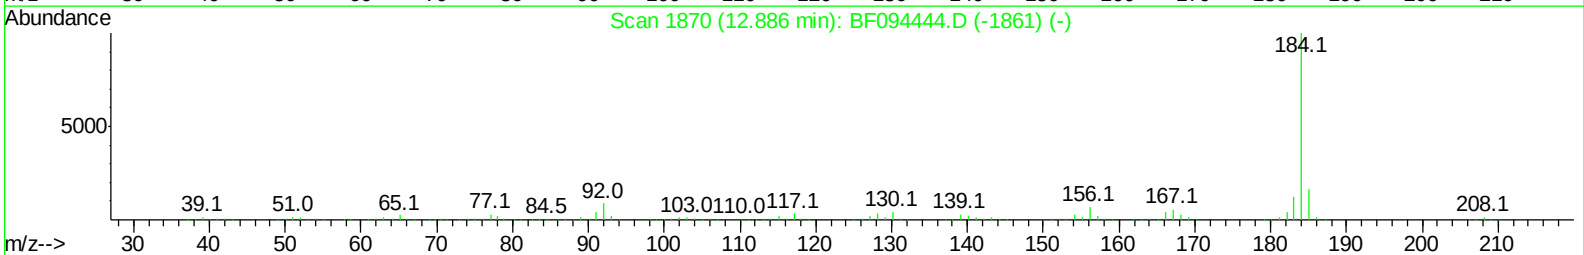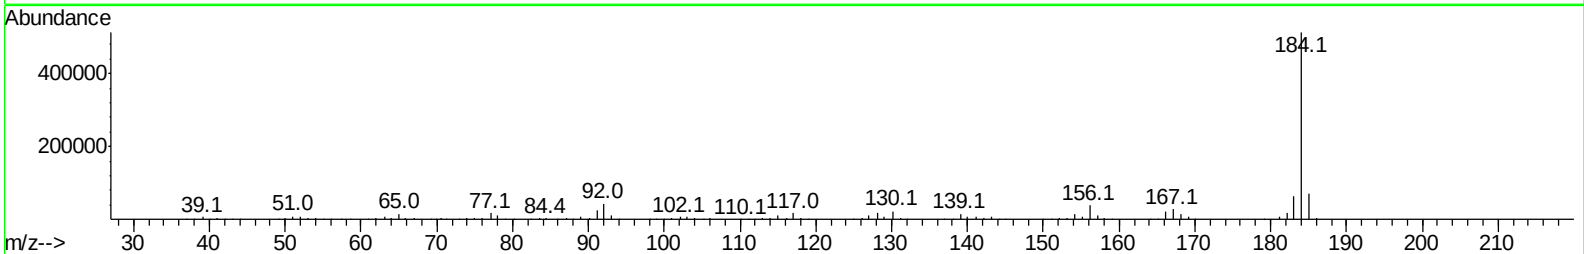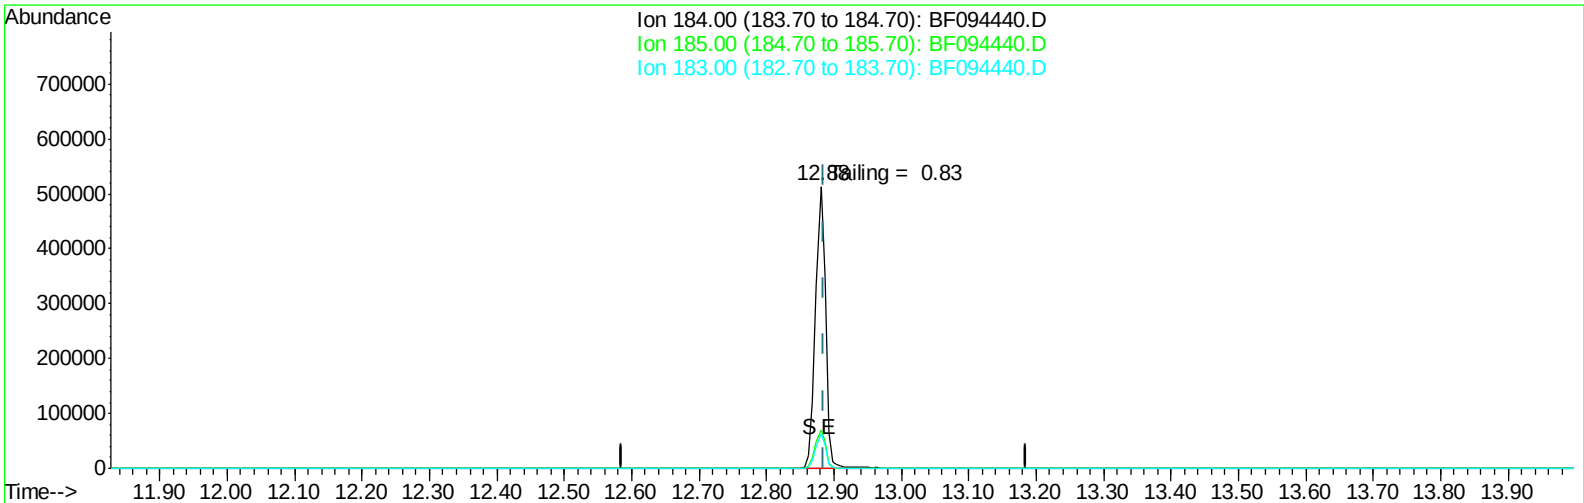

TIC: BF094440.D

(76) Benzidine

12.880min (-0.006) 0.00ng

response 512865

Ion	Exp%	Act%
184.00	100	100
185.00	19.40	13.76#
183.00	12.20	12.16
0.00	0.00	0.00