
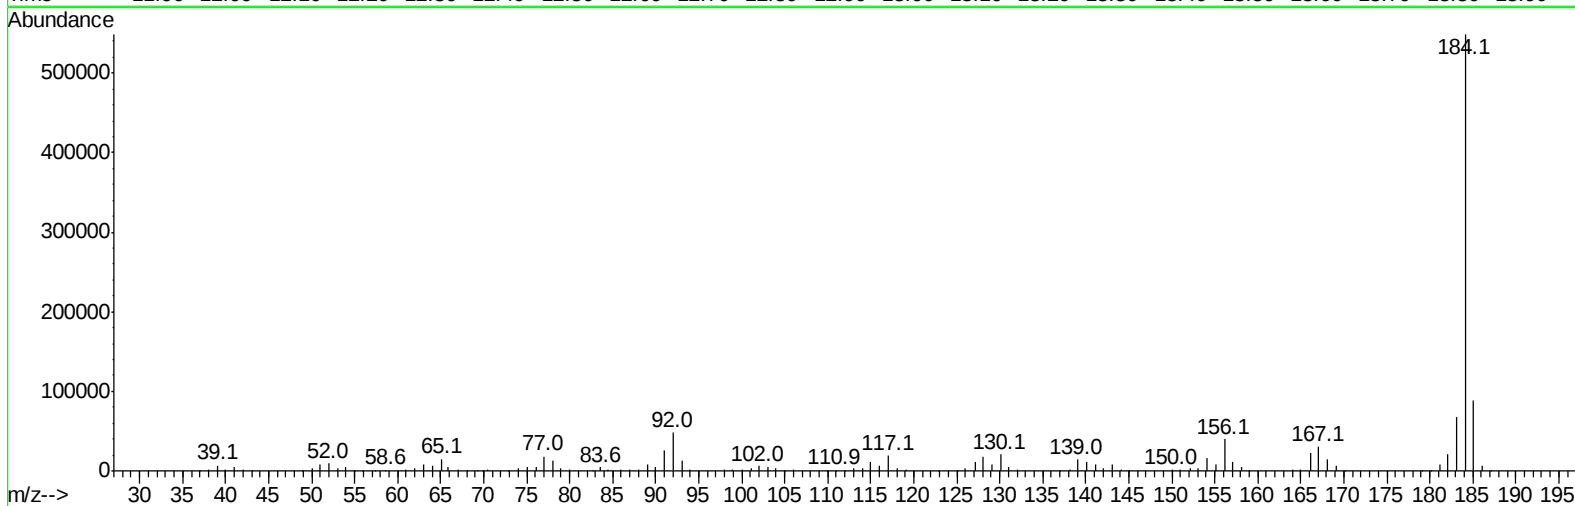


Data Path : Z:\HPCHEM1\BNA F\DATA\BF041717\
Data File : BF094449.D
Acq On : 17 Apr 2017 15:01
Operator : SJ/MA
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Apr 18 07:41:53 2017
Quant Method : Z:\HPCHEM1\BNA F\METHODS\8270-BF041717.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Apr 17 14:59:23 2017
Response via : Initial Calibration

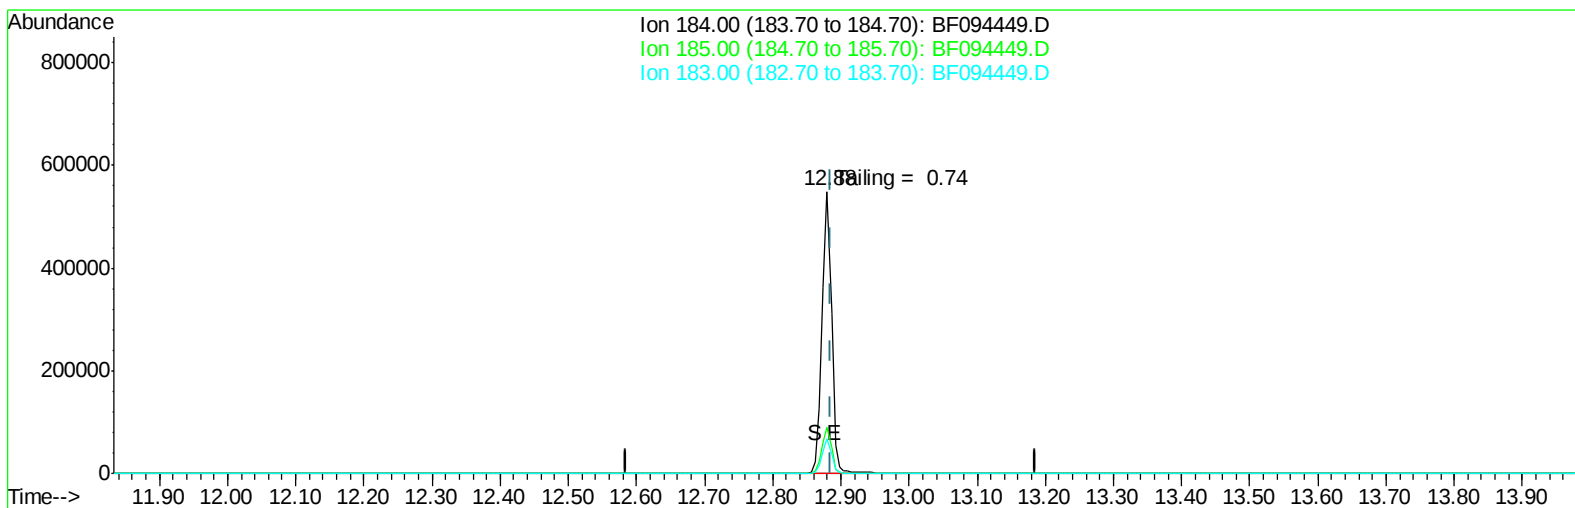

TIC: BF094449.D

(76) Benzidine



12.880min (-0.006) 0.00ng

response 519545

Ion	Exp%	Act%
184.00	100	100
185.00	19.40	16.18
183.00	12.20	12.29
0.00	0.00	0.00

```
Data Path : Z:\HPCHEM1\BNA F\DATA\BF041717\  
Data File : BF094449.D  
Acq On    : 17 Apr 2017  15:01  
Operator  : SJ/MA  
Sample    : DFTPP  
Misc      :  
ALS Vial  : 1      Sample Multiplier: 1
```

Quant Time: Apr 18 07:41:53 2017
Quant Method : Z:\HPCHEM1\BNA F\METHODS\8270-BF041717.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Apr 17 14:59:23 2017
Response via : Initial Calibration

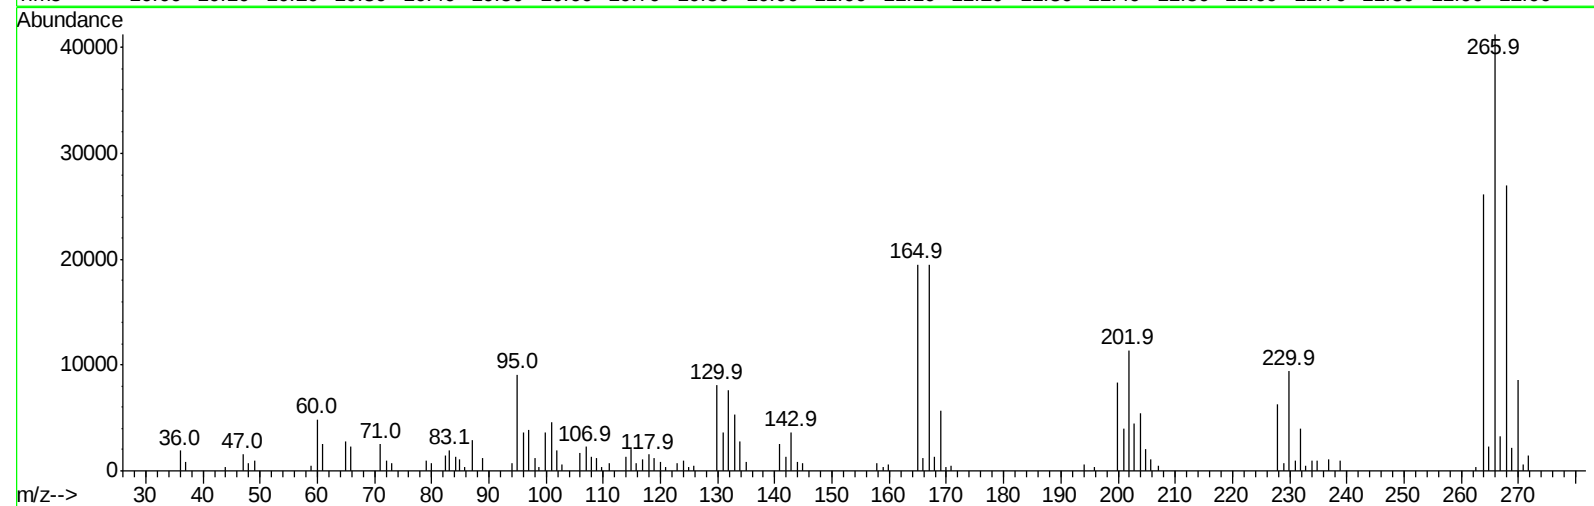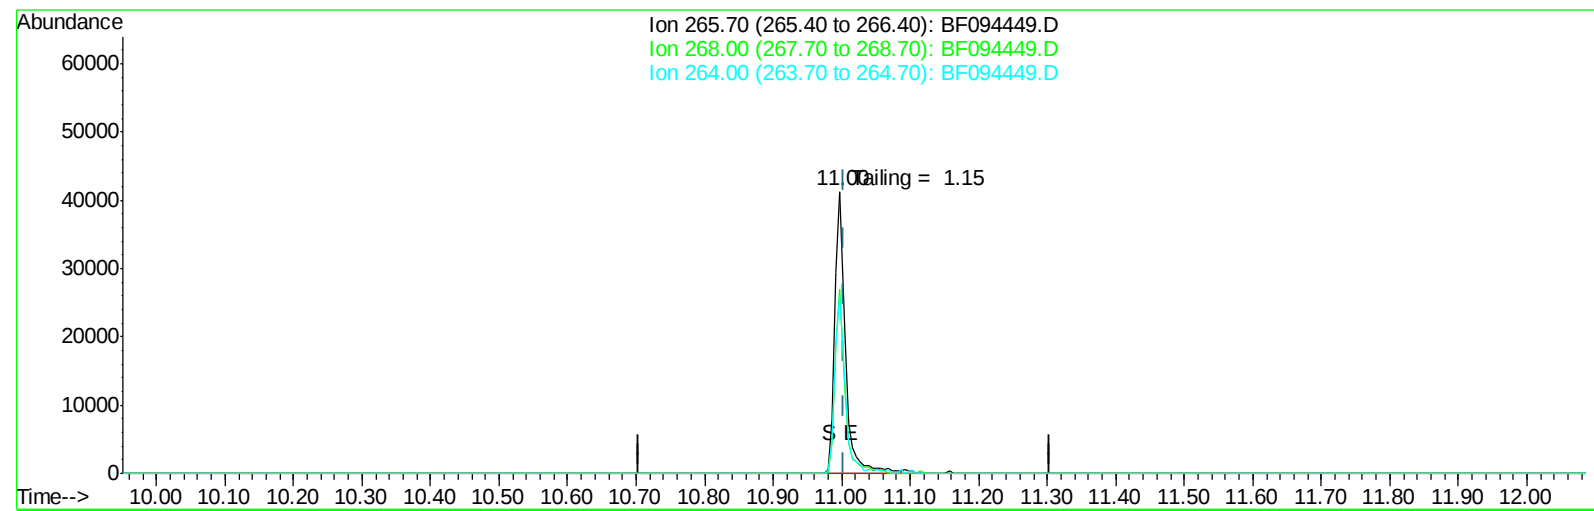

TIC: BF094449.D

(69) Pentachlorophenol (C)

10.998min (-0.006) 0.00ng

response 43214

Ion	Exp%	Act%
265.70	100	100
268.00	63.90	65.52
264.00	64.60	63.32
0.00	0.00	0.00