


Data Path : Z:\HPCHEM1\BNA_F\DATA\BF041717\
 Data File : BF094440.D
 Acq On : 17 Apr 2017 10:53
 Operator : SJ/MA
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF041717.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Mon Apr 17 14:59:23 2017

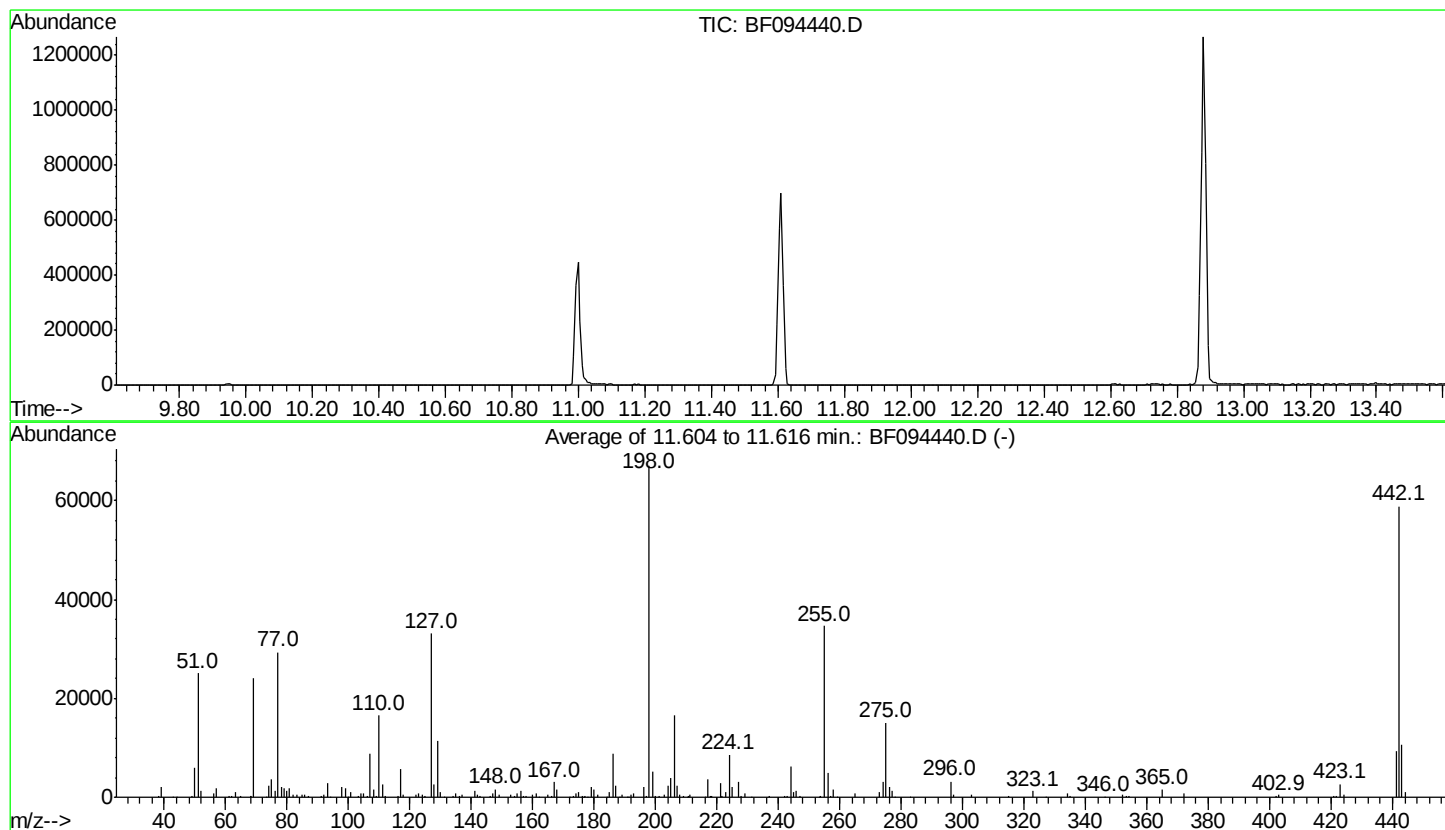

AutoFind: Scans 1652, 1653, 1654; Background Corrected with Scan 1646

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	37.4	25107	PASS
68	69	0.00	2	1.0	237	PASS
69	198	0.00	100	35.8	24007	PASS
70	69	0.00	2	0.0	0	PASS
127	198	10	80	49.3	33053	PASS
197	198	0.00	2	0.3	231	PASS
198	198	100	100	100.0	67090	PASS
199	198	5	9	7.7	5141	PASS
275	198	10	60	22.6	15137	PASS
365	198	1	100	2.3	1526	PASS
441	442	0.01	24	15.8	9294	PASS
442	198	50	100	87.8	58898	PASS
443	442	15	24	18.0	10615	PASS