


Data Path : Z:\HPCHEM1\BNA_F\DATA\BF041717\
 Data File : BF094449.D
 Acq On : 17 Apr 2017 15:01
 Operator : SJ/MA
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF041717.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Mon Apr 17 14:59:23 2017

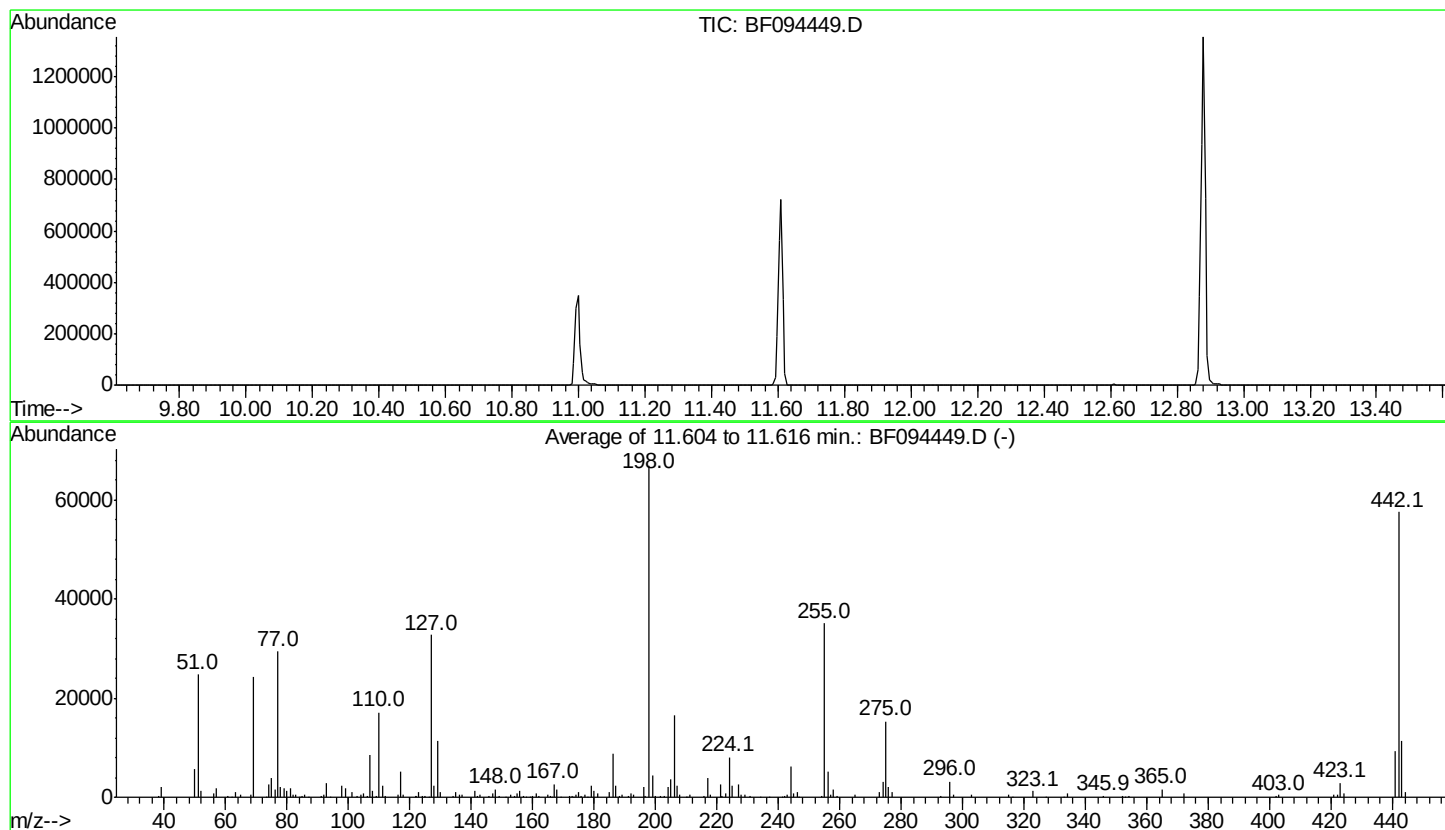

AutoFind: Scans 1652, 1653, 1654; Background Corrected with Scan 1646

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	36.9	24704	PASS
68	69	0.00	2	1.9	451	PASS
69	198	0.00	100	36.1	24179	PASS
70	69	0.00	2	0.0	0	PASS
127	198	10	80	48.9	32682	PASS
197	198	0.00	2	0.3	202	PASS
198	198	100	100	100.0	66896	PASS
199	198	5	9	6.5	4340	PASS
275	198	10	60	22.8	15276	PASS
365	198	1	100	2.4	1585	PASS
441	442	0.01	24	16.1	9231	PASS
442	198	50	100	86.0	57512	PASS
443	442	15	24	20.0	11475	PASS