
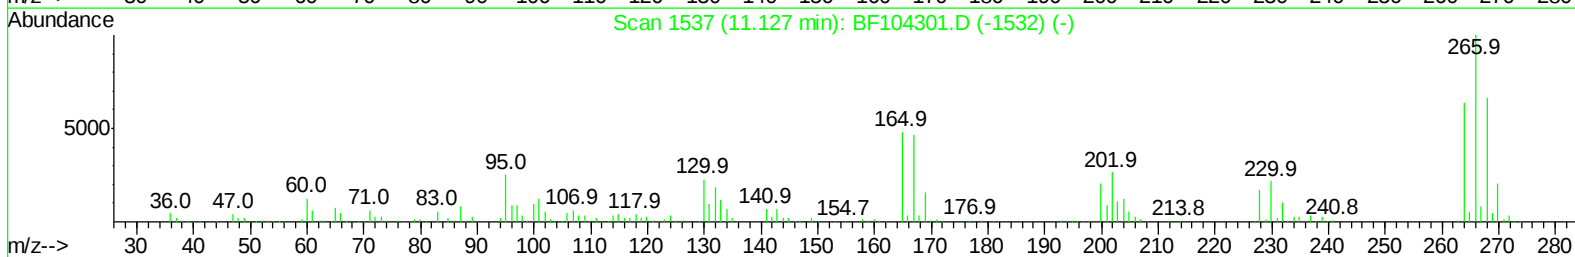
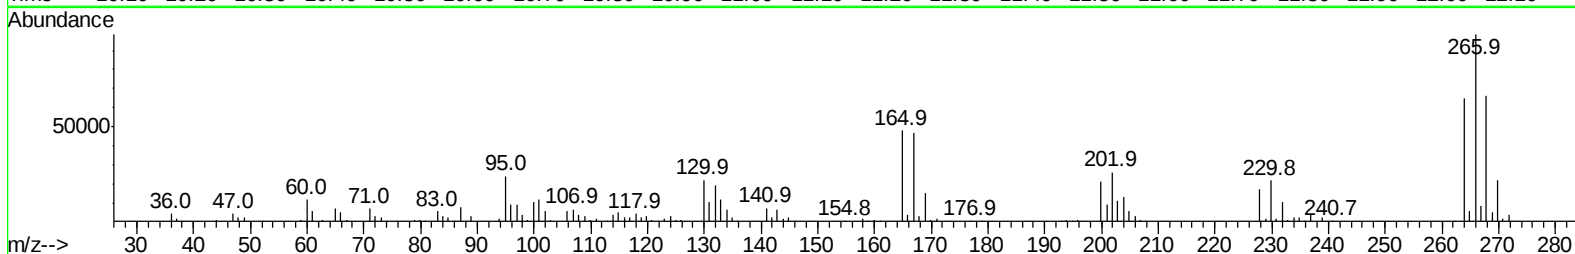


Data Path : Z:\HPCHEM1\BNA F\DATA\BF041718\
Data File : BF104560.D
Acq On : 17 Apr 2018 14:49
Operator : JU/SJ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Apr 18 03:49:14 2018
Quant Method : Z:\HPCHEM1\BNA F\METHODS\8270-BF040618.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Apr 17 17:08:38 2018
Response via : Initial Calibration

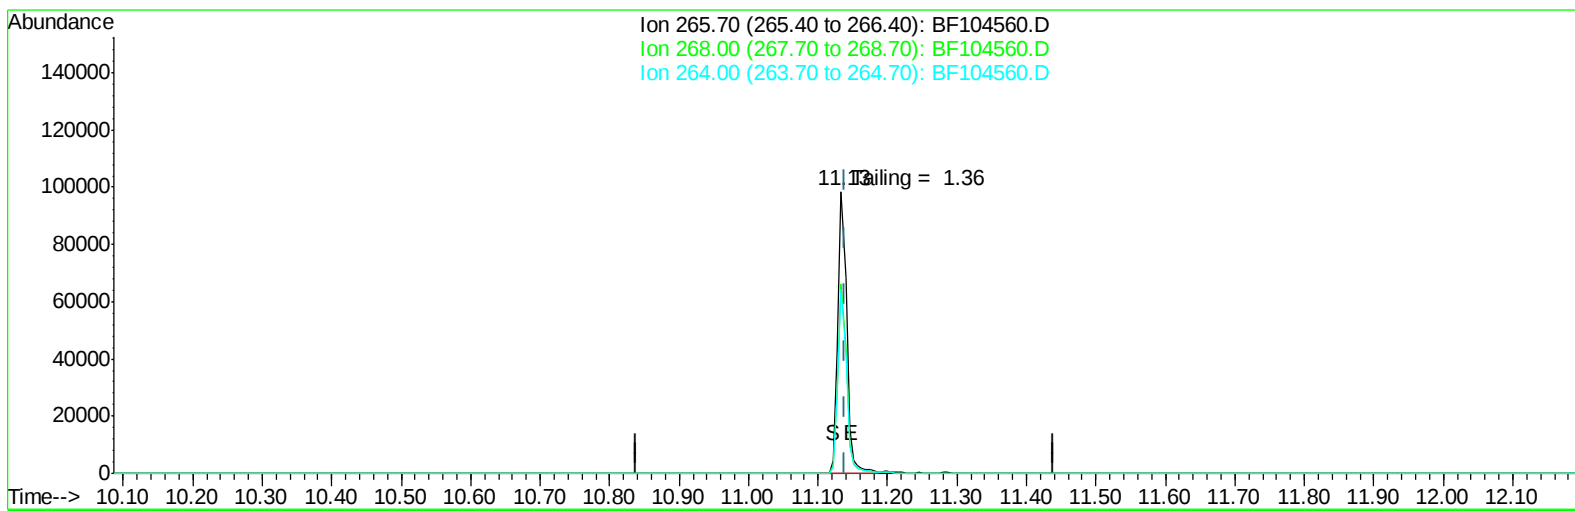

TIC: BF104560.D

(69) Pentachlorophenol (C)




11.133min (-0.006) 83957.03ng

response 85788

Ion	Exp%	Act%
265.70	100	100
268.00	63.90	67.38
264.00	61.90	65.62
0.00	0.00	0.00

Data Path : Z:\HPCHEM1\BNA F\DATA\BF041718\
Data File : BF104560.D
Acq On : 17 Apr 2018 14:49
Operator : JU/SJ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Apr 18 03:49:14 2018
Quant Method : Z:\HPCHEM1\BNA F\METHODS\8270-BF040618.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Apr 17 17:08:38 2018
Response via : Initial Calibration

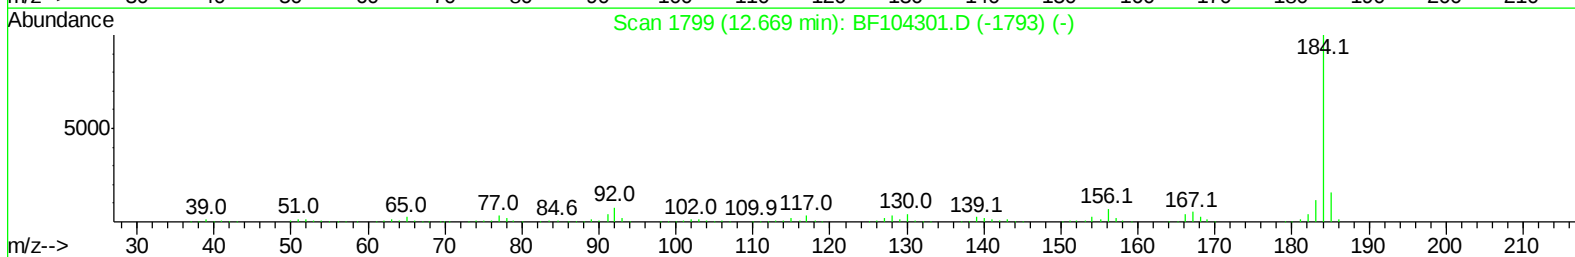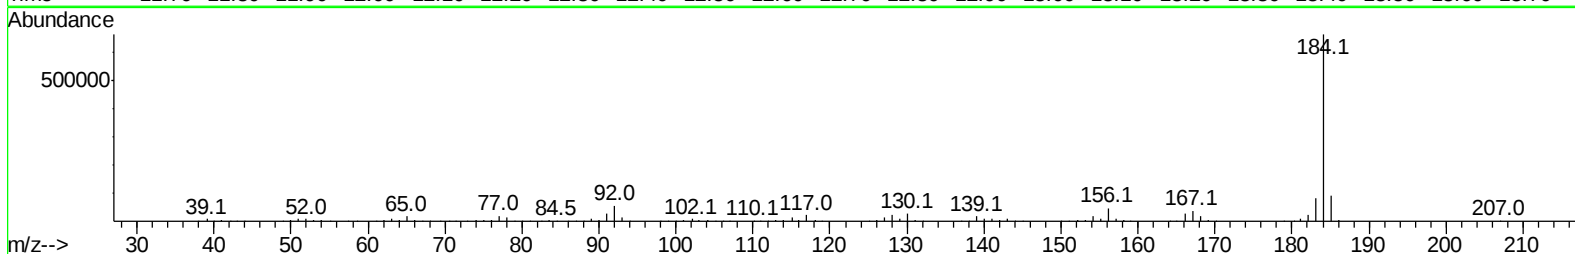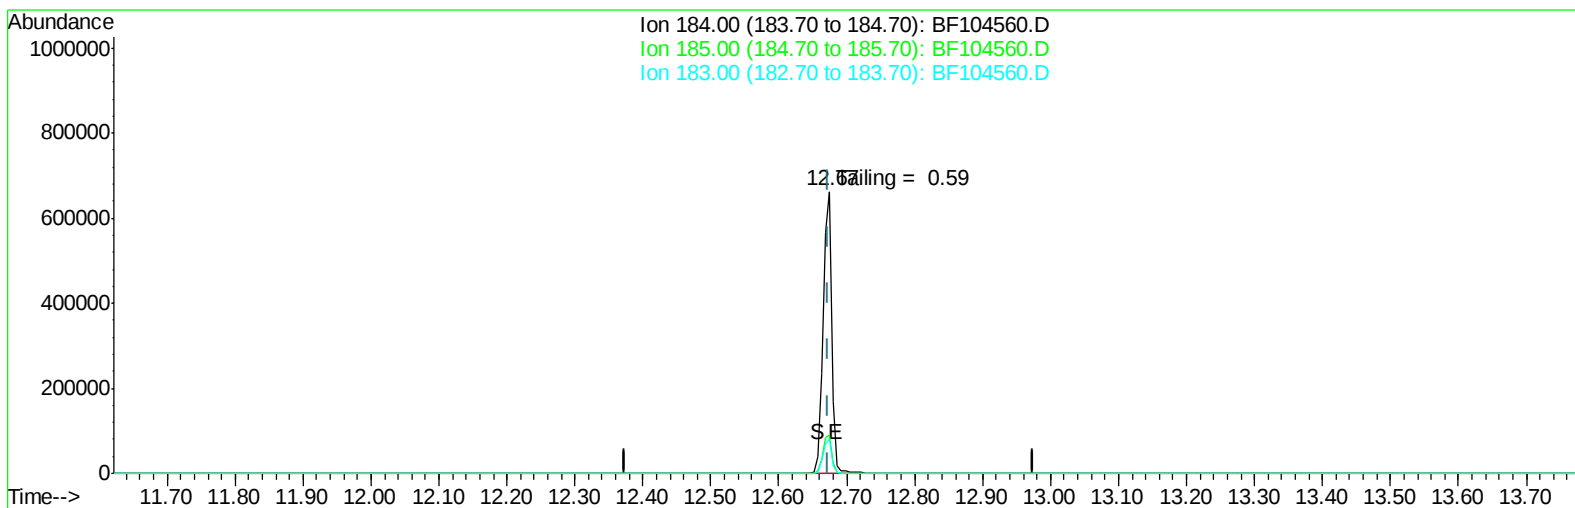

TIC: BF104560.D

(76) Benzidine

12.674min (+0.000) 0.00ng

response 607481

Ion	Exp%	Act%
184.00	100	100
185.00	15.70	13.85
183.00	11.60	12.14
0.00	0.00	0.00