


Data Path : Z:\HPCHEM1\BNA F\Data\BF041718\
 Data File : BF104560.D
 Acq On : 17 Apr 2018 14:49
 Operator : JU/SJ
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF040618.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Wed Apr 18 11:52:19 2018

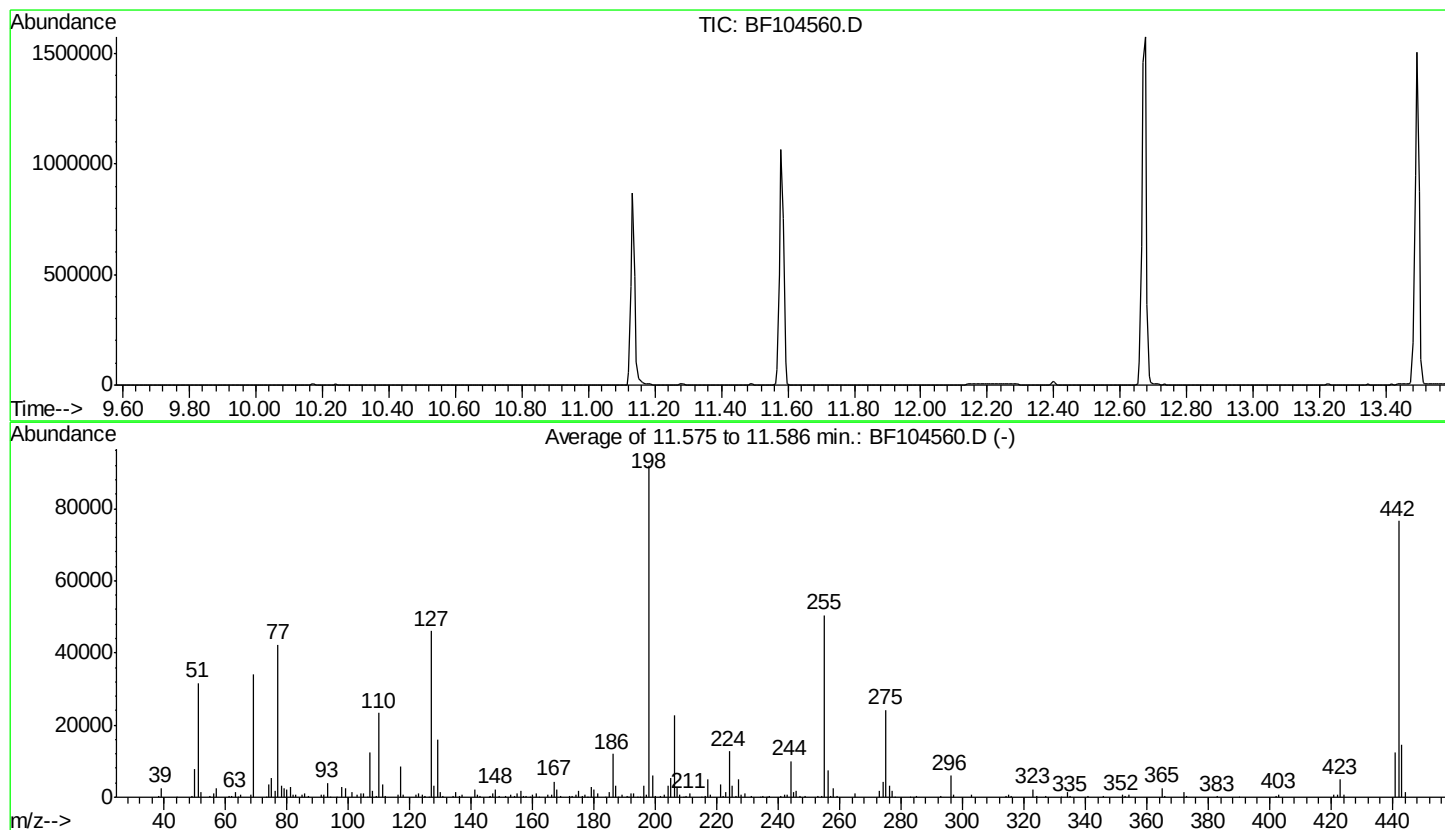

AutoFind: Scans 1613, 1614, 1615; Background Corrected with Scan 1608

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	34.4	31629	PASS
68	69	0.00	2	1.8	611	PASS
69	198	0.00	100	36.9	33914	PASS
70	69	0.00	2	0.0	0	PASS
127	198	10	80	50.1	46042	PASS
197	198	0.00	2	0.8	721	PASS
198	198	100	100	100.0	91893	PASS
199	198	5	9	6.7	6198	PASS
275	198	10	60	26.4	24232	PASS
365	198	1	100	2.9	2639	PASS
441	443	0.01	100	85.2	12428	PASS
442	198	50	100	83.2	76498	PASS
443	442	15	24	19.1	14585	PASS