
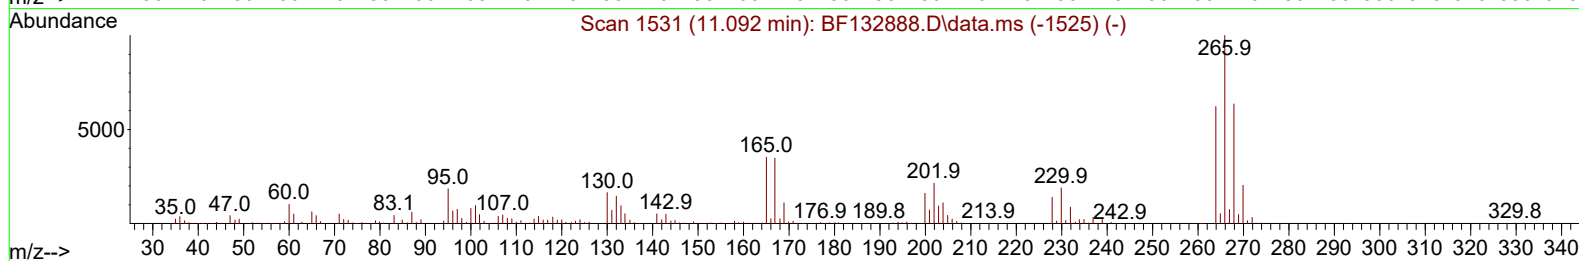
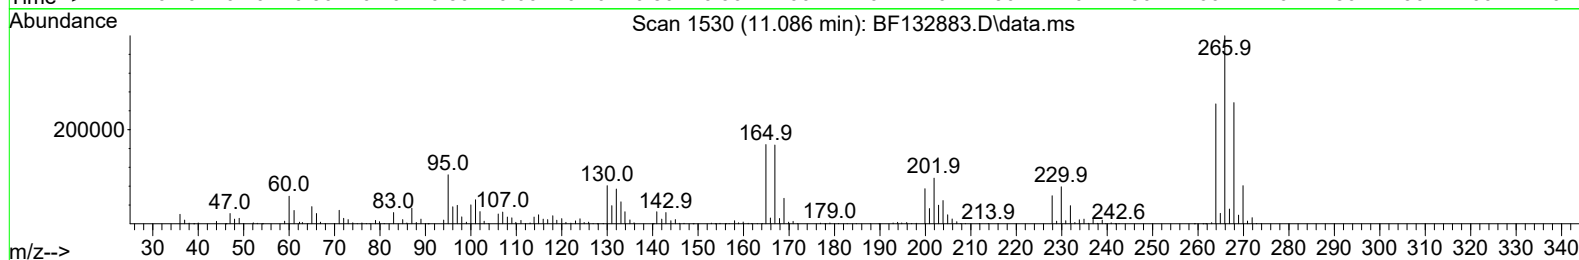


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF041723\
Data File : BF132883.D
Acq On : 17 Apr 2023 12:00
Operator : CG\JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Apr 18 07:06:15 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF041723.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Apr 18 04:51:21 2023
Response via : Initial Calibration

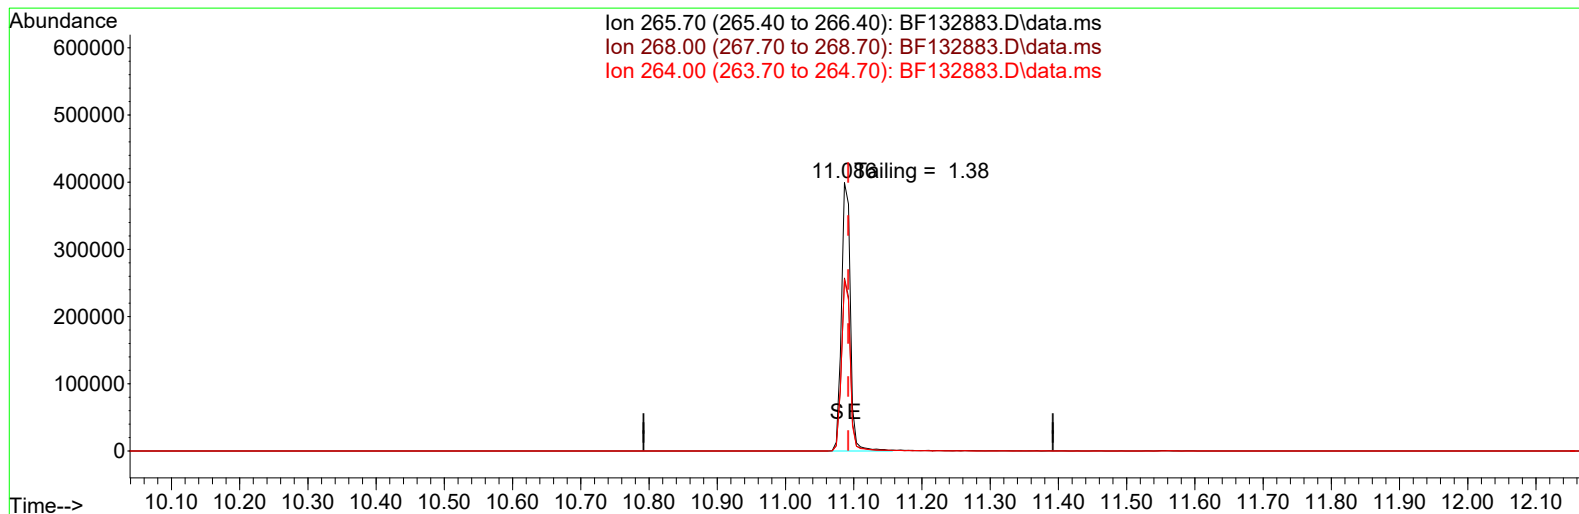

TIC: BF132883.D\data.ms

(70) Pentachlorophenol (C)




11.086min (-0.006) 174970.09 ng

response 362491

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	63.60	64.43
264.00	62.20	63.77
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF041723\
Data File : BF132883.D
Acq On : 17 Apr 2023 12:00
Operator : CG\JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Apr 18 07:06:15 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF041723.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Apr 18 04:51:21 2023
Response via : Initial Calibration

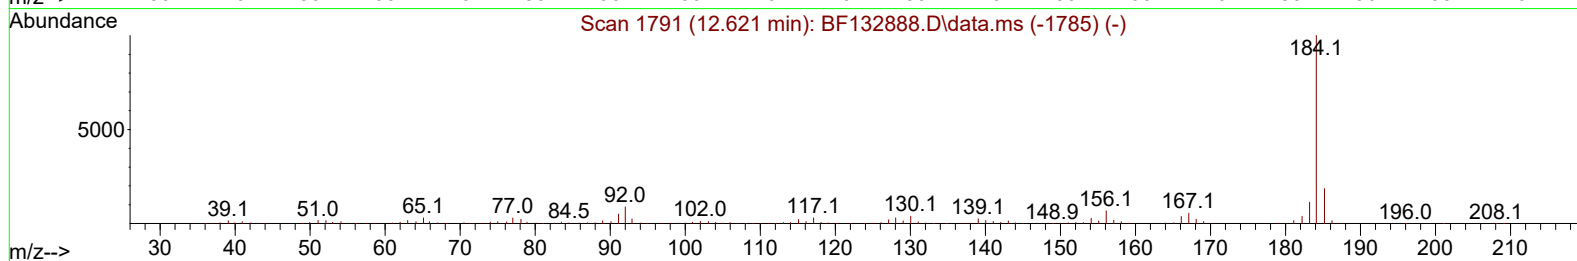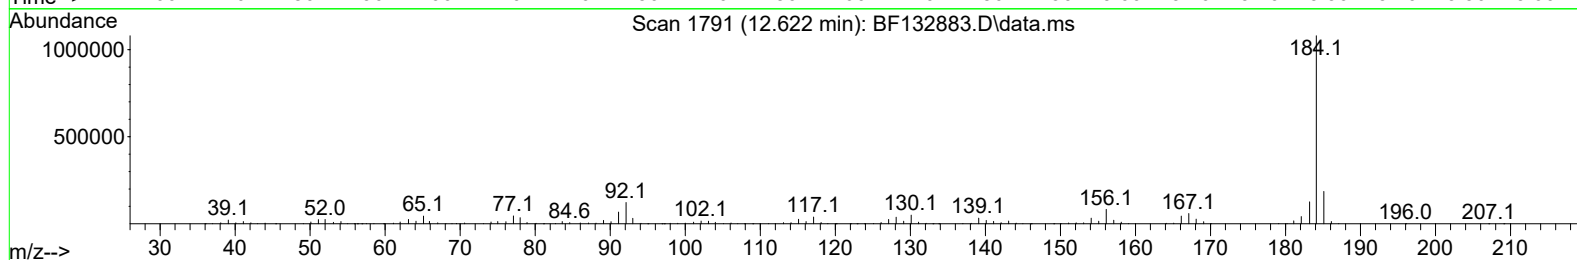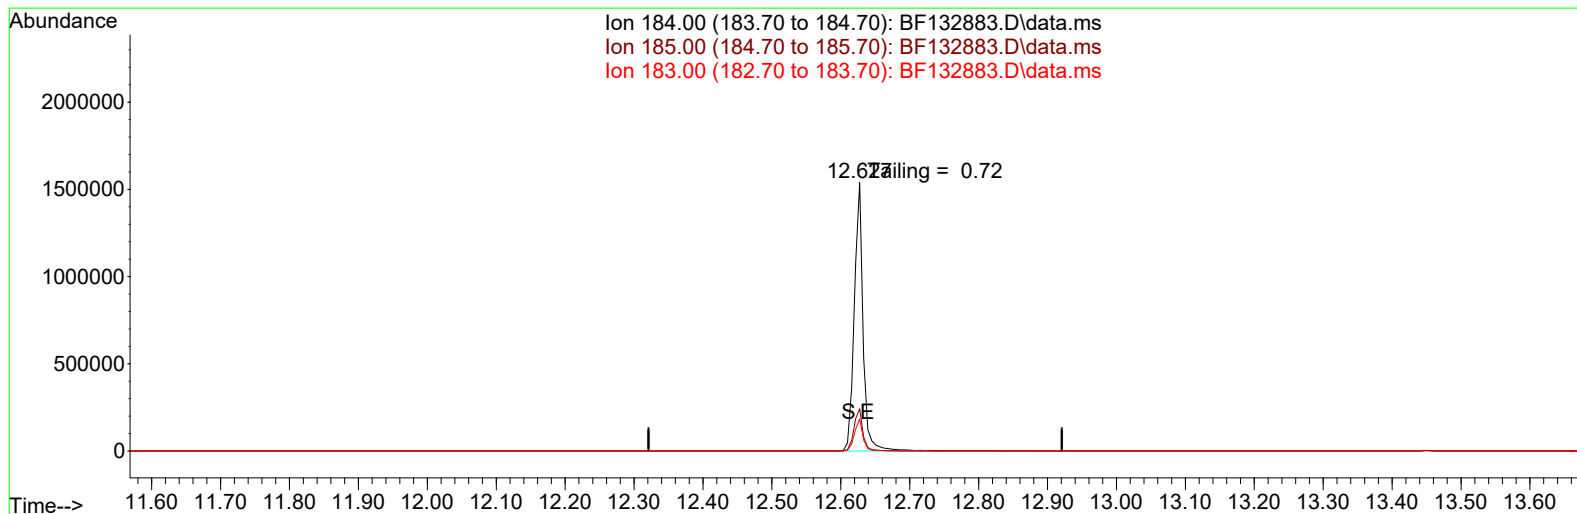

TIC: BF132883.D\data.ms

(77) Benzidine

12.621min (-12.621) 0.00 ng

response 0

Ion	Exp%	Act%
184.00	100.00	0.00
185.00	18.60	0.00#
183.00	11.30	0.00#
0.00	0.00	0.00