
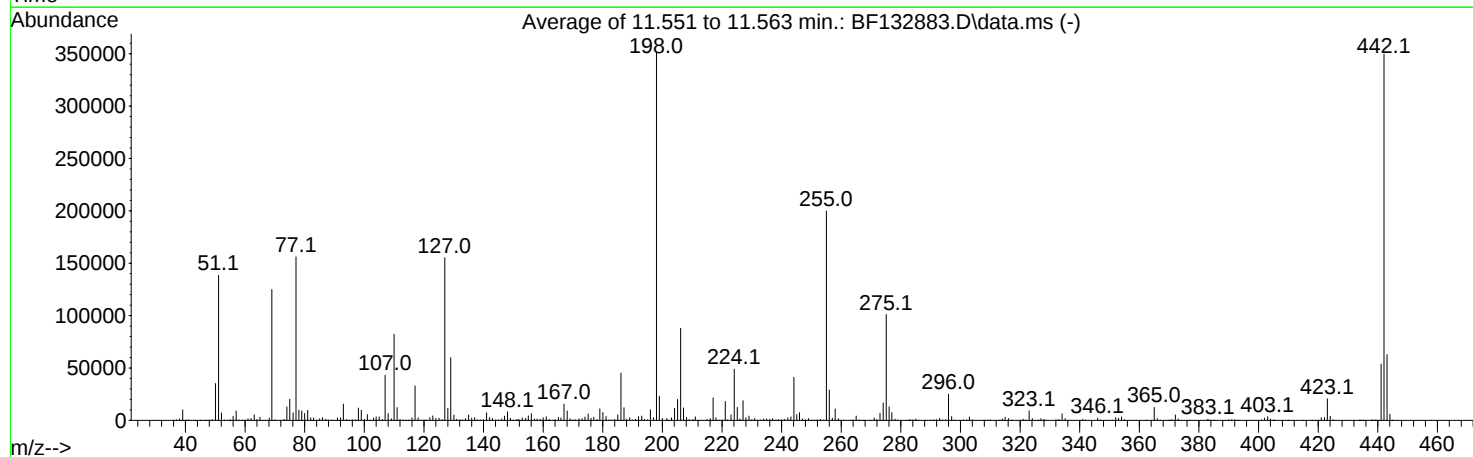


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF041723\
Data File : BF132883.D
Acq On : 17 Apr 2023 12:00
Operator : CG\JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF041723.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Tue Apr 18 04:51:21 2023

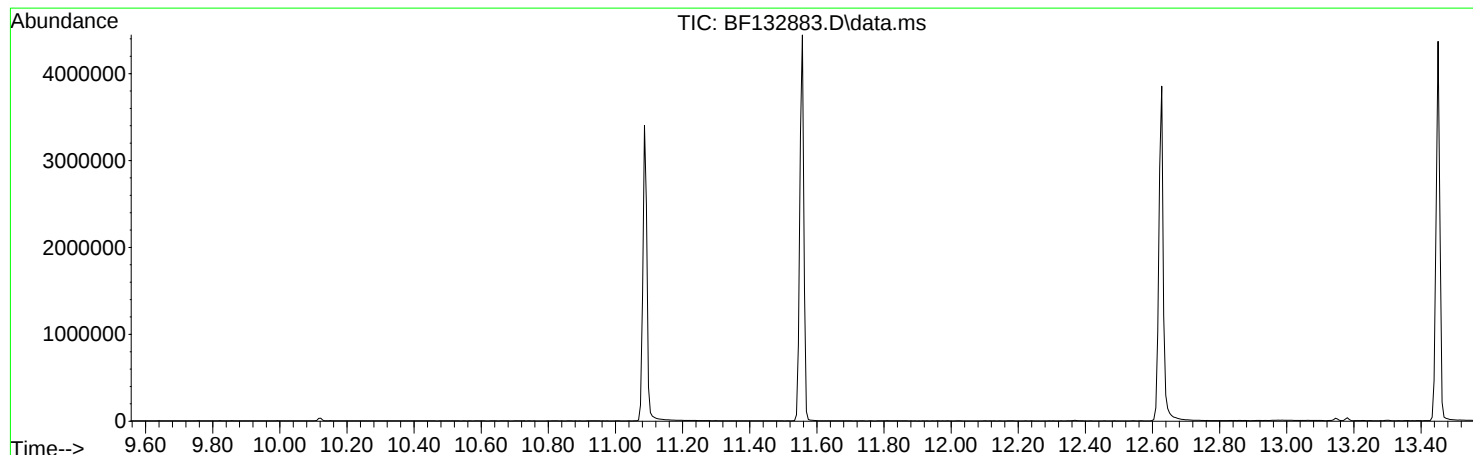




AutoFind: Scans 1609, 1610, 1611; Background Corrected with Scan 1603

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	39.5	138627	PASS
68	69	0.00	2	1.7	2155	PASS
69	198	0.00	100	35.6	125000	PASS
70	69	0.00	2	0.5	606	PASS
127	198	10	80	44.3	155424	PASS
197	198	0.00	2	0.7	2595	PASS
198	198	100	100	100.0	351189	PASS
199	198	5	9	6.6	23042	PASS
275	198	10	60	28.8	101096	PASS
365	198	1	100	3.5	12436	PASS
441	198	0.01	100	15.3	53744	PASS
442	442	50	100	100.0	349611	PASS
443	442	15	24	18.0	62808	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF041723\
Data File : BF132883.D
Acq On : 17 Apr 2023 12:00
Operator : CG\JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Quant Time: Apr 18 07:06:15 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF041723.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Apr 18 04:51:21 2023
Response via : Initial Calibration

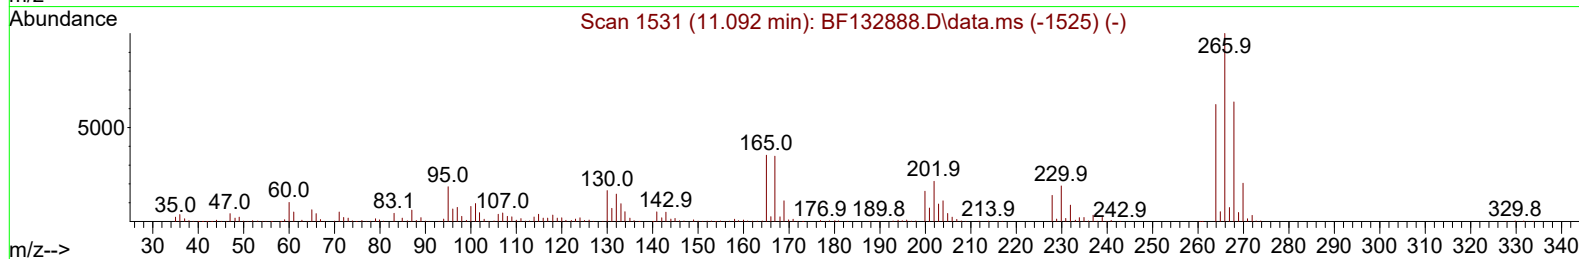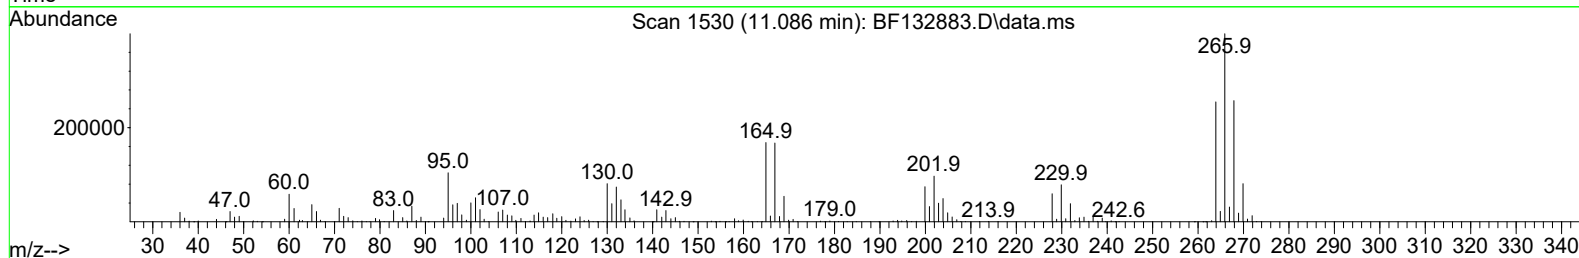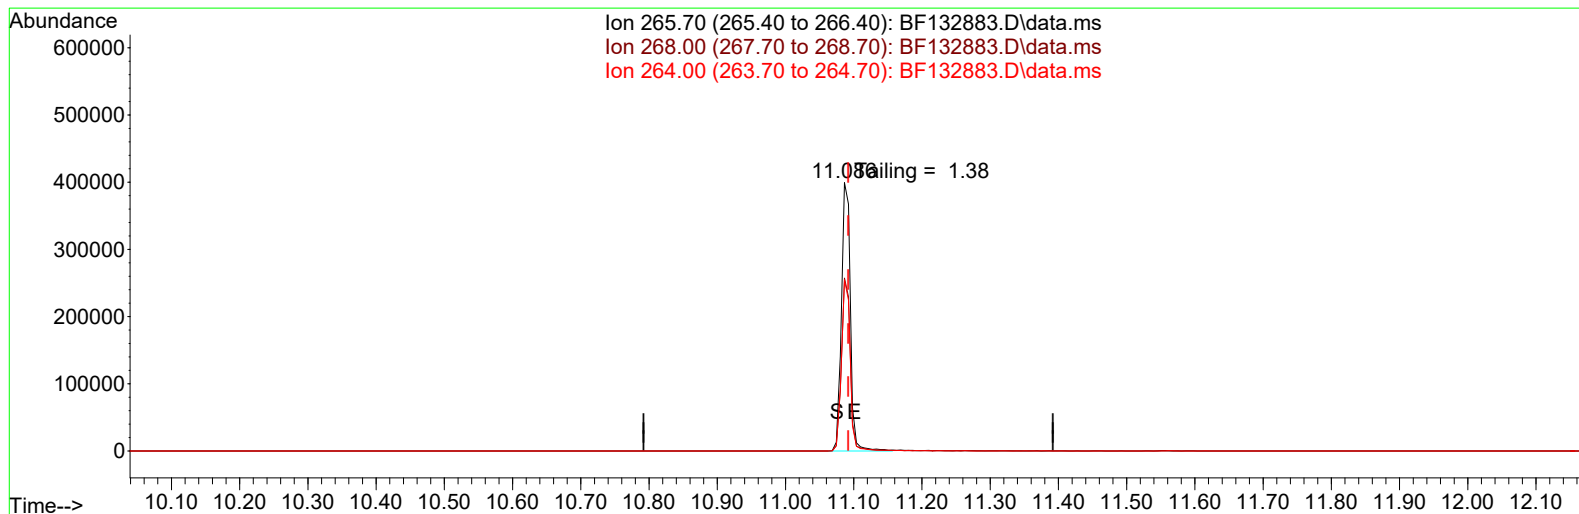

TIC: BF132883.D\data.ms

(70) Pentachlorophenol (C)

11.086min (-0.006) 174970.09 ng




response 362491

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	63.60	64.43
264.00	62.20	63.77
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF041723\
Data File : BF132883.D
Acq On : 17 Apr 2023 12:00
Operator : CG\JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Quant Time: Apr 18 07:06:15 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF041723.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Apr 18 04:51:21 2023
Response via : Initial Calibration

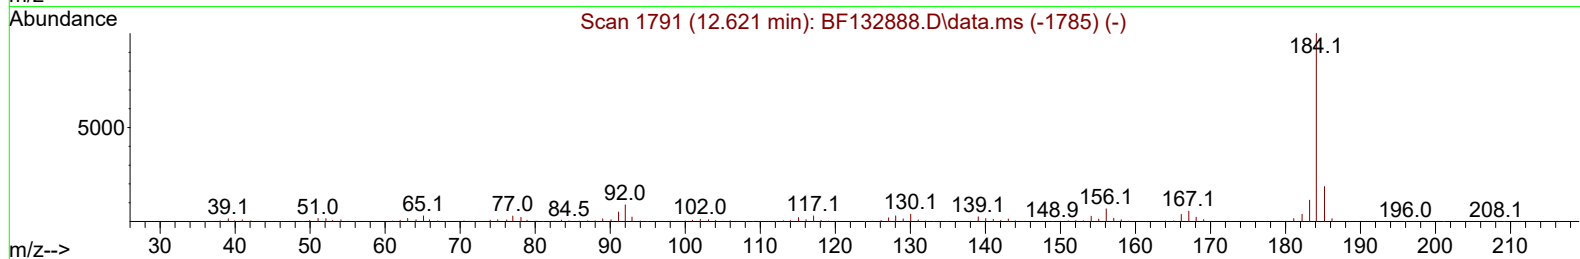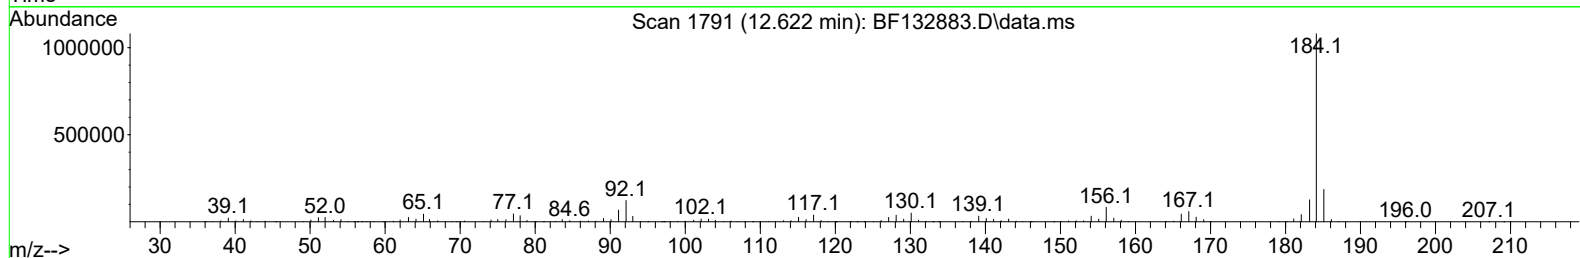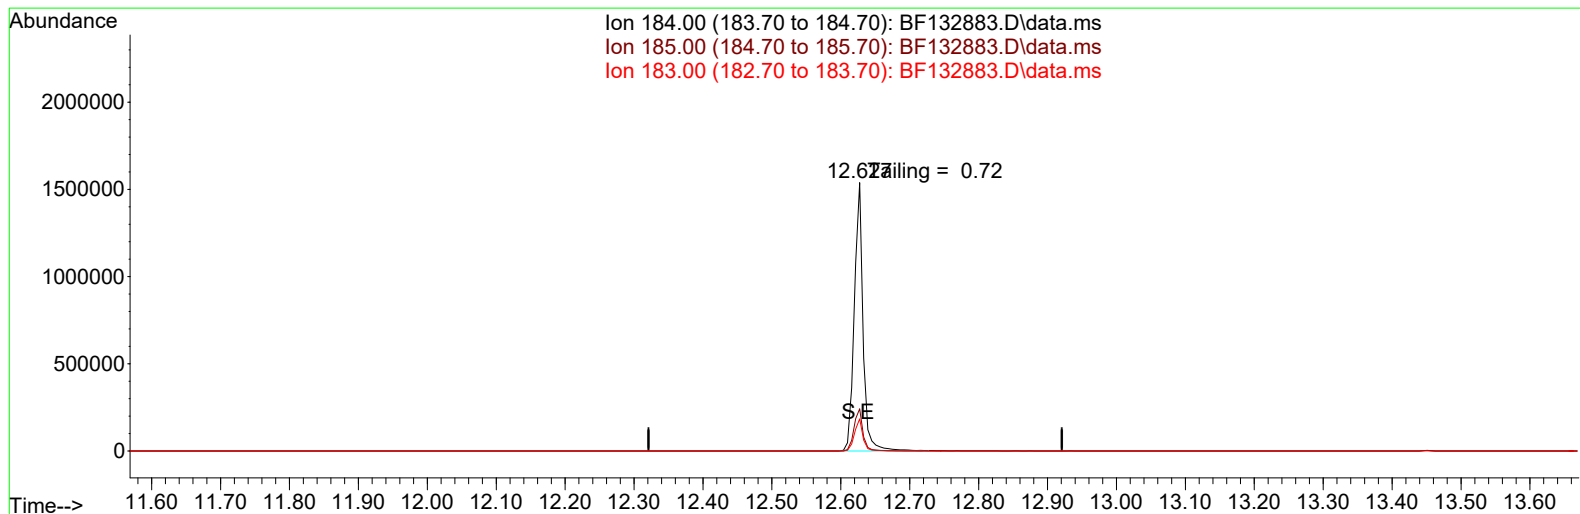

TIC: BF132883.D\data.ms

(77) Benzidine

12.621min (-12.621) 0.00 ng

response 0

Ion	Exp%	Act%
184.00	100.00	0.00
185.00	18.60	0.00#
183.00	11.30	0.00#
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
4/17/2023	BNA_F	<u>BF132883.D</u>
Compound Name	Response	Retention Time
DDT	547670	13.451
DDD	7138	13.145
DDE	174	12.816
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
7312	554982	1.32

Instrument :
BNA_F
ClientSampleId :
DFTPP