
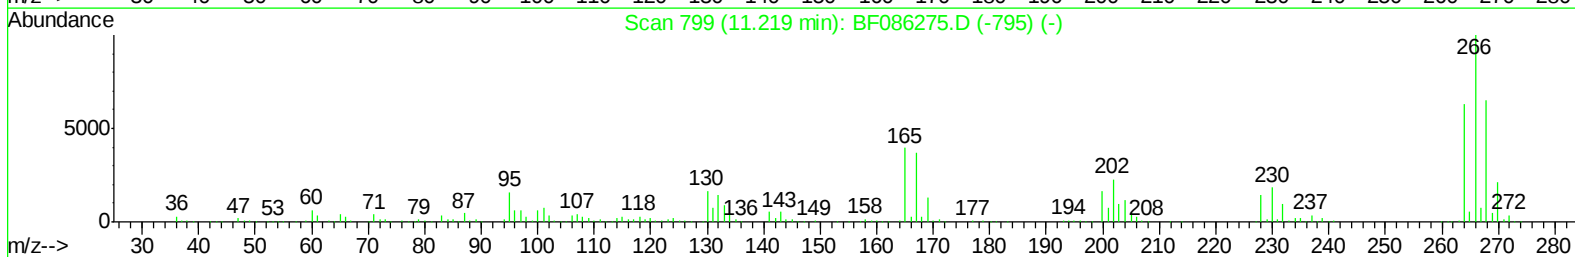
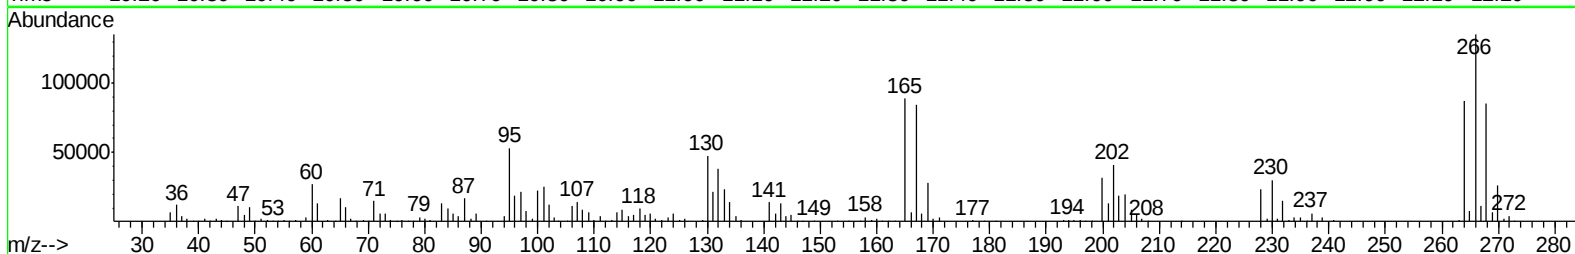


Data Path : Z:\HPCHEM1\BNA_F\Data\BF041816\
Data File : BF086274.D
Acq On : 18 Apr 2016 11:26
Operator : UM/SJ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Apr 19 04:43:52 2016
Quant Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF041516.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Apr 15 15:56:31 2016
Response via : Initial Calibration

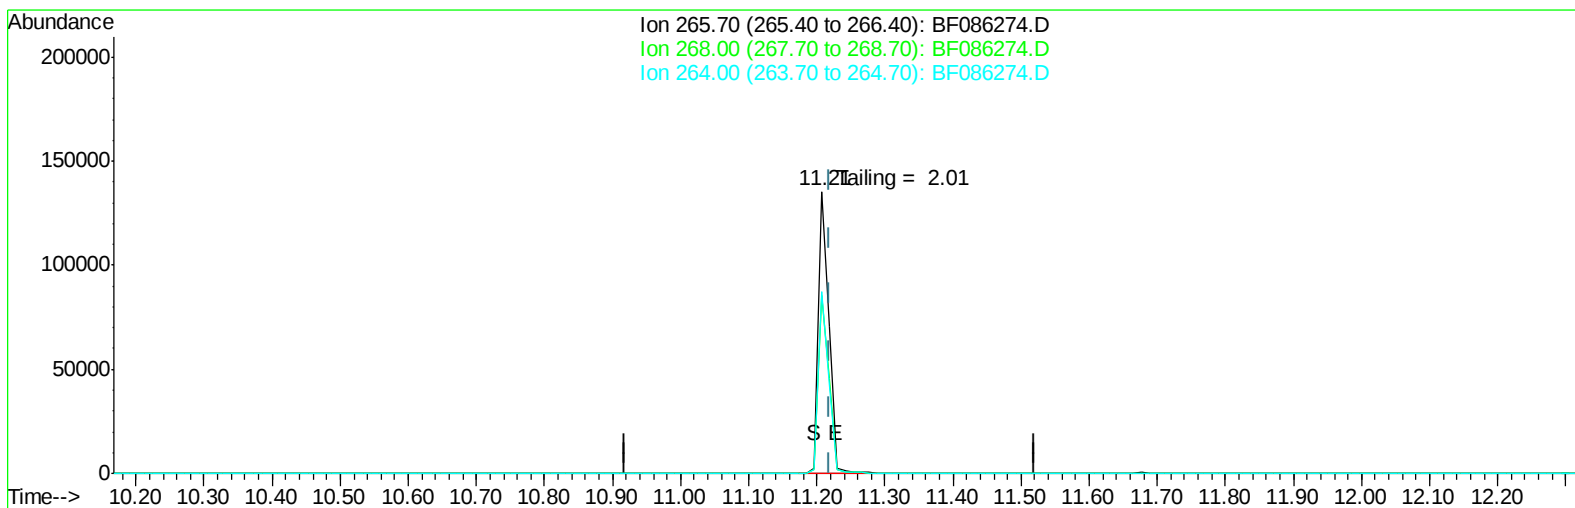

TIC: BF086274.D

(69) Pentachlorophenol (C)




11.208min (-0.012) 111308.14ng

response 146998

Ion	Exp%	Act%
265.70	100	100
268.00	66.20	62.98
264.00	64.10	64.62
0.00	0.00	0.00

Data Path : Z:\HPCHEM1\BNA_F\Data\BF041816\
Data File : BF086274.D
Acq On : 18 Apr 2016 11:26
Operator : UM/SJ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Apr 19 04:43:52 2016
Quant Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF041516.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Apr 15 15:56:31 2016
Response via : Initial Calibration

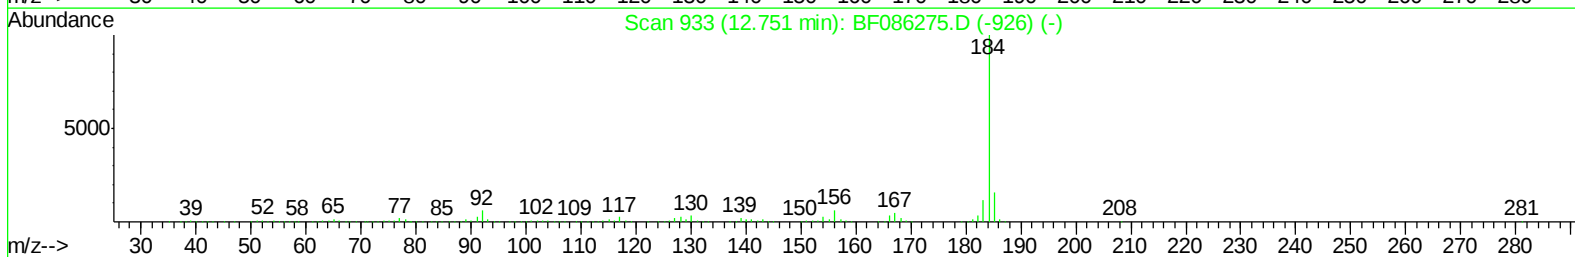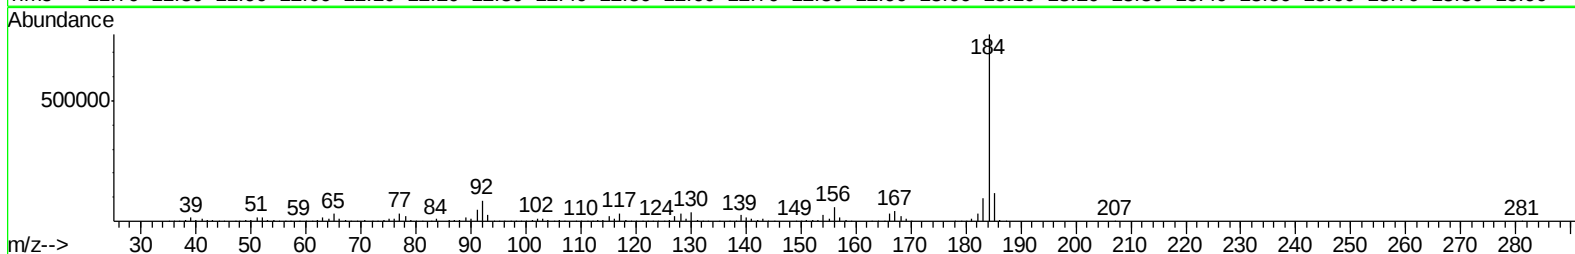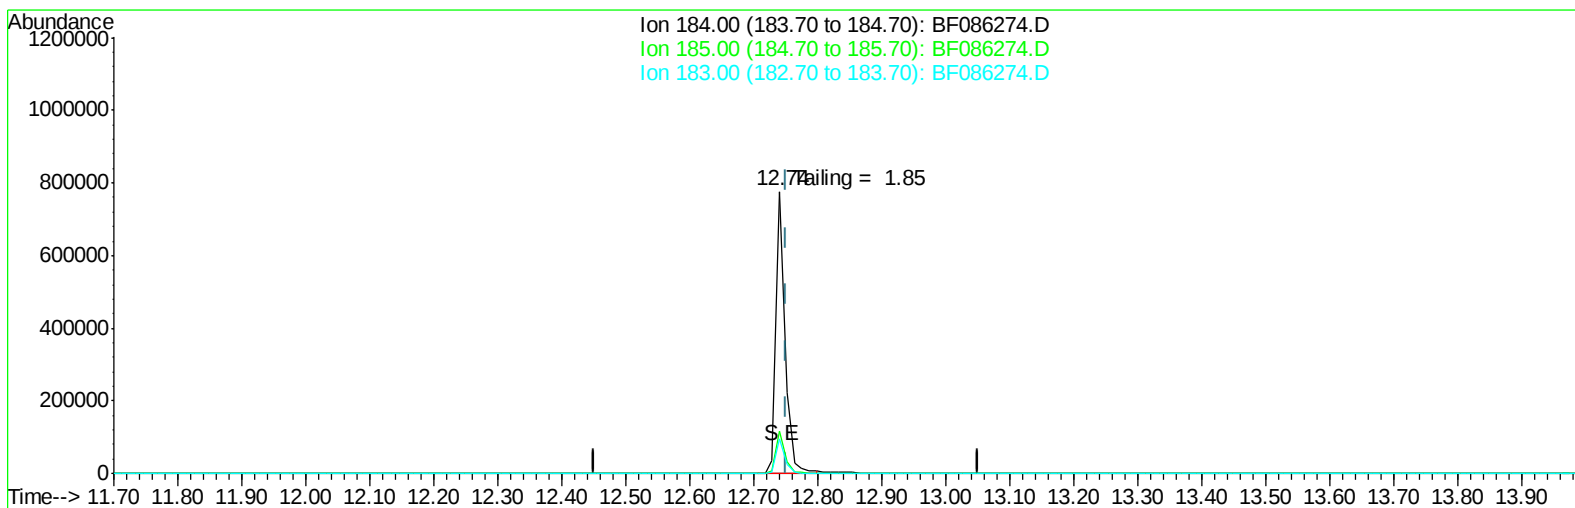

TIC: BF086274.D

(76) Benzidine

12.739min (-0.012) 19075.55ng

response 768818

Ion	Exp%	Act%
184.00	100	100
185.00	17.70	15.03
183.00	12.20	12.13
0.00	0.00	0.00