


Data Path : Z:\HPCHEM1\BNA_F\Data\BF041816\
 Data File : BF086274.D
 Acq On : 18 Apr 2016 11:26
 Operator : UM/SJ
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF041516.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Fri Apr 15 15:56:31 2016

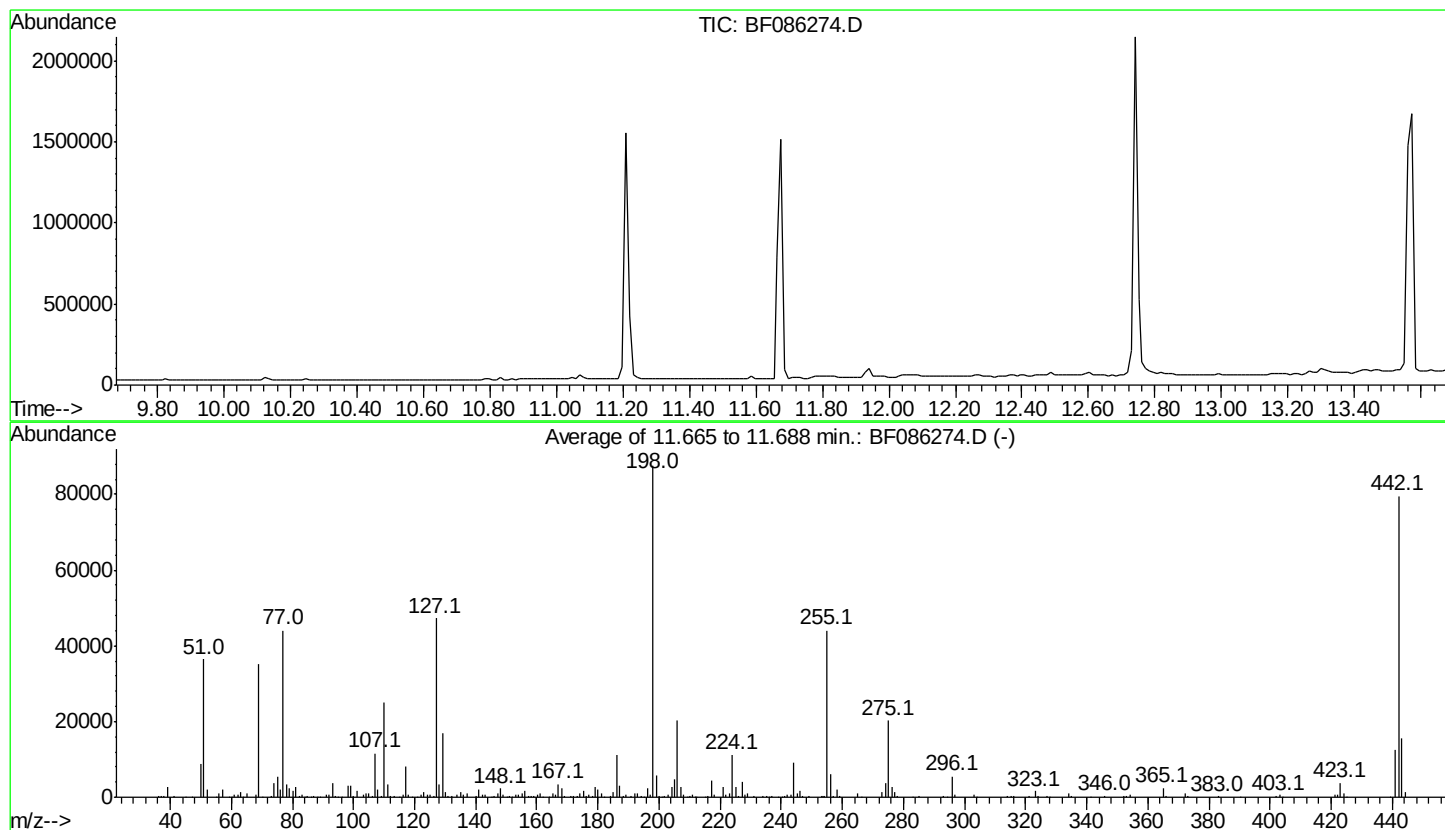

AutoFind: Scans 838, 839, 840; Background Corrected with Scan 835

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	41.6	36464	PASS
68	69	0.00	2	1.5	535	PASS
69	198	0.00	100	40.2	35211	PASS
70	69	0.00	2	0.4	131	PASS
127	198	10	80	53.9	47231	PASS
197	198	0.00	2	0.9	830	PASS
198	198	100	100	100.0	87583	PASS
199	198	5	9	6.6	5807	PASS
275	198	10	60	23.0	20133	PASS
365	198	1	100	2.9	2523	PASS
441	442	0.01	24	15.8	12585	PASS
442	198	50	100	90.9	79602	PASS
443	442	15	24	19.5	15516	PASS