
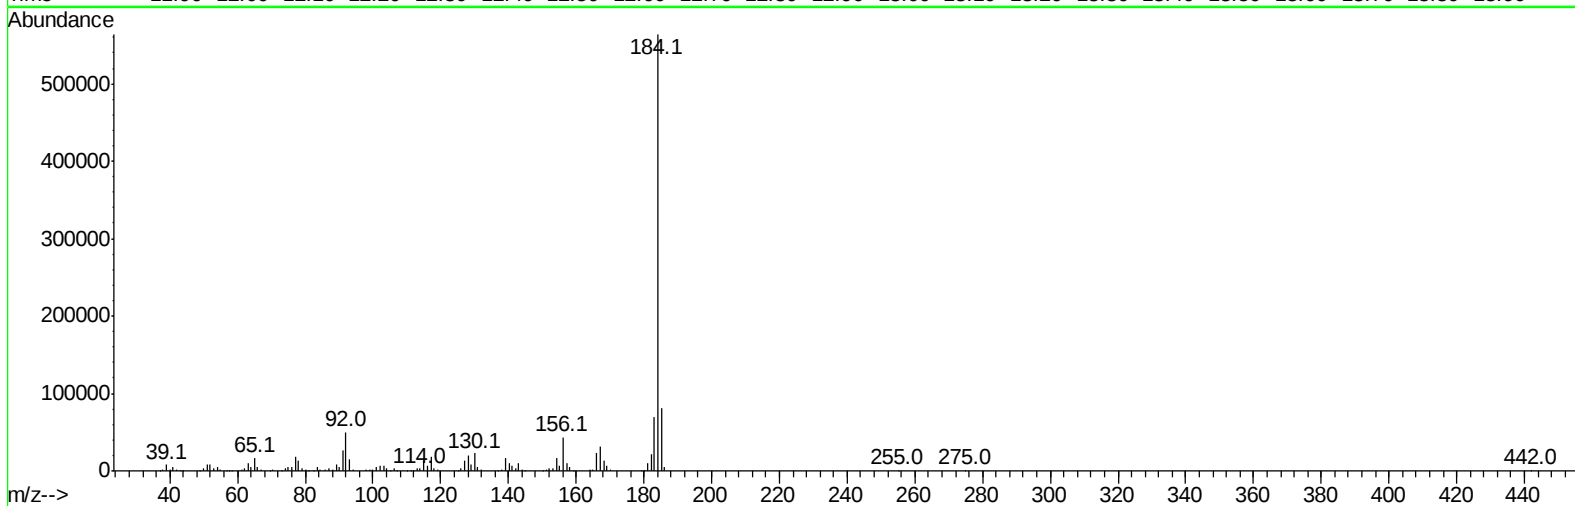


Data Path : Z:\HPCHEM1\BNA F\DATA\BF041817\
 Data File : BF094480.D
 Acq On : 18 Apr 2017 11:58
 Operator : SJ/MA
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Quant Time: Apr 19 07:50:17 2017
 Quant Method : Z:\HPCHEM1\BNA F\METHODS\8270-BF041717.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Mon Apr 17 14:59:23 2017
 Response via : Initial Calibration

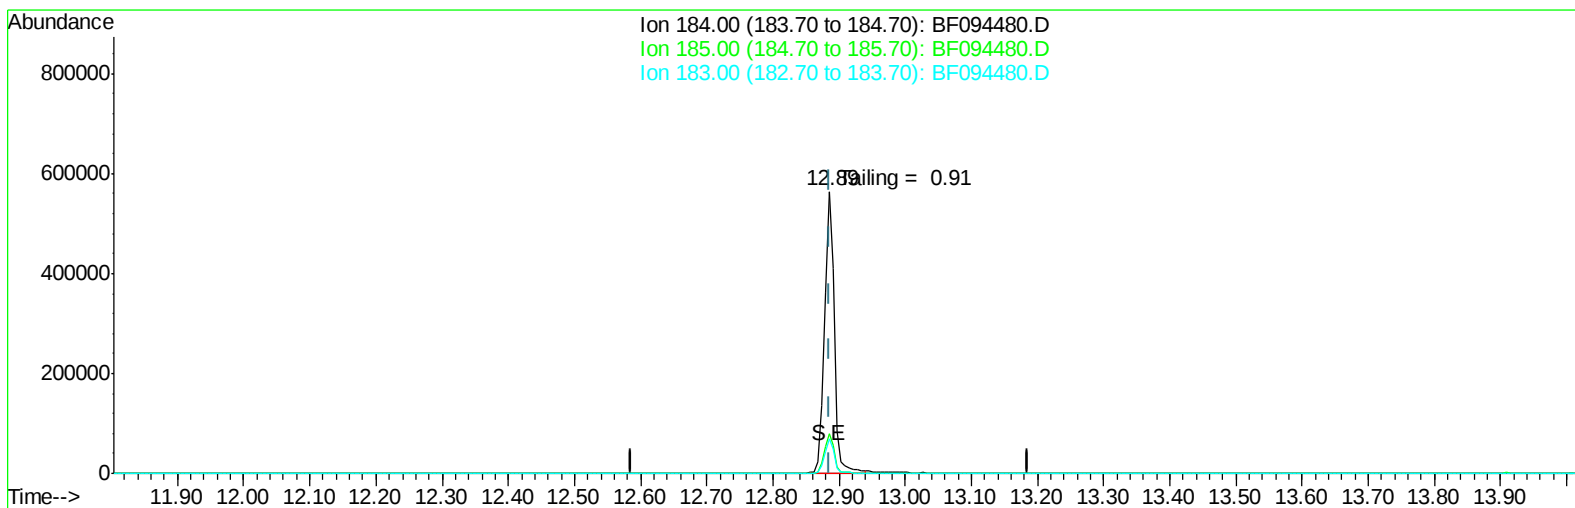

TIC: BF094480.D

(76) Benzidine



12.886min (-0.000) 0.00ng

response 597809

Ion	Exp%	Act%
184.00	100	100
185.00	19.40	14.27#
183.00	12.20	12.42
0.00	0.00	0.00

Data Path : Z:\HPCHEM1\BNA F\DATA\BF041817\
Data File : BF094480.D
Acq On : 18 Apr 2017 11:58
Operator : SJ/MA
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Apr 19 07:50:17 2017
Quant Method : Z:\HPCHEM1\BNA F\METHODS\8270-BF041717.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Apr 17 14:59:23 2017
Response via : Initial Calibration

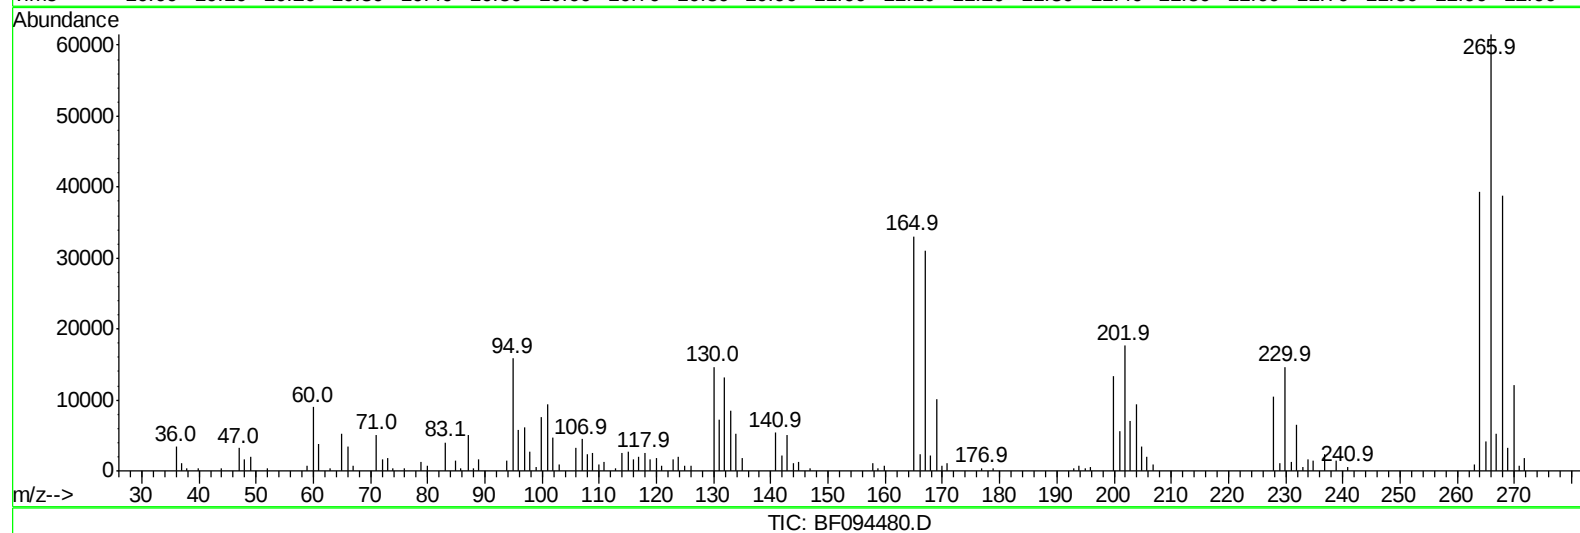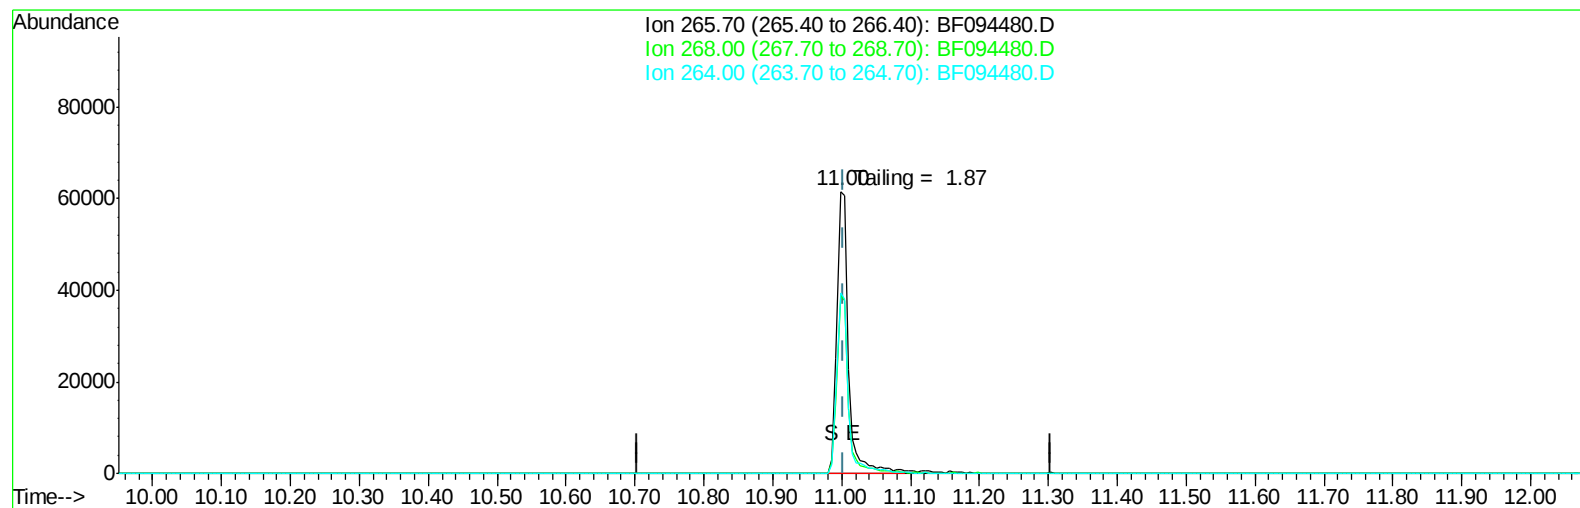

(69) Pentachlorophenol (C)

10.998min (-0.006) 0.00ng

response 70075

Ion	Exp%	Act%
265.70	100	100
268.00	63.90	63.14
264.00	64.60	64.01
0.00	0.00	0.00