


Data Path : Z:\HPCHEM1\BNA F\Data\BF041817\
 Data File : BF094480.D
 Acq On : 18 Apr 2017 11:58
 Operator : SJ/MA
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF041717.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Mon Apr 17 14:59:23 2017

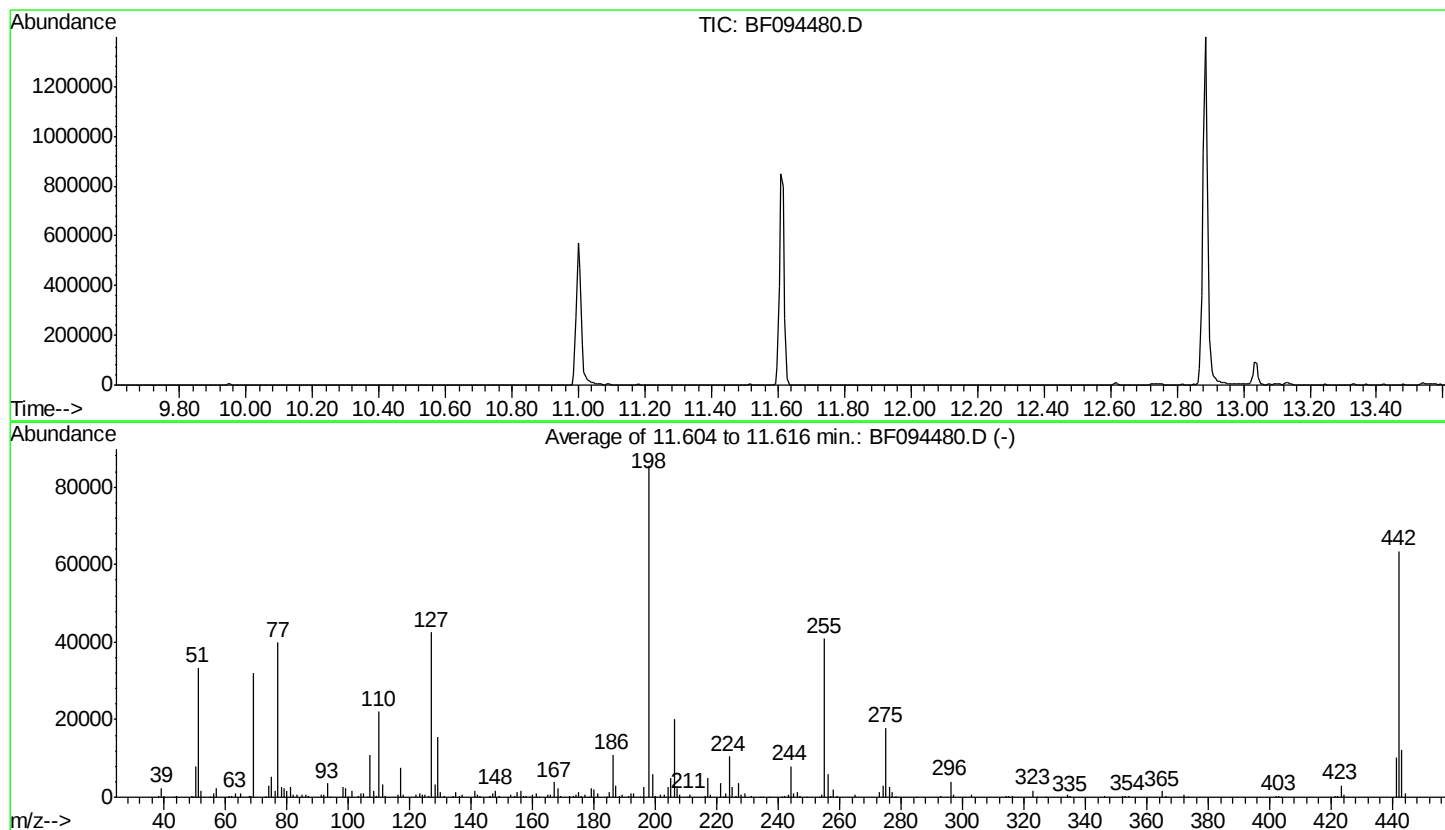

AutoFind: Scans 1686, 1687, 1688; Background Corrected with Scan 1681

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	39.1	33424	PASS
68	69	0.00	2	1.2	383	PASS
69	198	0.00	100	37.3	31917	PASS
70	69	0.00	2	0.0	0	PASS
127	198	10	80	49.7	42496	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	85514	PASS
199	198	5	9	6.8	5855	PASS
275	198	10	60	21.0	17946	PASS
365	198	1	100	1.9	1650	PASS
441	442	0.01	24	15.9	10081	PASS
442	198	50	100	74.3	63544	PASS
443	442	15	24	19.0	12077	PASS