
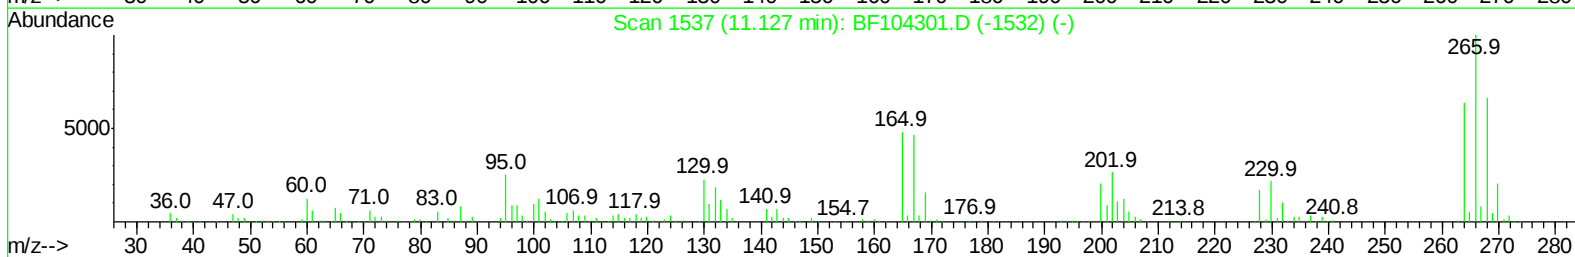
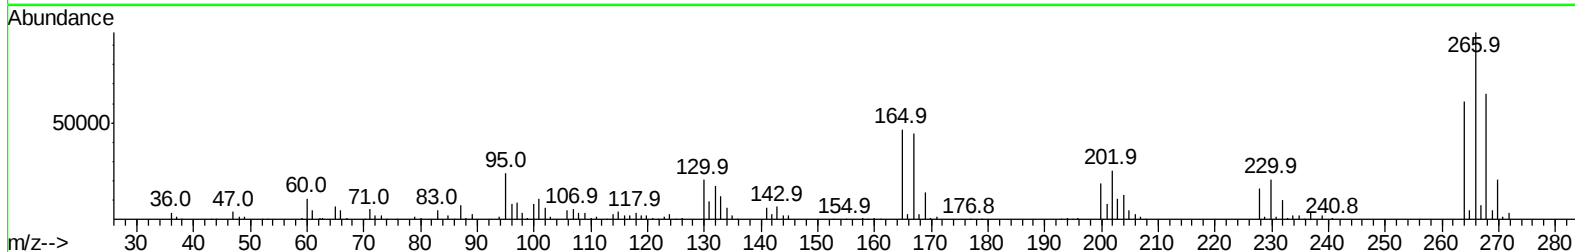


Data Path : Z:\HPCHEM1\BNA F\DATA\BF041818\
Data File : BF104587.D
Acq On : 18 Apr 2018 8:49
Operator : JU/SJ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Apr 19 02:21:35 2018
Quant Method : Z:\HPCHEM1\BNA F\METHODS\8270-BF040618.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Apr 18 11:52:19 2018
Response via : Initial Calibration

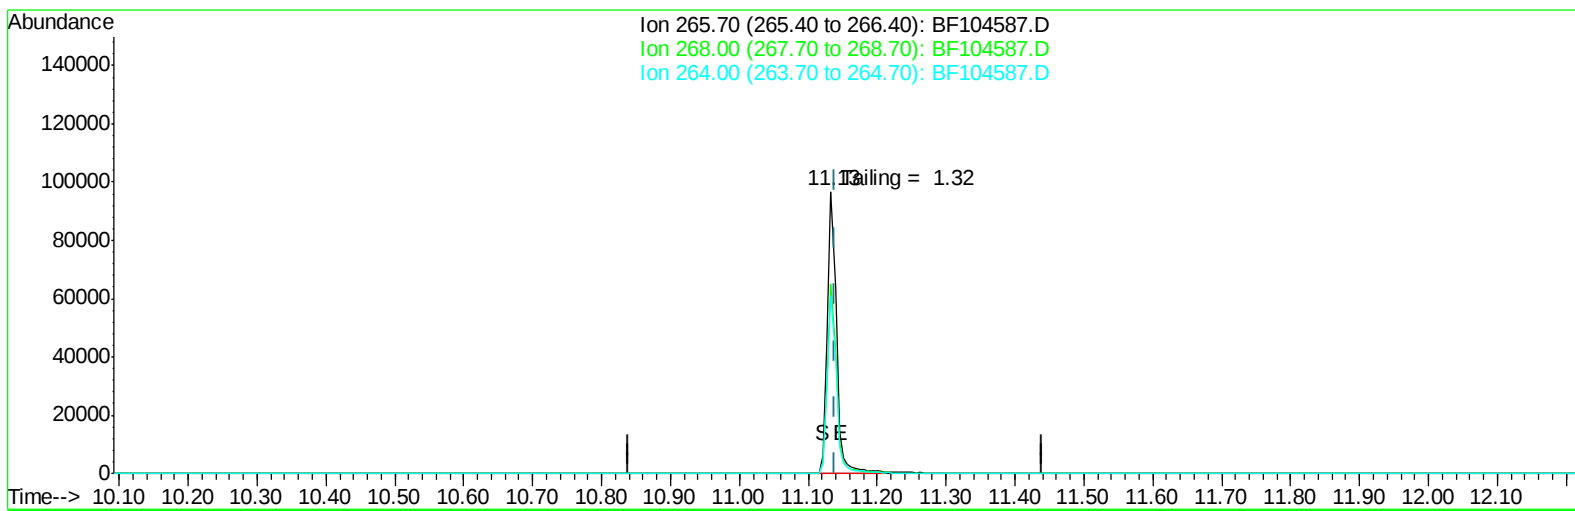

TIC: BF104587.D

(69) Pentachlorophenol (C)




11.133min (-0.006) 28220.88ng

response 86509

Ion	Exp%	Act%
265.70	100	100
268.00	63.90	67.47
264.00	61.90	63.40
0.00	0.00	0.00

Data Path : Z:\HPCHEM1\BNA F\DATA\BF041818\
 Data File : BF104587.D
 Acq On : 18 Apr 2018 8:49
 Operator : JU/SJ
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Quant Time: Apr 19 02:21:35 2018
 Quant Method : Z:\HPCHEM1\BNA F\METHODS\8270-BF040618.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed Apr 18 11:52:19 2018
 Response via : Initial Calibration

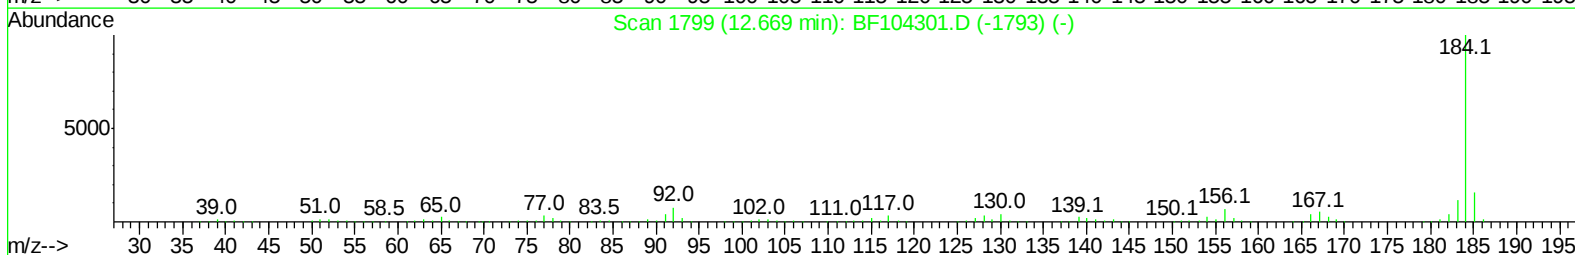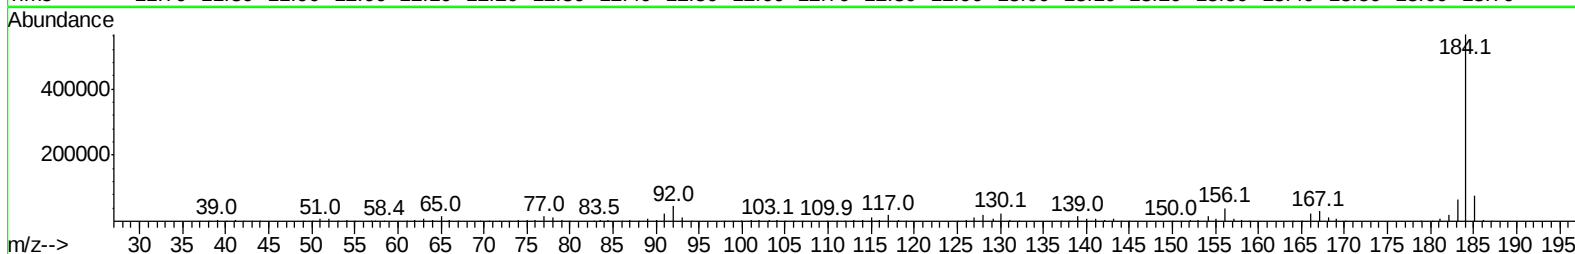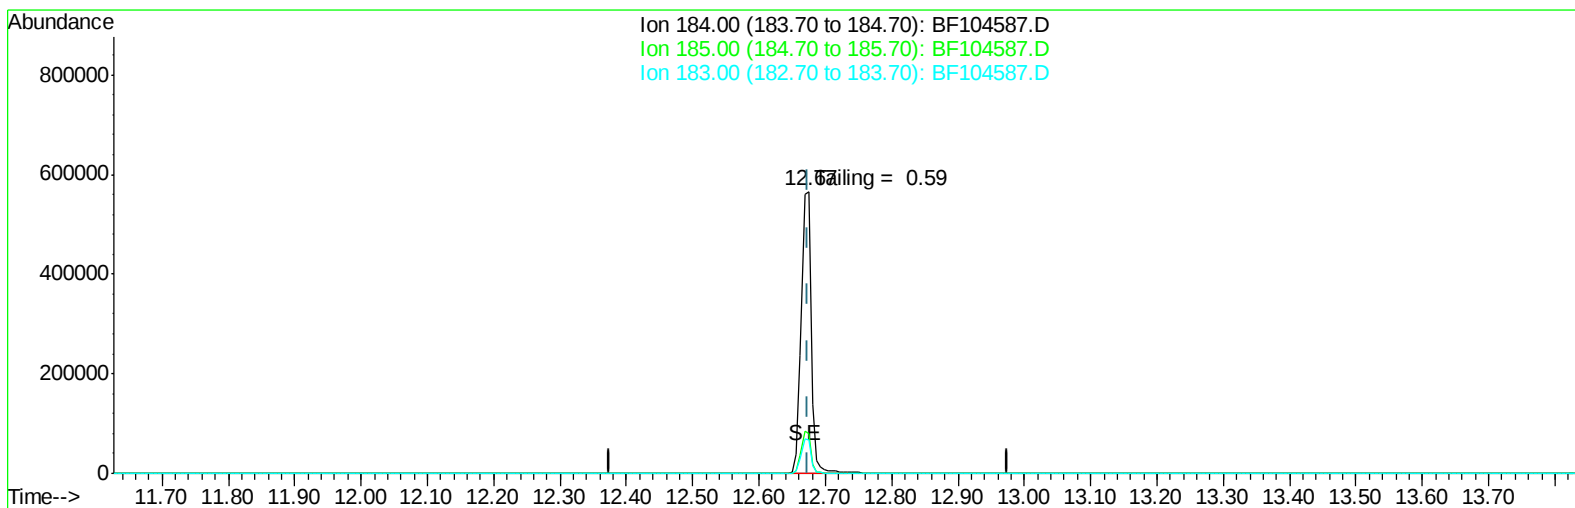

TIC: BF104587.D

(76) Benzidine

12.674min (-0.000) 0.00ng

response 574635

Ion	Exp%	Act%
184.00	100	100
185.00	15.70	14.06
183.00	11.60	12.03
0.00	0.00	0.00