
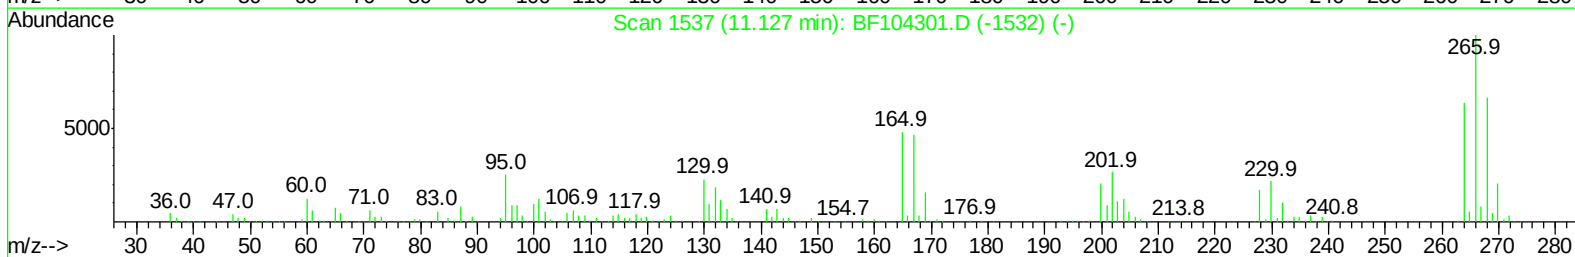
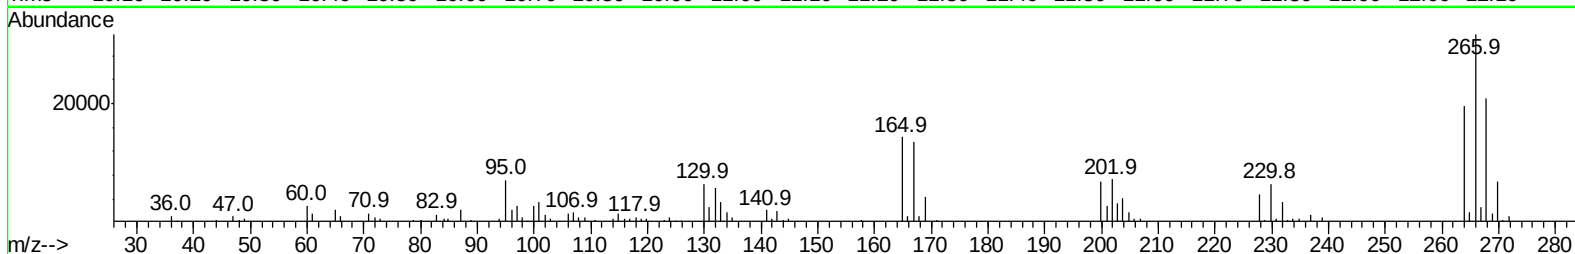


Data Path : Z:\HPCHEM1\BNA F\DATA\BF041818\
Data File : BF104614.D
Acq On : 18 Apr 2018 21:44
Operator : JU/SJ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Apr 19 02:23:33 2018
Quant Method : Z:\HPCHEM1\BNA F\METHODS\8270-BF040618.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Apr 18 11:52:19 2018
Response via : Initial Calibration

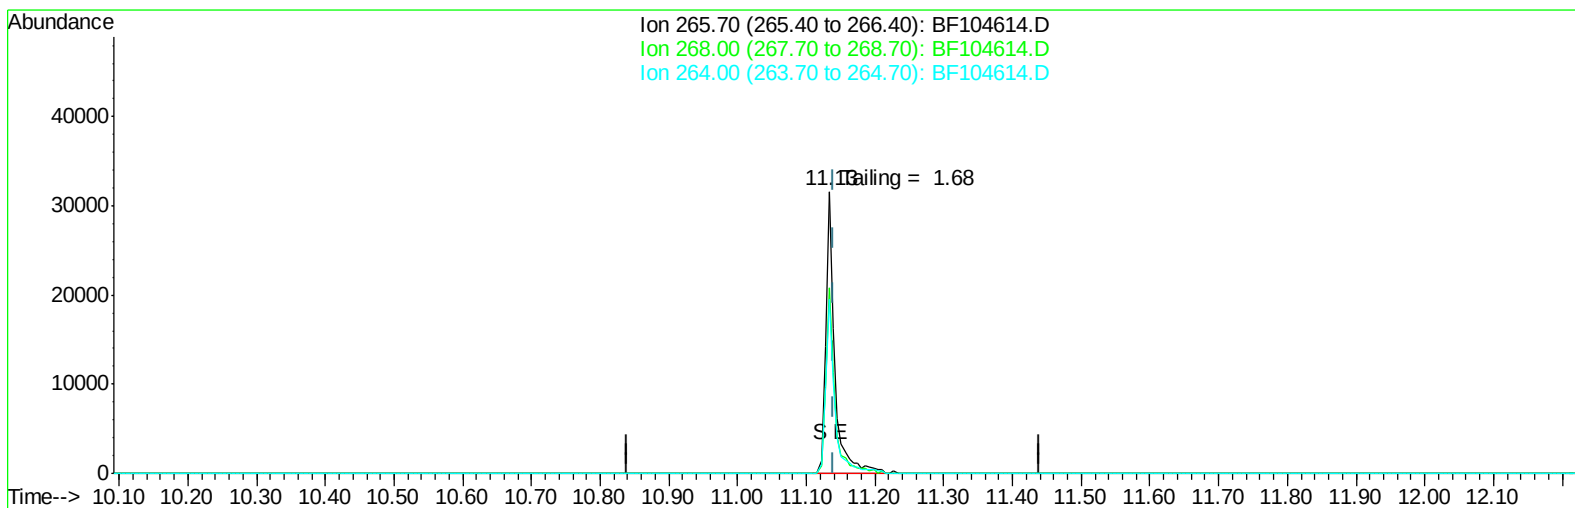

TIC: BF104614.D

(69) Pentachlorophenol (C)




11.133min (-0.006) 0.00ng

response 29103

Ion	Exp%	Act%
265.70	100	100
268.00	63.90	65.82
264.00	61.90	61.82
0.00	0.00	0.00

Data Path : Z:\HPCHEM1\BNA F\DATA\BF041818\
Data File : BF104614.D
Acq On : 18 Apr 2018 21:44
Operator : JU/SJ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Apr 19 02:23:33 2018
Quant Method : Z:\HPCHEM1\BNA F\METHODS\8270-BF040618.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Apr 18 11:52:19 2018
Response via : Initial Calibration

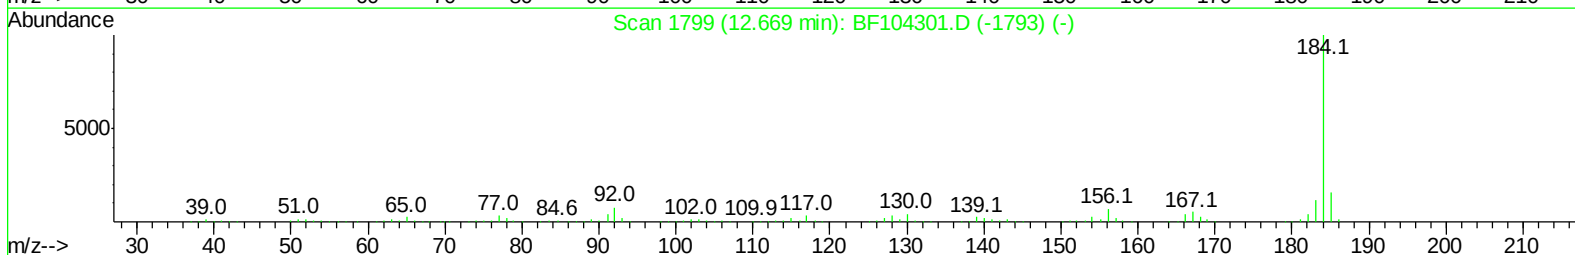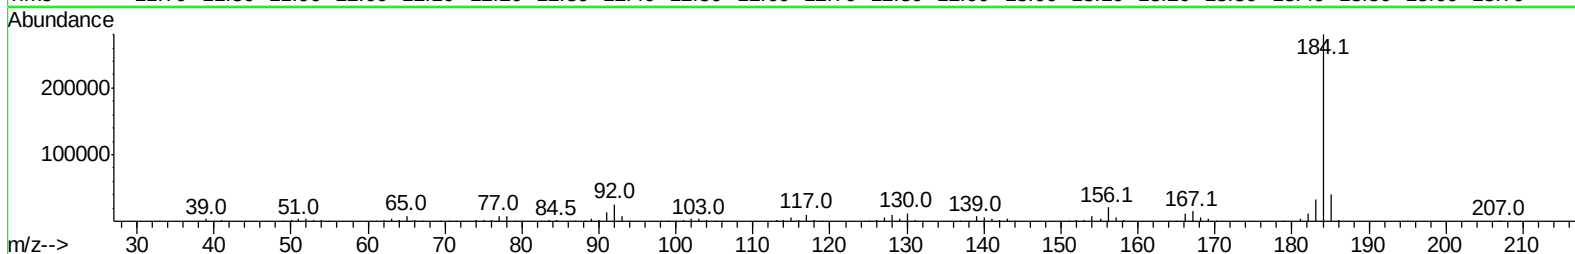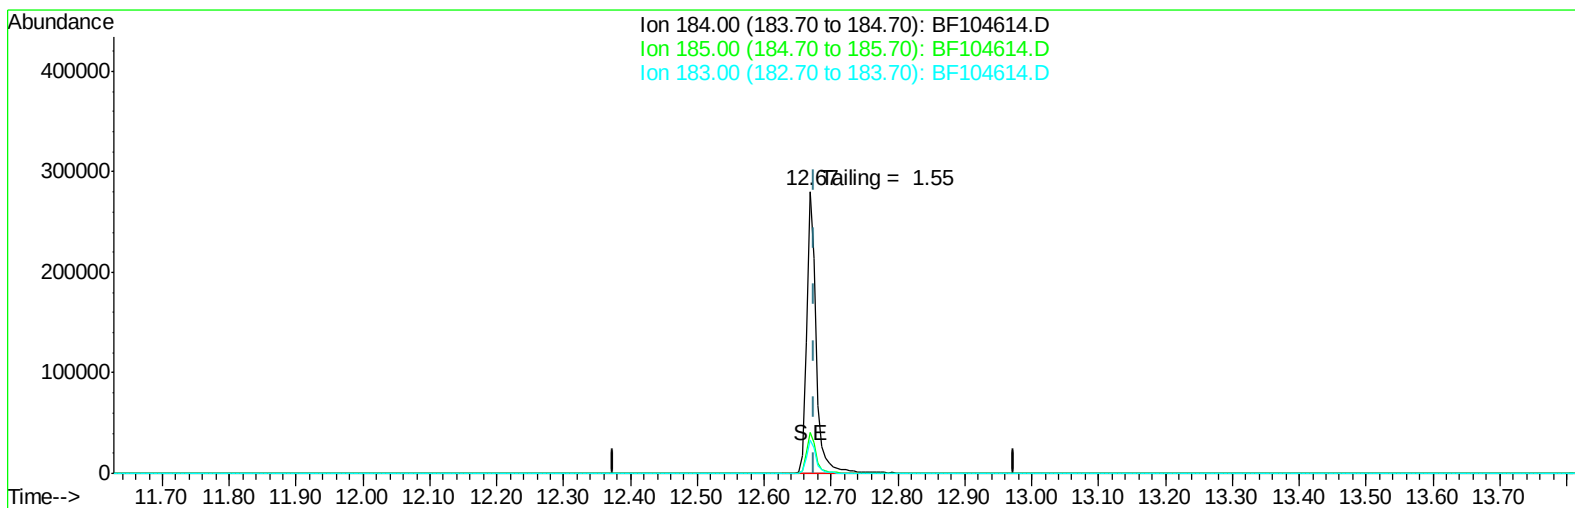

TIC: BF104614.D

(76) Benzidine

12.668min (-0.006) -20.00ng

response 282451

Ion	Exp%	Act%
184.00	100	100
185.00	15.70	14.77
183.00	11.60	11.71
0.00	0.00	0.00