


Data Path : Z:\HPCHEM1\BNA F\Data\BF041818\
 Data File : BF104614.D
 Acq On : 18 Apr 2018 21:44
 Operator : JU/SJ
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF040618.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Wed Apr 18 11:52:19 2018

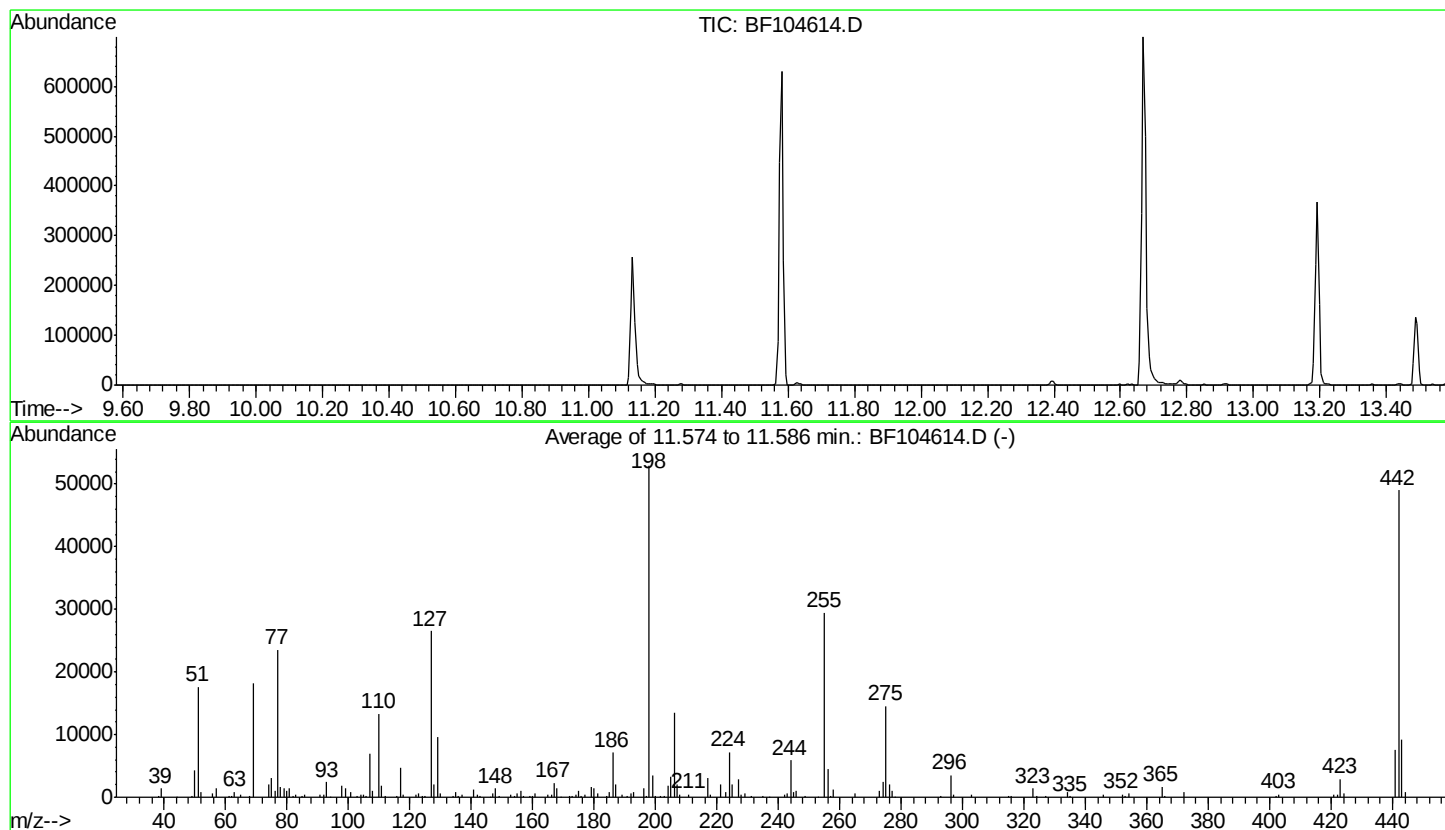

AutoFind: Scans 1613, 1614, 1615; Background Corrected with Scan 1608

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	33.3	17661	PASS
68	69	0.00	2	1.0	183	PASS
69	198	0.00	100	34.3	18157	PASS
70	69	0.00	2	0.0	0	PASS
127	198	10	80	50.0	26488	PASS
197	198	0.00	2	0.4	202	PASS
198	198	100	100	100.0	52965	PASS
199	198	5	9	6.4	3406	PASS
275	198	10	60	27.5	14550	PASS
365	198	1	100	3.1	1657	PASS
441	443	0.01	100	81.0	7505	PASS
442	198	50	100	92.6	49040	PASS
443	442	15	24	18.9	9269	PASS