

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF041822\
 Data File : BF127820.D
 Acq On : 18 Apr 2022 11:01
 Operator : CG\JU
 Sample : PB144160BL
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 PB144160BL

Integration Parameters: rteint.p
 Integrator: RTE
 Smoothing : ON Filtering: 5
 Sampling : 1 Min Area: 3 % of largest Peak
 Start Thrs: 0.2 Max Peaks: 100
 Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF040622.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC: BF127820.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	5.222	494	499	513	rBV	272471	422616	6.23%	1.021%
2	5.593	556	562	565	rBV	4538117	5270882	77.73%	12.729%
3	6.581	723	730	733	rBV	4007164	5307907	78.28%	12.819%
4	6.951	789	793	796	rVB	1274457	1172913	17.30%	2.833%
5	7.516	882	889	892	rBV	3216028	3724074	54.92%	8.994%
6	8.234	1005	1011	1014	rBV	1554782	1494876	22.04%	3.610%
7	9.310	1187	1194	1197	rBV	5826937	6551593	96.62%	15.822%
8	9.992	1304	1310	1313	rBV	1973482	1734420	25.58%	4.189%
9	10.786	1437	1445	1448	rBV	4020515	4121428	60.78%	9.953%
10	11.486	1557	1564	1567	rBV	2026194	1795525	26.48%	4.336%
11	12.880	1798	1801	1804	rBV	165701	128227	1.89%	0.310%
12	13.080	1829	1835	1838	rBV	6231886	6781098	100.00%	16.376%
13	13.586	1918	1921	1926	rBV	105555	99528	1.47%	0.240%
14	14.133	2009	2014	2017	rBV	1551426	1502293	22.15%	3.628%
15	15.651	2266	2272	2280	rBV	993733	1300587	19.18%	3.141%




Sum of corrected areas: 41407967

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF041822\
Data File : BF127820.D
Acq On : 18 Apr 2022 11:01
Operator : CG\JU
Sample : PB144160BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PB144160BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF040622.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

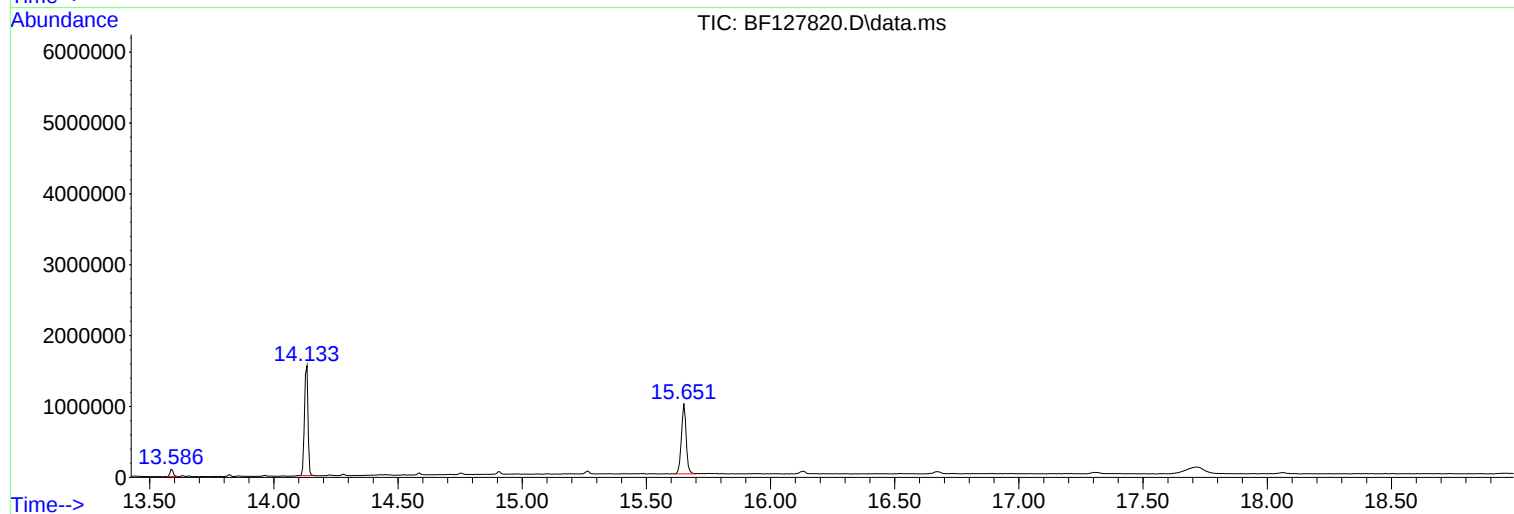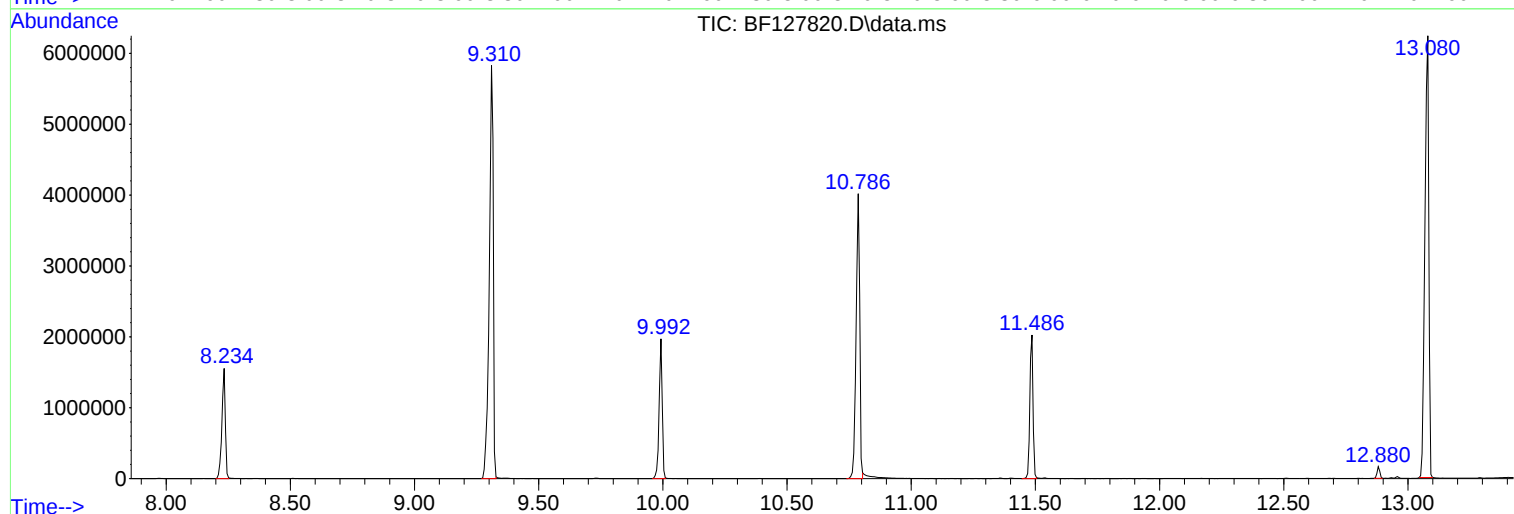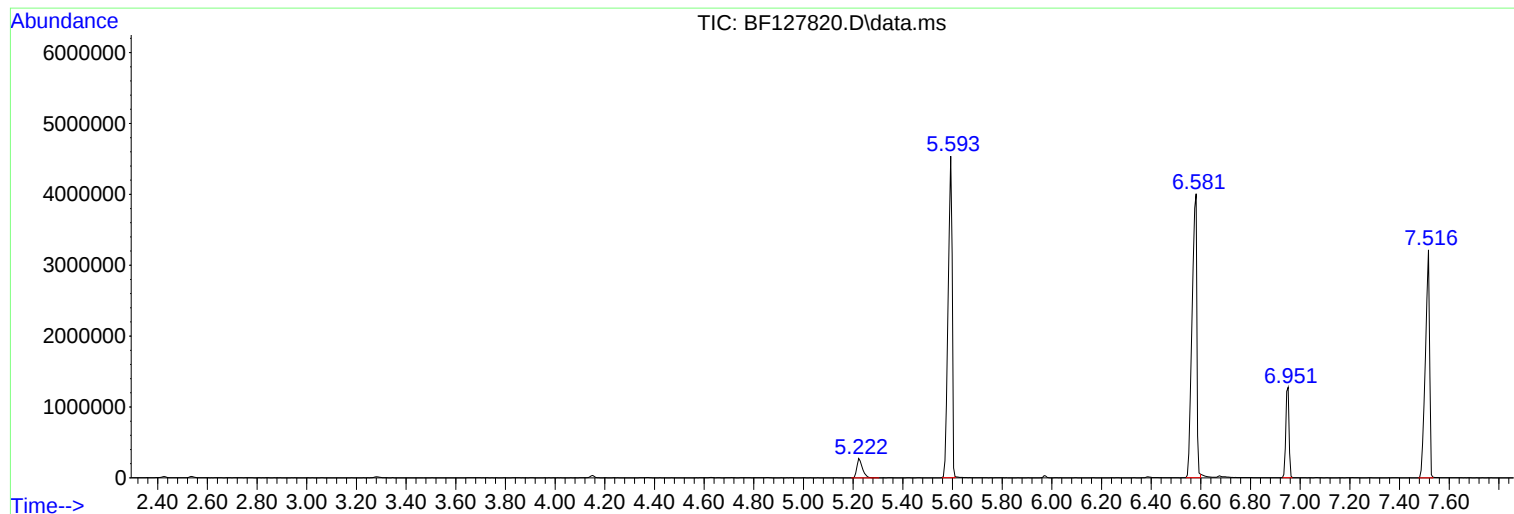

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF041822\
Data File : BF127820.D
Acq On : 18 Apr 2022 11:01
Operator : CG\JU
Sample : PB144160BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PB144160BL










Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF040622.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 2-Pentanone, 4-hydroxy-4-me... Concentration Rank 1

R.T.	EstConc	Area	Relative to ISTD	R.T.
5.222	7.21 ng	422616	1,4-Dichlorobenzene-d4	6.951

Hit#	of	5	Tentative ID	MW	MolForm	CAS#	Qual
1	2-Pentanone, 4-hydroxy-4-methyl-	116	C6H12O2	000123-42-2	45		
2	Acetic acid, cyano-, 1,1-dimethy...	141	C7H11NO2	001116-98-9	25		
3	1-Propen-2-ol, acetate	100	C5H8O2	000108-22-5	12		
4	2,3-Butanedione, monooxime	101	C4H7NO2	000057-71-6	9		
5	Butane, 1-ethoxy-	102	C6H14O	000628-81-9	9		

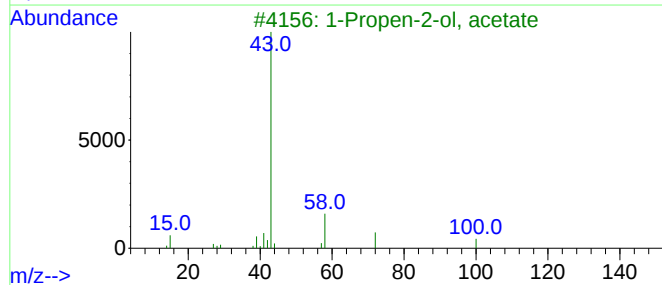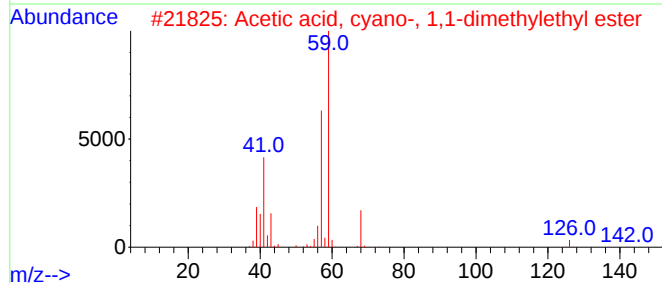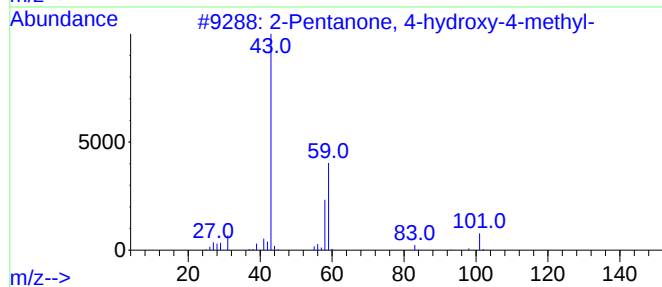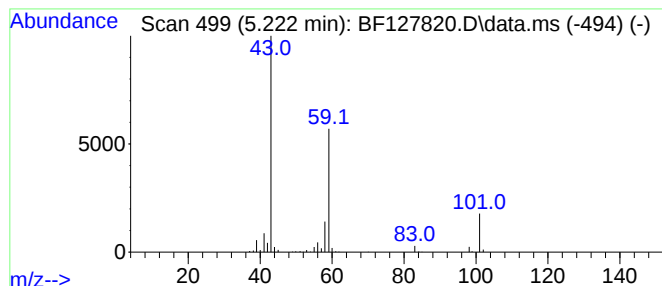

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF041822\
Data File : BF127820.D
Acq On : 18 Apr 2022 11:01
Operator : CG\JU
Sample : PB144160BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PB144160BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF040622.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
2-Pentanone, 4-...	5.222	7.2	ng	422616	1	6.951	1172910	20.0