

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF041822\
 Data File : BF127823.D
 Acq On : 18 Apr 2022 14:06
 Operator : CG\JU
 Sample : PB144168BL
 Misc :
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 PB144168BL

Integration Parameters: rteint.p
 Integrator: RTE
 Smoothing : ON Filtering: 5
 Sampling : 1 Min Area: 3 % of largest Peak
 Start Thrs: 0.2 Max Peaks: 100
 Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF040622.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC: BF127823.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	5.587	555	561	564	rBV	4232376	5035277	77.15%	12.773%
2	6.575	722	729	732	rBV	3959794	5112986	78.34%	12.970%
3	6.945	788	792	796	rBV	1240407	1153274	17.67%	2.926%
4	7.516	882	889	892	rBV	3061187	3511498	53.80%	8.908%
5	8.234	1005	1011	1014	rBV	1508399	1457606	22.33%	3.698%
6	9.310	1187	1194	1197	rBV	5743694	6236766	95.56%	15.821%
7	9.992	1303	1310	1313	rBV	1886380	1689020	25.88%	4.285%
8	10.786	1438	1445	1448	rBV	3770946	3887019	59.55%	9.860%
9	11.486	1556	1564	1567	rBV	1992671	1748458	26.79%	4.435%
10	13.080	1826	1835	1838	rBV	6209442	6526798	100.00%	16.557%
11	14.133	2010	2014	2021	rVB	1725947	1567828	24.02%	3.977%
12	14.204	2023	2026	2034	rBV	170557	217017	3.33%	0.551%
13	15.651	2266	2272	2282	rVB	965857	1277033	19.57%	3.240%




Sum of corrected areas: 39420580

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF041822\
Data File : BF127823.D
Acq On : 18 Apr 2022 14:06
Operator : CG\JU
Sample : PB144168BL
Misc :
ALS Vial : 6 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PB144168BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF040622.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

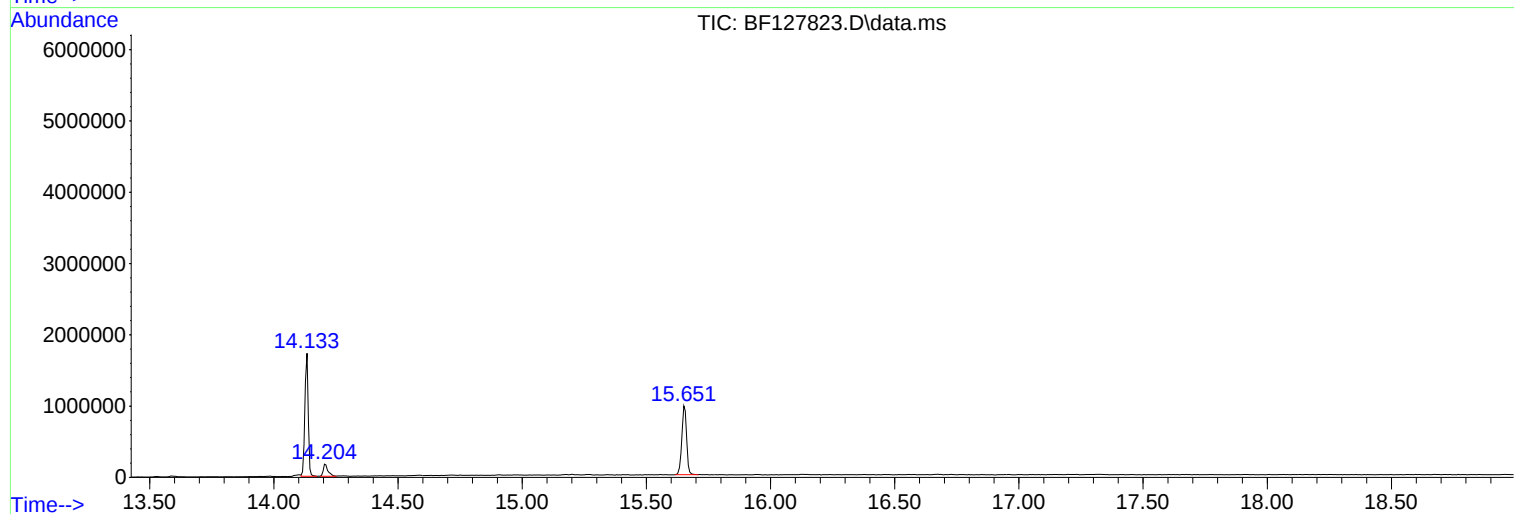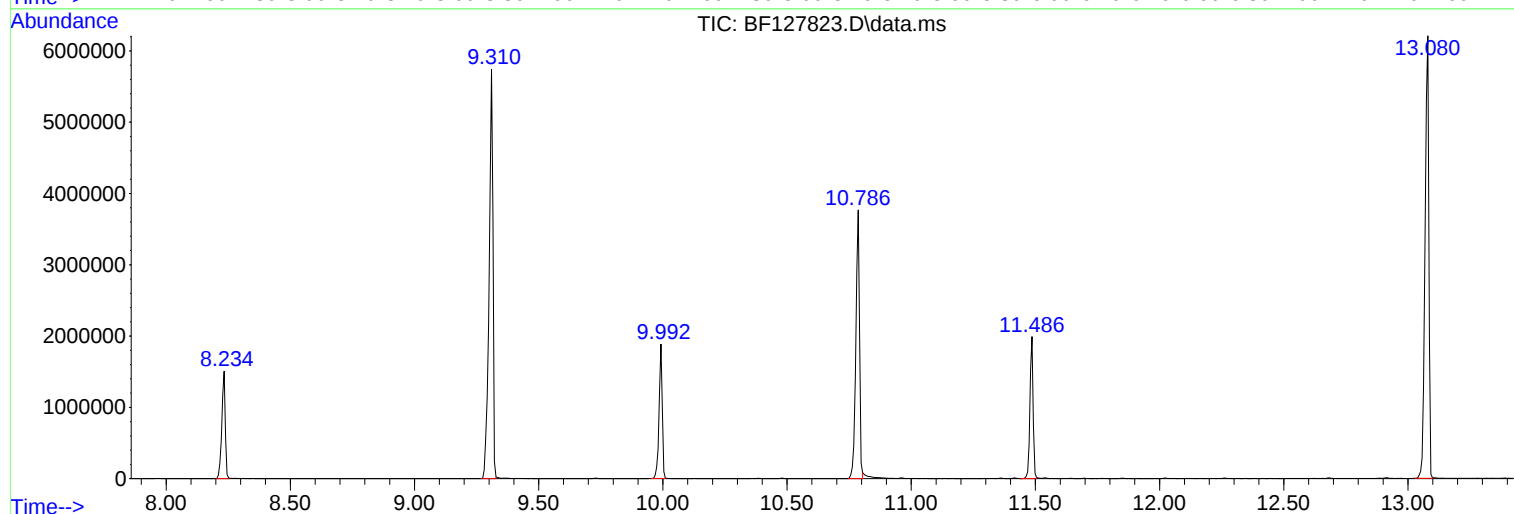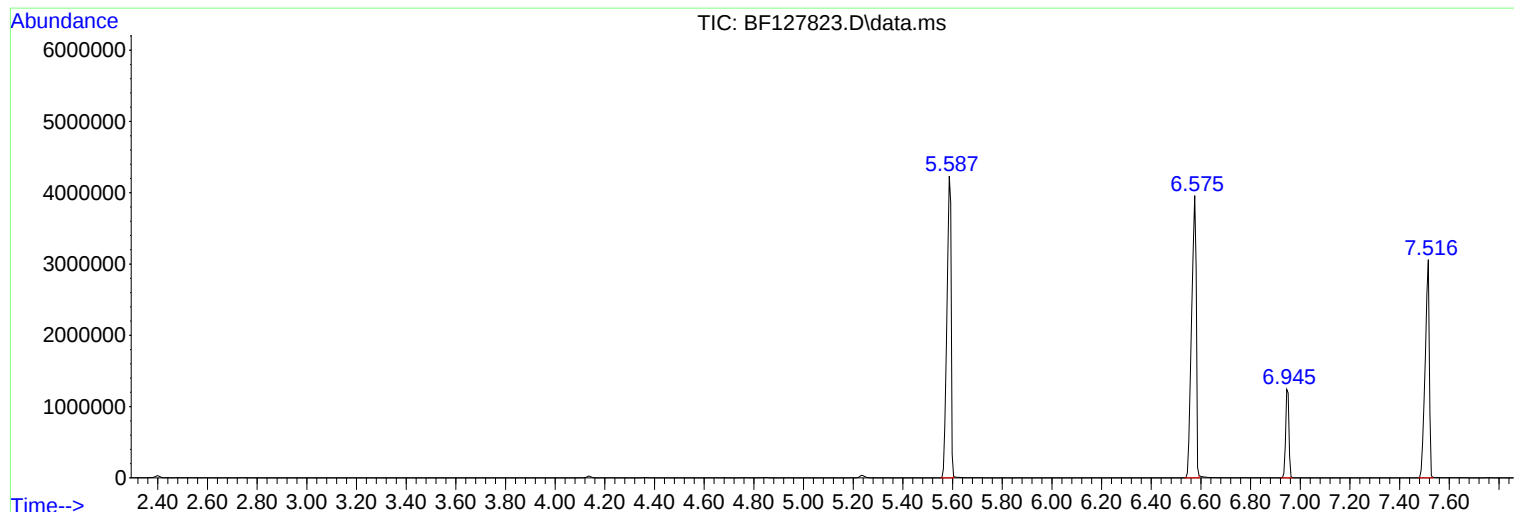

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF041822\
Data File : BF127823.D
Acq On : 18 Apr 2022 14:06
Operator : CG\JU
Sample : PB144168BL
Misc :
ALS Vial : 6 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PB144168BL










Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF040622.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 Triphenylphosphine oxide Concentration Rank 1

R.T.	EstConc	Area	Relative to ISTD	R.T.
14.204	2.77 ng	217017	Chrysene-d12	14.133

Hit#	of	5	Tentative ID	MW	MolForm	CAS#	Qual
1			Triphenylphosphine oxide	278	C18H15OP	000791-28-6	98
2			(E)-7-Benzylidene-1-azabicyclo[3...]	293	C15H19NO3S	1000483-83-4	53
3			Formaldehyde, (triphenylphosphor...	304	C19H17N2P	015990-54-2	45
4			2-Propenoic acid, 2-cyano-3-(3-p...	277	C18H15NO2	1000080-00-3	37
5			Carbazol-1-one, 1,2,3,4-tetrahyd...	277	C18H15NO2	299962-12-2	37

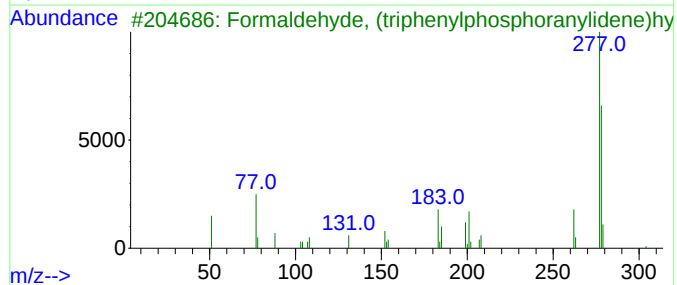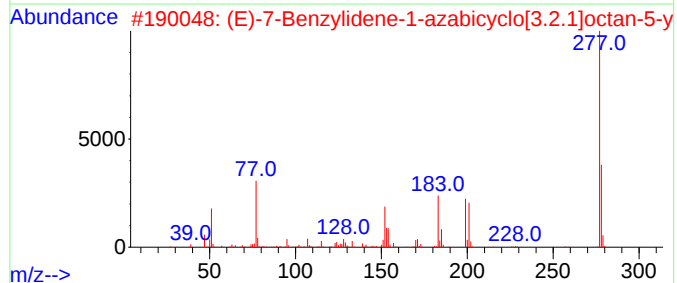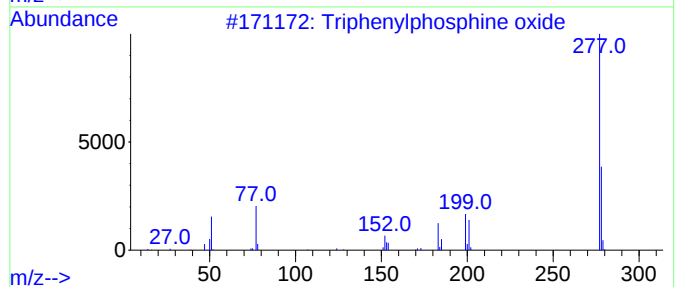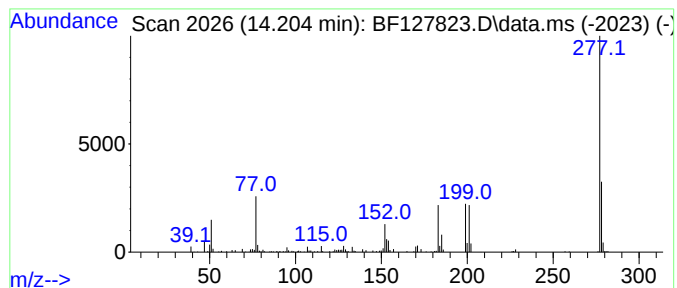

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF041822\
Data File : BF127823.D
Acq On : 18 Apr 2022 14:06
Operator : CG\JU
Sample : PB144168BL
Misc :
ALS Vial : 6 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PB144168BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF040622.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
Triphenylphosph...	14.204	2.8	ng	217017	5	14.133	1567830	20.0