


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF041822\
 Data File : BF127818.D
 Acq On : 18 Apr 2022 10:05
 Operator : CG\JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF040622.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Wed Apr 13 16:40:15 2022

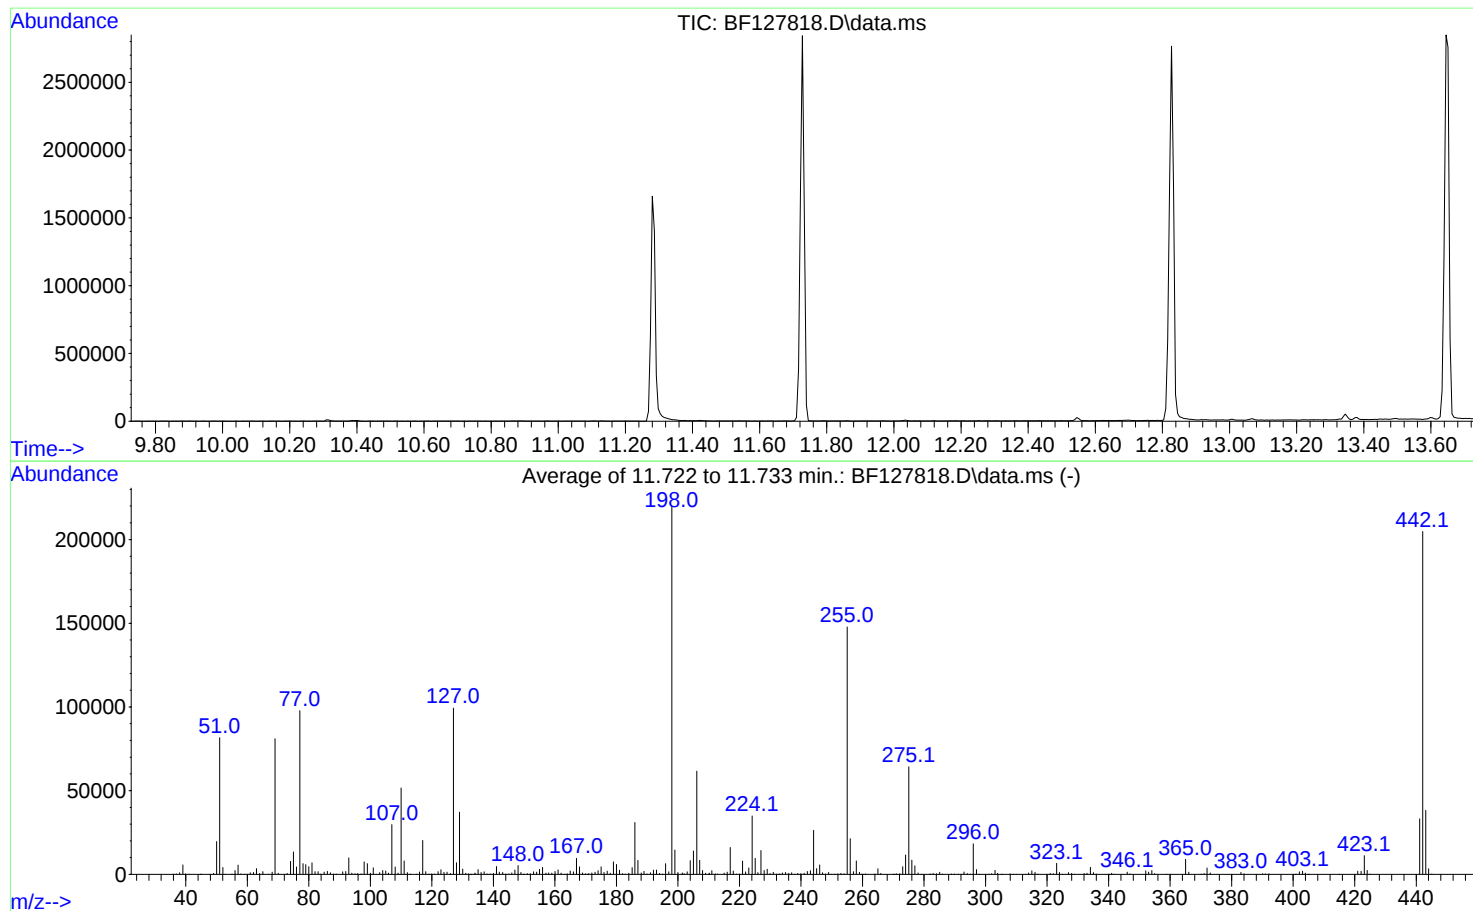




AutoFind: Scans 1604, 1605, 1606; Background Corrected with Scan 1599

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	37.1	81603	PASS
68	69	0.00	2	1.6	1333	PASS
69	198	0.00	100	36.9	81109	PASS
70	69	0.00	2	0.8	655	PASS
127	198	10	80	45.2	99352	PASS
197	198	0.00	2	0.7	1575	PASS
198	198	100	100	100.0	219755	PASS
199	198	5	9	6.6	14513	PASS
275	198	10	60	29.2	64192	PASS
365	198	1	100	4.1	8981	PASS
441	198	0.01	100	15.1	33165	PASS
442	442	50	100	100.0	204861	PASS
443	442	15	24	18.7	38227	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF041822\
Data File : BF127818.D
Acq On : 18 Apr 2022 10:05
Operator : CG\JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Quant Time: Apr 19 07:56:36 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF040622.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Apr 13 16:40:15 2022
Response via : Initial Calibration

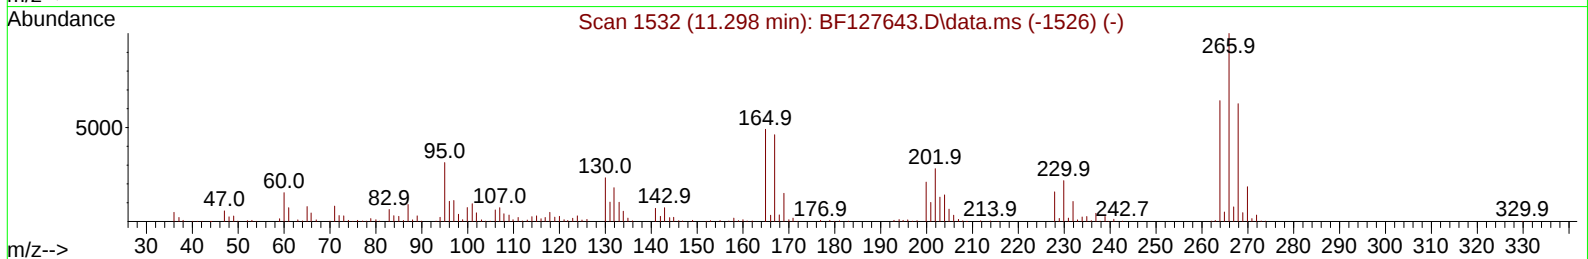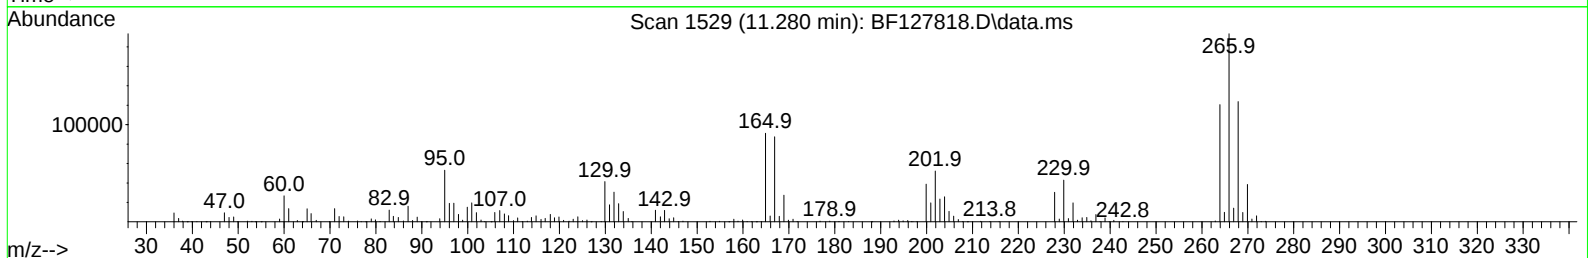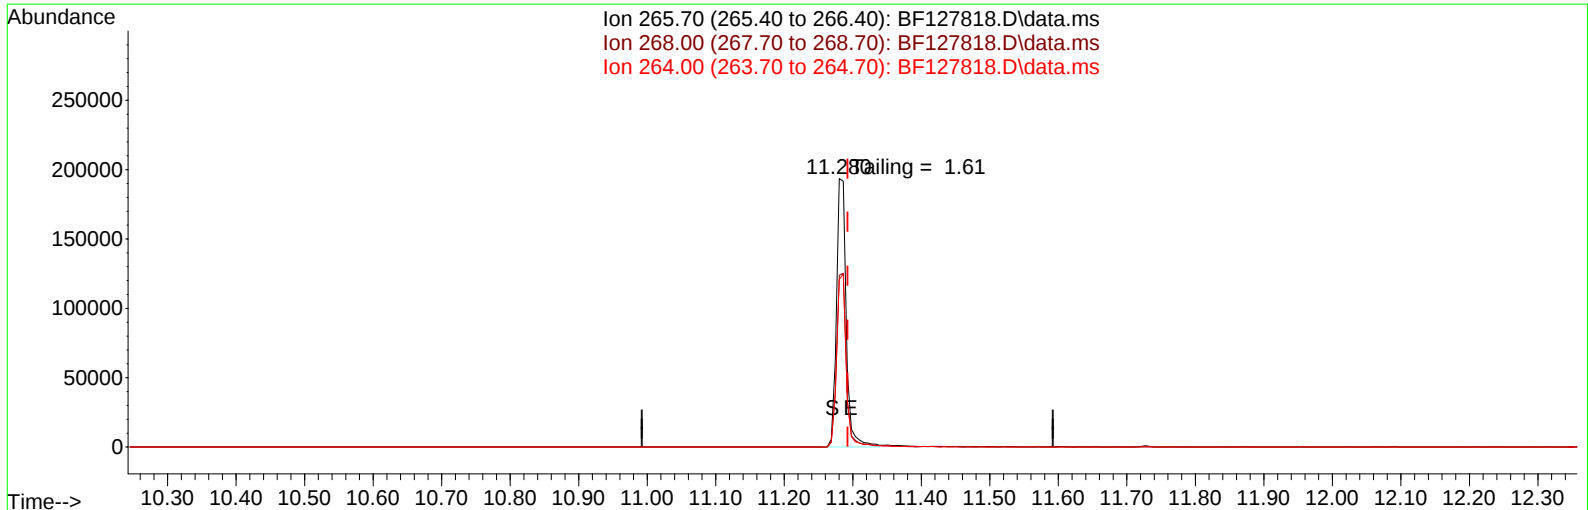

TIC: BF127818.D\data.ms

(70) Pentachlorophenol (C)

11.280min (-0.012) 303892.21 ng




response 192636

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	63.00	63.96
264.00	60.60	62.36
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF041822\
 Data File : BF127818.D
 Acq On : 18 Apr 2022 10:05
 Operator : CG\JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Quant Time: Apr 19 07:56:36 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF040622.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed Apr 13 16:40:15 2022
 Response via : Initial Calibration

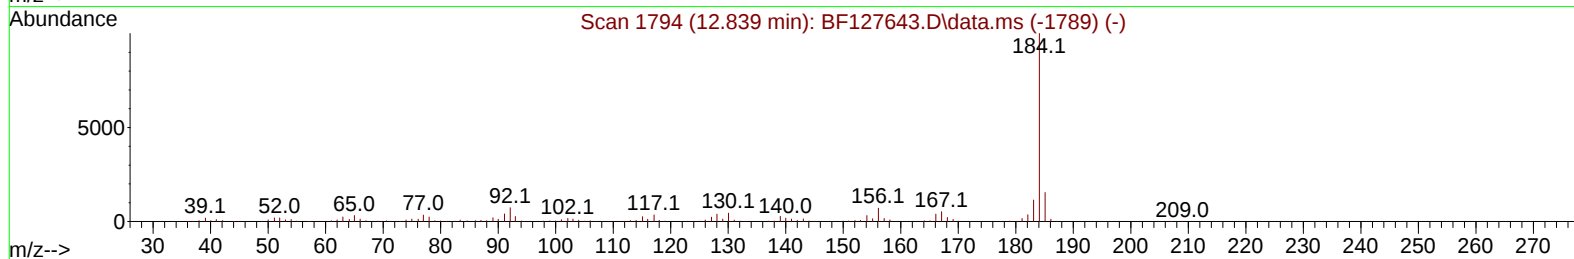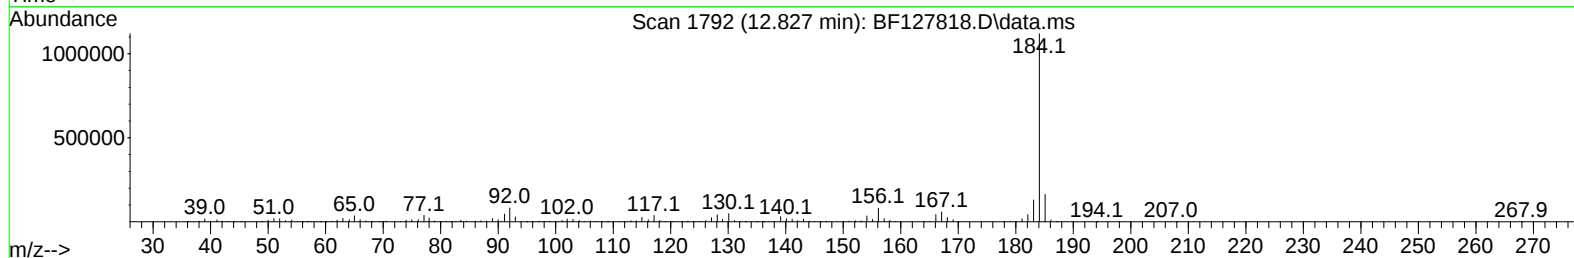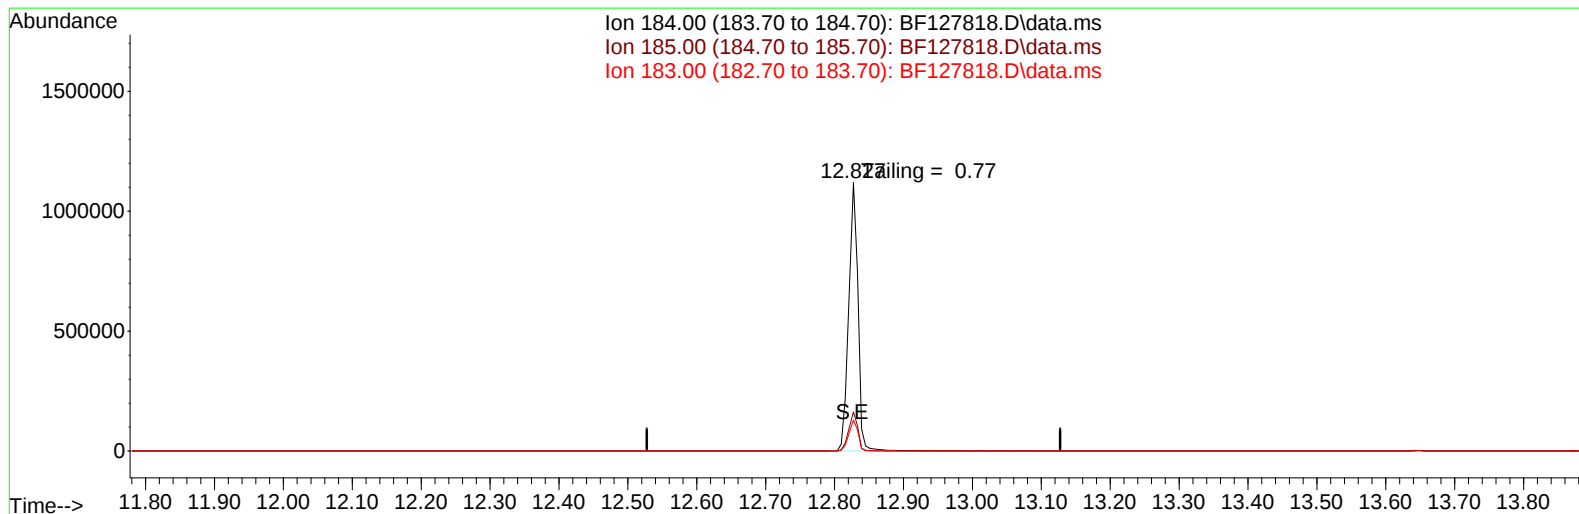

TIC: BF127818.D\data.ms

(77) Benzidine

12.827min (-12.827) 0.00 ng

response 0

Ion	Exp%	Act%
184.00	100.00	0.00
185.00	15.20	0.00#
183.00	11.70	0.00#
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
4/18/2022	BNA_F	<u>BF127818.D</u>
Compound Name	Response	Retention Time
DDT	543970	13.651
DDD	10279	13.345
DDE	931	13.01
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
11210	555180	2.02

Instrument :
BNA_F
ClientSampleId :
DFTPP