
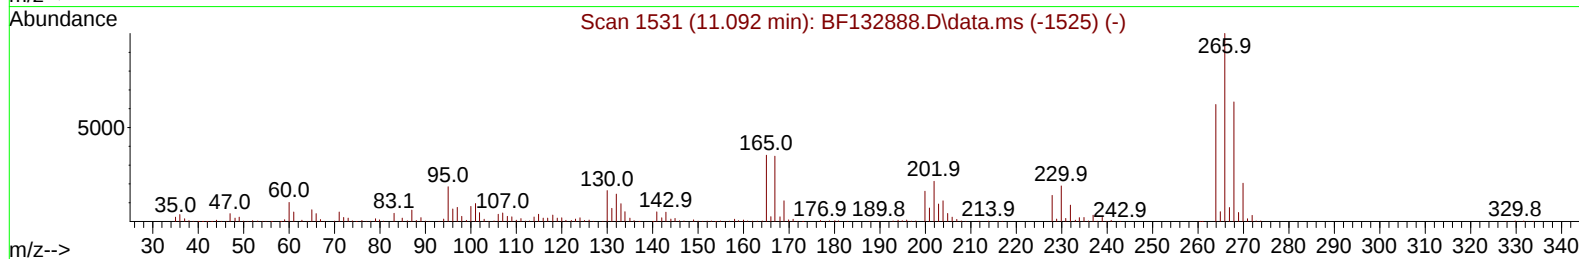
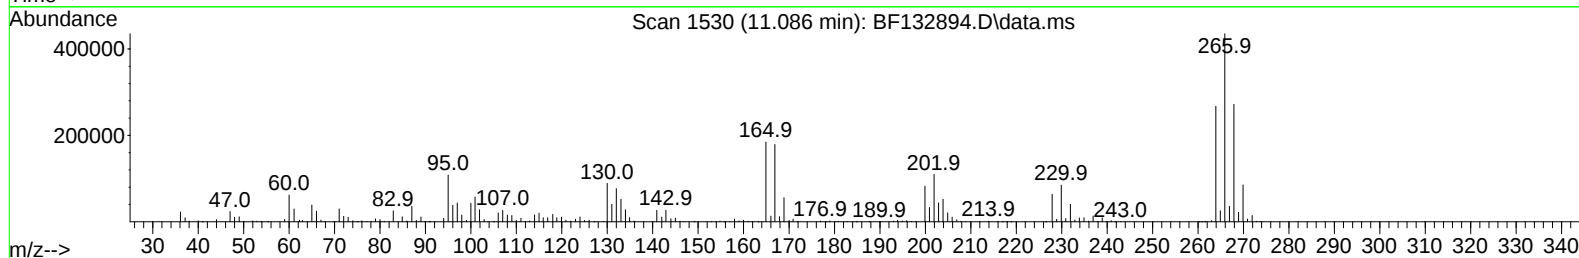


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF041823\
Data File : BF132894.D
Acq On : 18 Apr 2023 09:59
Operator : CG\JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Apr 18 12:05:21 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF041723.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Apr 18 04:51:21 2023
Response via : Initial Calibration

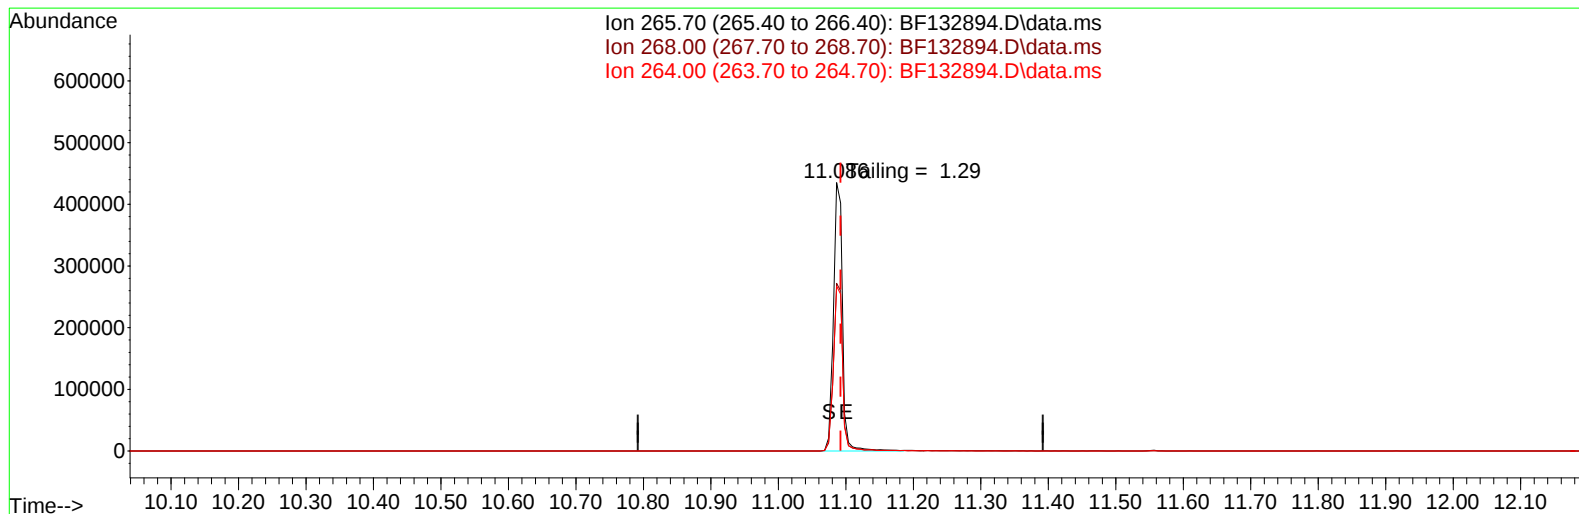

TIC: BF132894.D\data.ms

(70) Pentachlorophenol (C)




11.086min (-0.006) 894217.81 ng

response 403329

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	63.60	62.51
264.00	62.20	61.44
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF041823\
 Data File : BF132894.D
 Acq On : 18 Apr 2023 09:59
 Operator : CG\JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Quant Time: Apr 18 12:05:21 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF041723.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue Apr 18 04:51:21 2023
 Response via : Initial Calibration

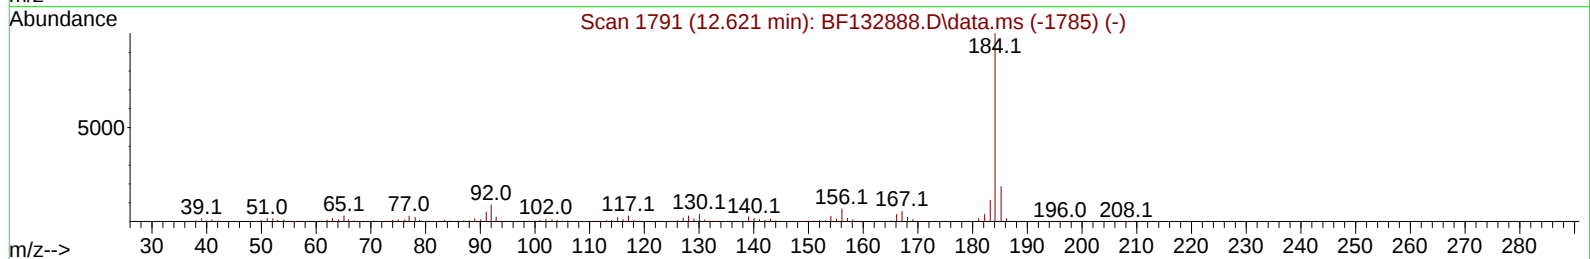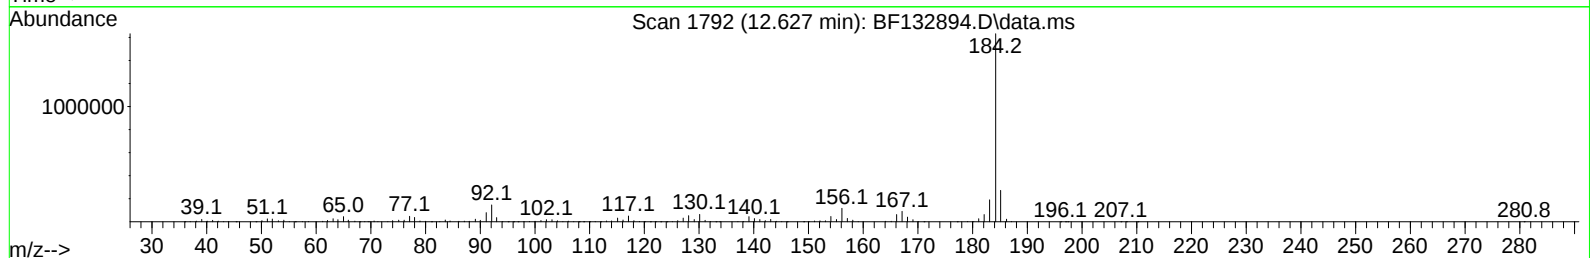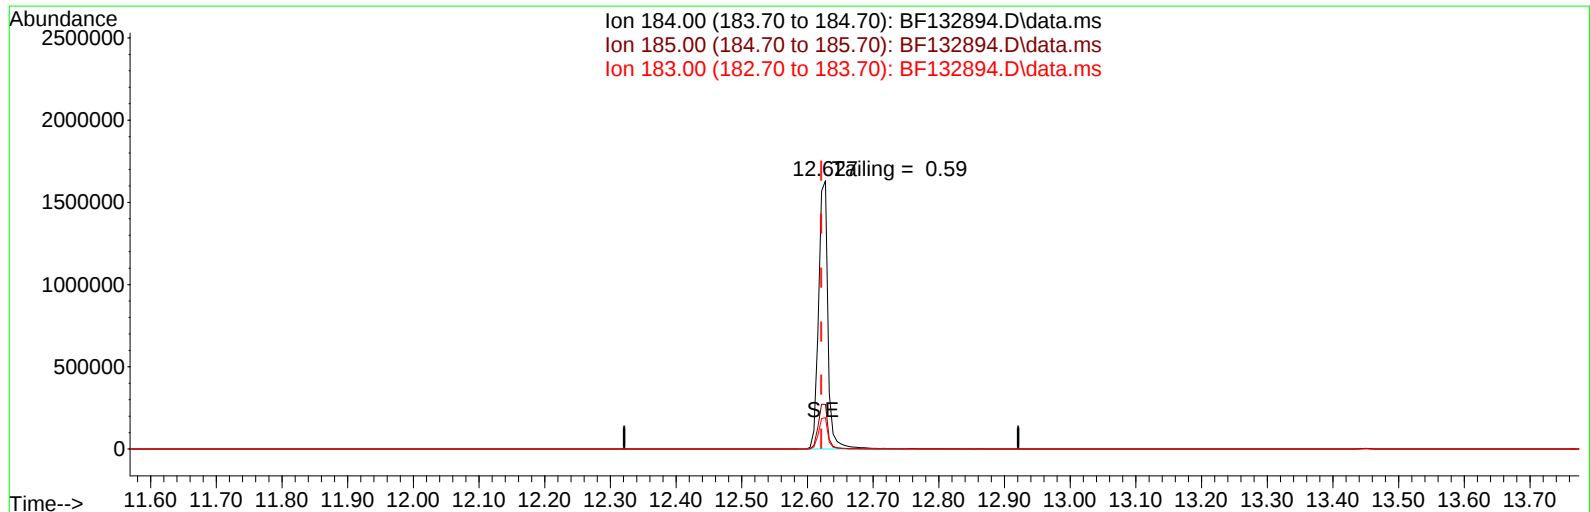

TIC: BF132894.D\data.ms

(77) Benzidine**12.627min (+ 0.006) 294829.78 ng****response 1635015**

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	18.60	16.67
183.00	11.30	11.69
0.00	0.00	0.00