


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF041823\
Data File : BF132894.D
Acq On : 18 Apr 2023 09:59
Operator : CG\JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF041723.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Tue Apr 18 04:51:21 2023

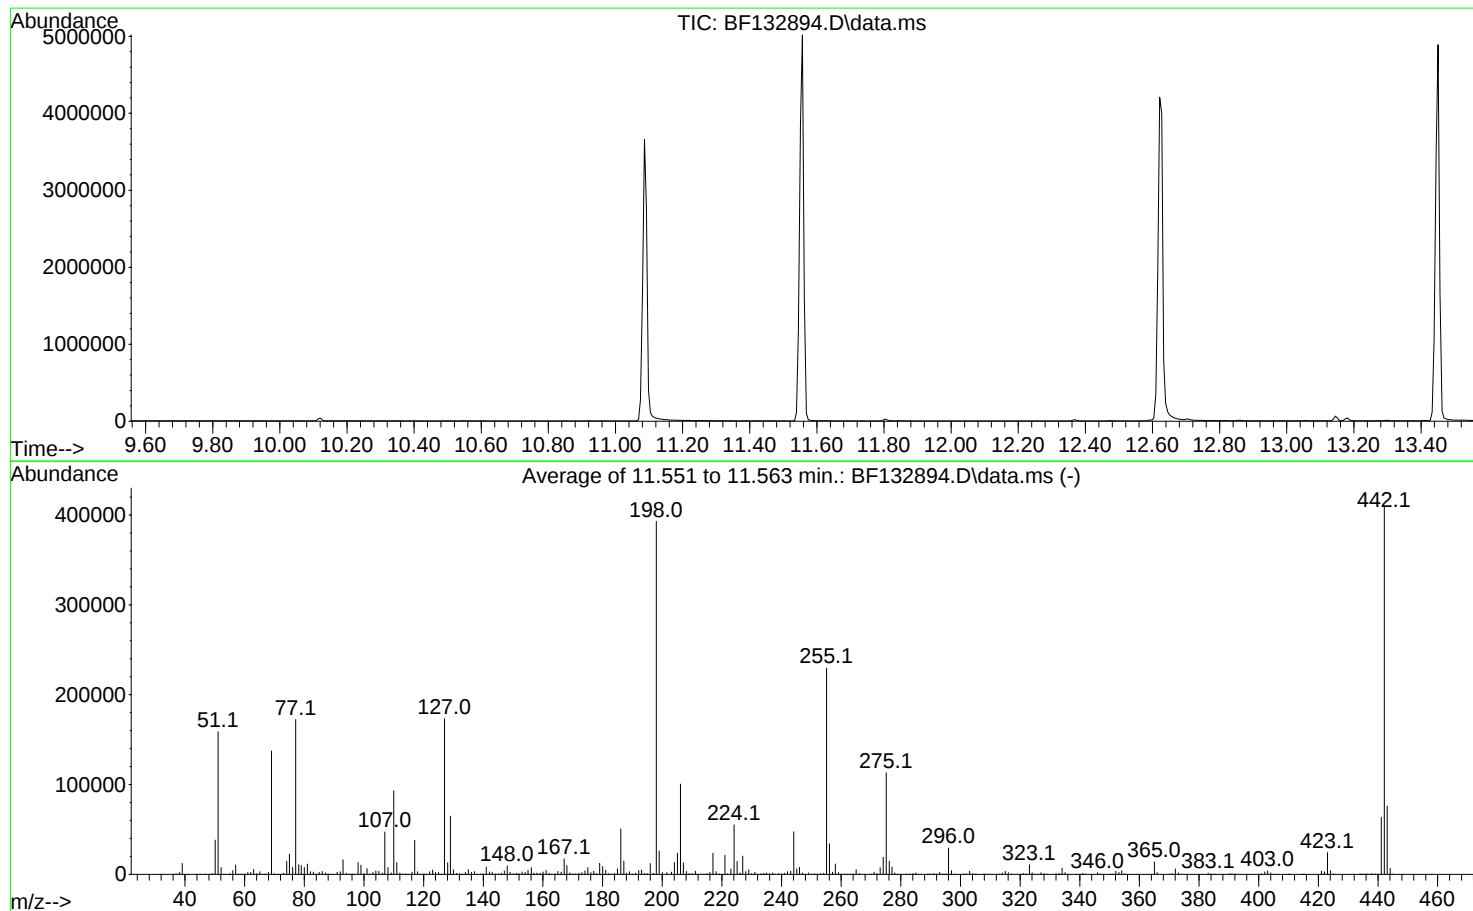




AutoFind: Scans 1609, 1610, 1611; Background Corrected with Scan 1603

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	40.4	158787	PASS
68	69	0.00	2	1.6	2251	PASS
69	198	0.00	100	35.0	137435	PASS
70	69	0.00	2	0.5	751	PASS
127	198	10	80	44.1	173205	PASS
197	198	0.00	2	0.3	1125	PASS
198	198	100	100	100.0	392875	PASS
199	198	5	9	6.6	26032	PASS
275	198	10	60	28.8	113165	PASS
365	198	1	100	3.5	13791	PASS
441	198	0.01	100	16.2	63509	PASS
442	442	50	100	100.0	409515	PASS
443	442	15	24	18.6	76128	PASS

```
Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF041823\  
Data File : BF132894.D  
Acq On    : 18 Apr 2023  09:59  
Operator  : CG\JU  
Sample    : DFTPP  
Misc      :  
ALS Vial  : 1    Sample Multiplier: 1
```

Instrument :
BNA_F
ClientSampleId :
DFTPP

Quant Time: Apr 18 12:05:21 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF041723.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Qlast Update : Tue Apr 18 04:51:21 2023
Response via : Initial Calibration

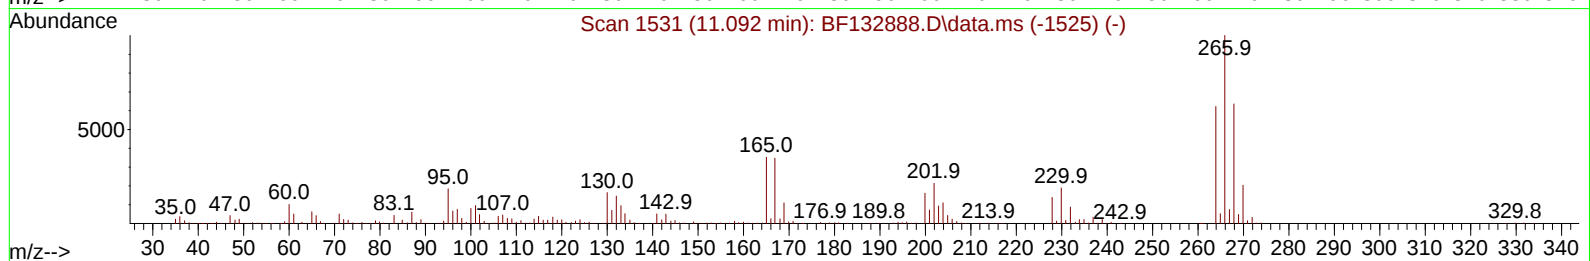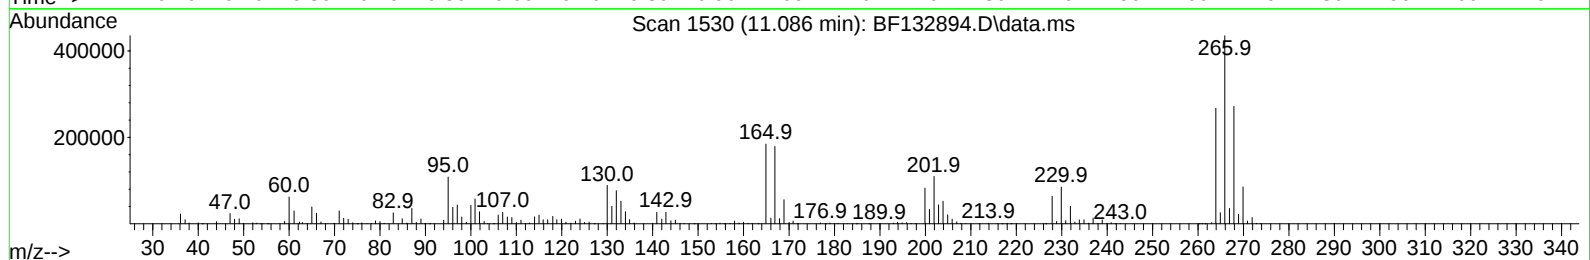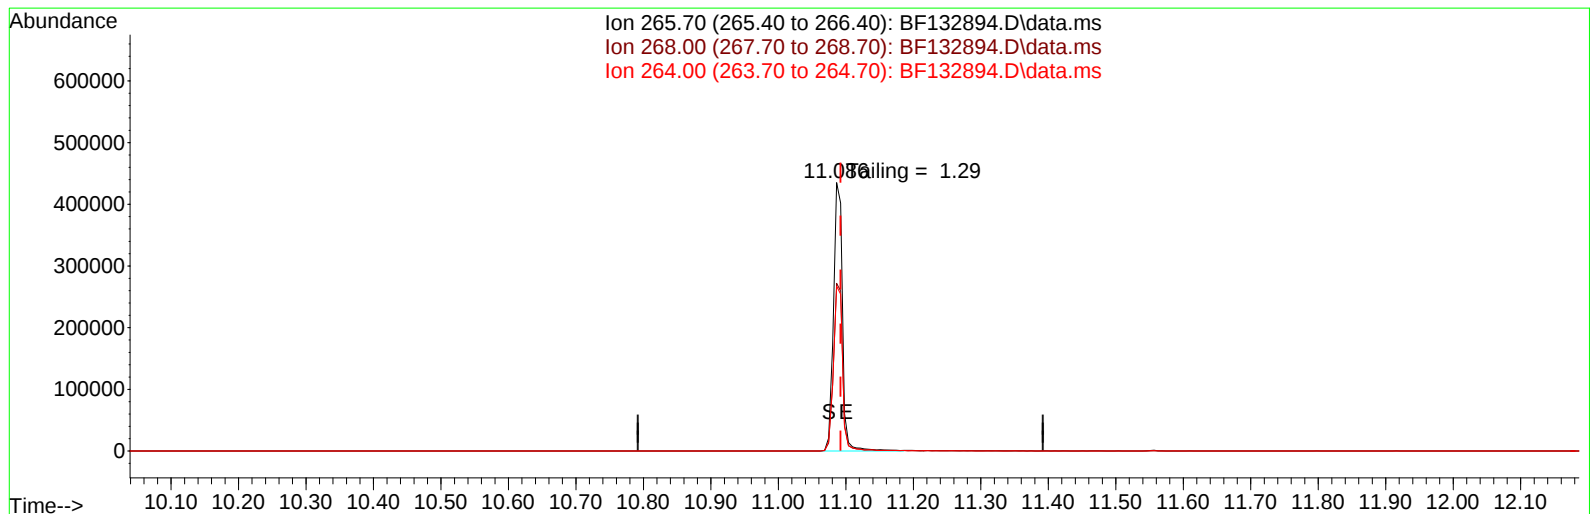

TIC: BF132894.D\data.ms

(70) Pentachlorophenol (C)

11.086min (-0.006) 894217.81 ng




response 403329

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	63.60	62.51
264.00	62.20	61.44
0.00	0.00	0.00

```
Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF041823\  
Data File : BF132894.D  
Acq On    : 18 Apr 2023  09:59  
Operator  : CG\JU  
Sample    : DFTPP  
Misc      :  
ALS Vial  : 1    Sample Multiplier: 1
```

Instrument :
BNA_F
ClientSampleId :
DFTPP

Quant Time: Apr 18 12:05:21 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF041723.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Qlast Update : Tue Apr 18 04:51:21 2023
Response via : Initial Calibration

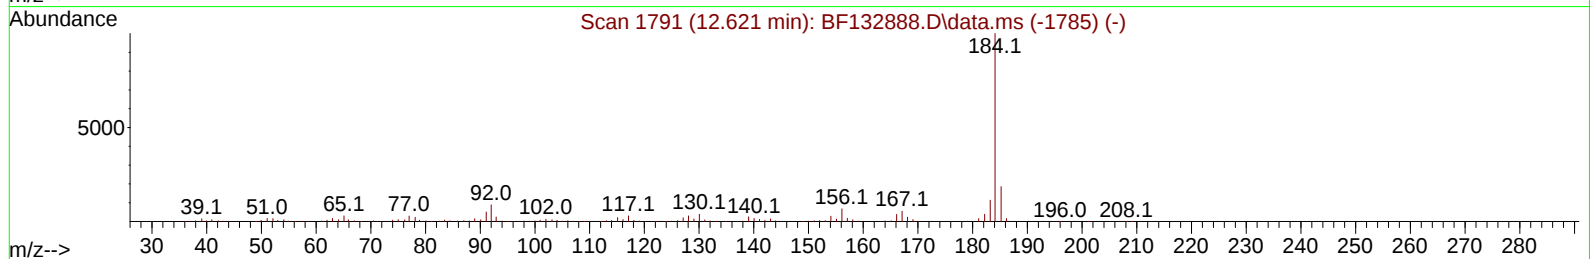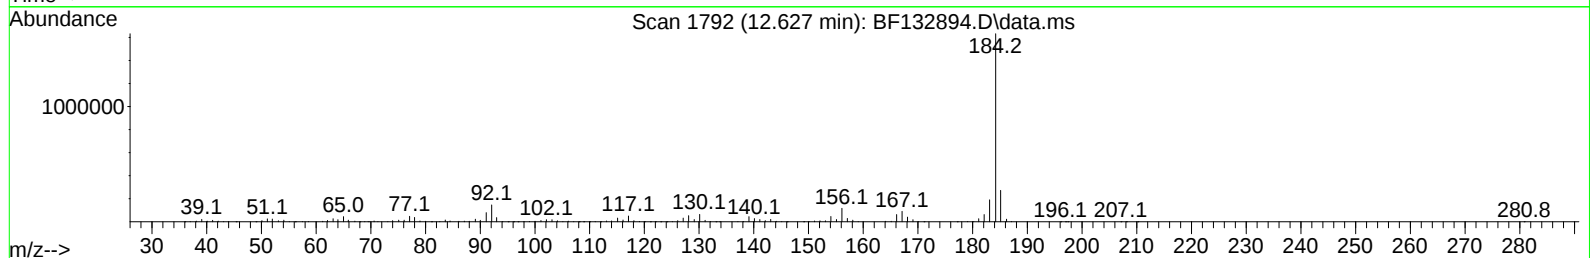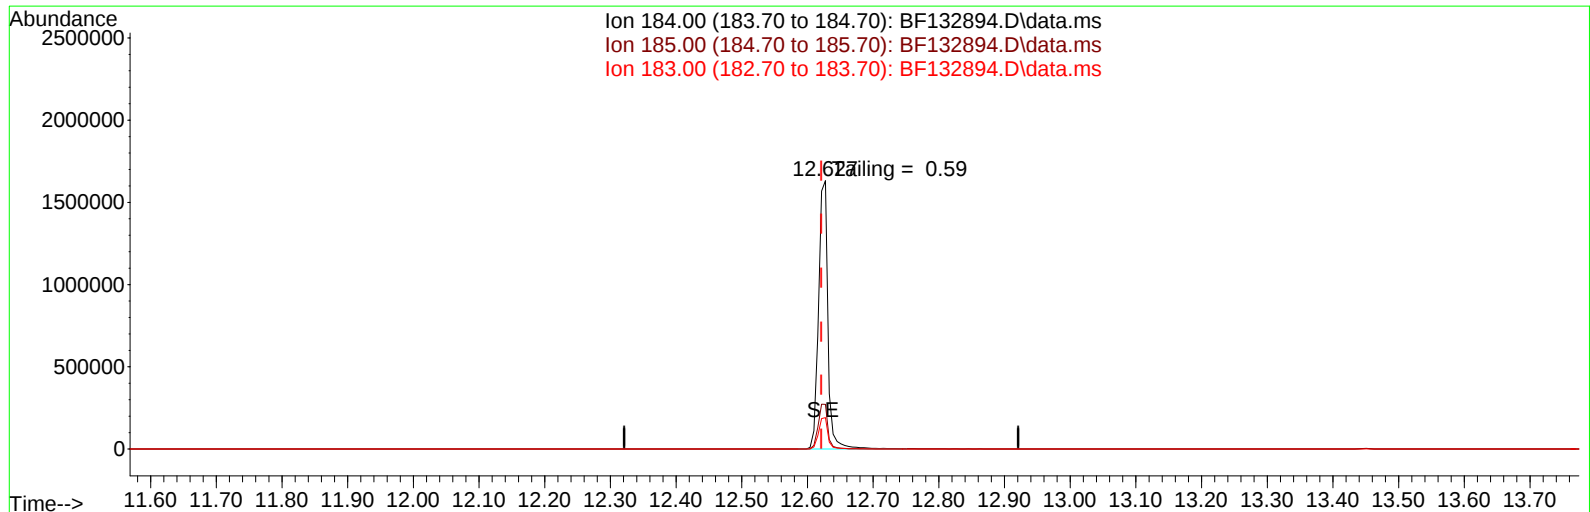

TIC: BF132894.D\data.ms

(77) Benzidine

12.627min (+ 0.006) 294829.78 ng

response **1635015**

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	18.60	16.67
183.00	11.30	11.69
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
4/18/2023	BNA_F	<u>BF132894.D</u>
Compound Name	Response	Retention Time
DDT	679838	13.451
DDD	12395	13.145
DDE	255	12.816
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
12650	692488	1.83

Instrument :
BNA_F
ClientSampleId :
DFTPP