

Data Path : Z:\HPCHEM1\BNA F\DATA\BF041918\
 Data File : BF104635.D
 Acq On : 19 Apr 2018 18:32
 Operator : JU/SJ
 Sample : J2165-05 5X
 Misc :
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :

Quant Time: Apr 20 00:54:49 2018
 Quant Method : Z:\HPCHEM1\BNA F\METHODS\8270-BF040618.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Thu Apr 19 14:44:03 2018
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	6.80	152	129146	20.00	ng	0.00
21) Naphthalene-d8	8.09	136	492228	20.00	ng	0.00
38) Acenaphthene-d10	9.84	164	197509	20.00	ng	-0.01
63) Phenanthrene-d10	11.33	188	306852	20.00	ng	0.00
75) Chrysene-d12	13.98	240	275639	20.00	ng	0.00
86) Perylene-d12	15.44	264	258218	20.00	ng	0.00

System Monitoring Compounds						
5) 2-Fluorophenol	5.41	112	166525	19.72	ng	0.00
7) Phenol-d6	6.43	99	197608	19.04	ng	-0.01
23) Nitrobenzene-d5	7.36	82	110950	14.72	ng	-0.02
41) 2,4,6-Tribromophenol	10.63	330	35794	17.47	ng	0.00
44) 2-Fluorobiphenyl	9.16	172	193885	15.51	ng	-0.01
78) Terphenyl-d14	12.92	244	146912	12.15	ng	0.00


Target Compounds				Qvalue		
9) Benzaldehyde	6.35	77	333	Below Cal	#	1
31) Naphthalene	8.11	128	51992	2.121 ng		97
37) 2-Methylnaphthalene	8.80	142	40637	2.563 ng		98
48) Acenaphthylene	9.70	152	81260	3.952 ng		98
51) Acenaphthene	9.87	154	30854	2.459 ng		98
54) Dibenzofuran	10.05	168	49329	2.821 ng	#	94
57) Fluorene	10.39	166	92458	7.265 ng		99
64) 4,6-Dinitro-2-methylphenol	10.66	198	124	7.417 ng	#	1
70) Phenanthrene	11.36	178	548370	32.090 ng		99
71) Anthracene	11.40	178	166651	9.594 ng		98
72) Carbazole	11.56	167	40322	2.376 ng		99
74) Fluoranthene	12.55	202	749611	41.985 ng		98
76) Benzidine	12.65	184	1347	Below Cal	#	1
77) Pyrene	12.78	202	718200	35.152 ng		100
80) Benzo(a)anthracene	13.97	228	421860	25.619 ng		95
82) Chrysene	14.00	228	343300	20.297 ng		97
85) Indeno(1,2,3-cd)pyrene	16.89	276	140869	9.804 ng		94
87) Benzo(b)fluoranthene	15.02	252	575620	35.295 ng	#	95
88) Benzo(k)fluoranthene	15.02	252	575620	37.386 ng		98
89) Benzo(a)pyrene	15.38	252	299040	20.493 ng	#	95
90) Dibenzo(a,h)anthracene	16.90	278	40759	3.401 ng	#	88
91) Benzo(g,h,i)perylene	17.33	276	132507	11.412 ng		96


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\HPCHEM1\BNA F\DATA\BF041918\
Data File : BF104635.D
Acq On : 19 Apr 2018 18:32
Operator : JU/SJ
Sample : J2165-05 5X
Misc :
ALS Vial : 5 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :

Quant Time: Apr 20 00:54:49 2018
Quant Method : Z:\HPCHEM1\BNA F\METHODS\8270-BF040618.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Apr 19 14:44:03 2018
Response via : Initial Calibration

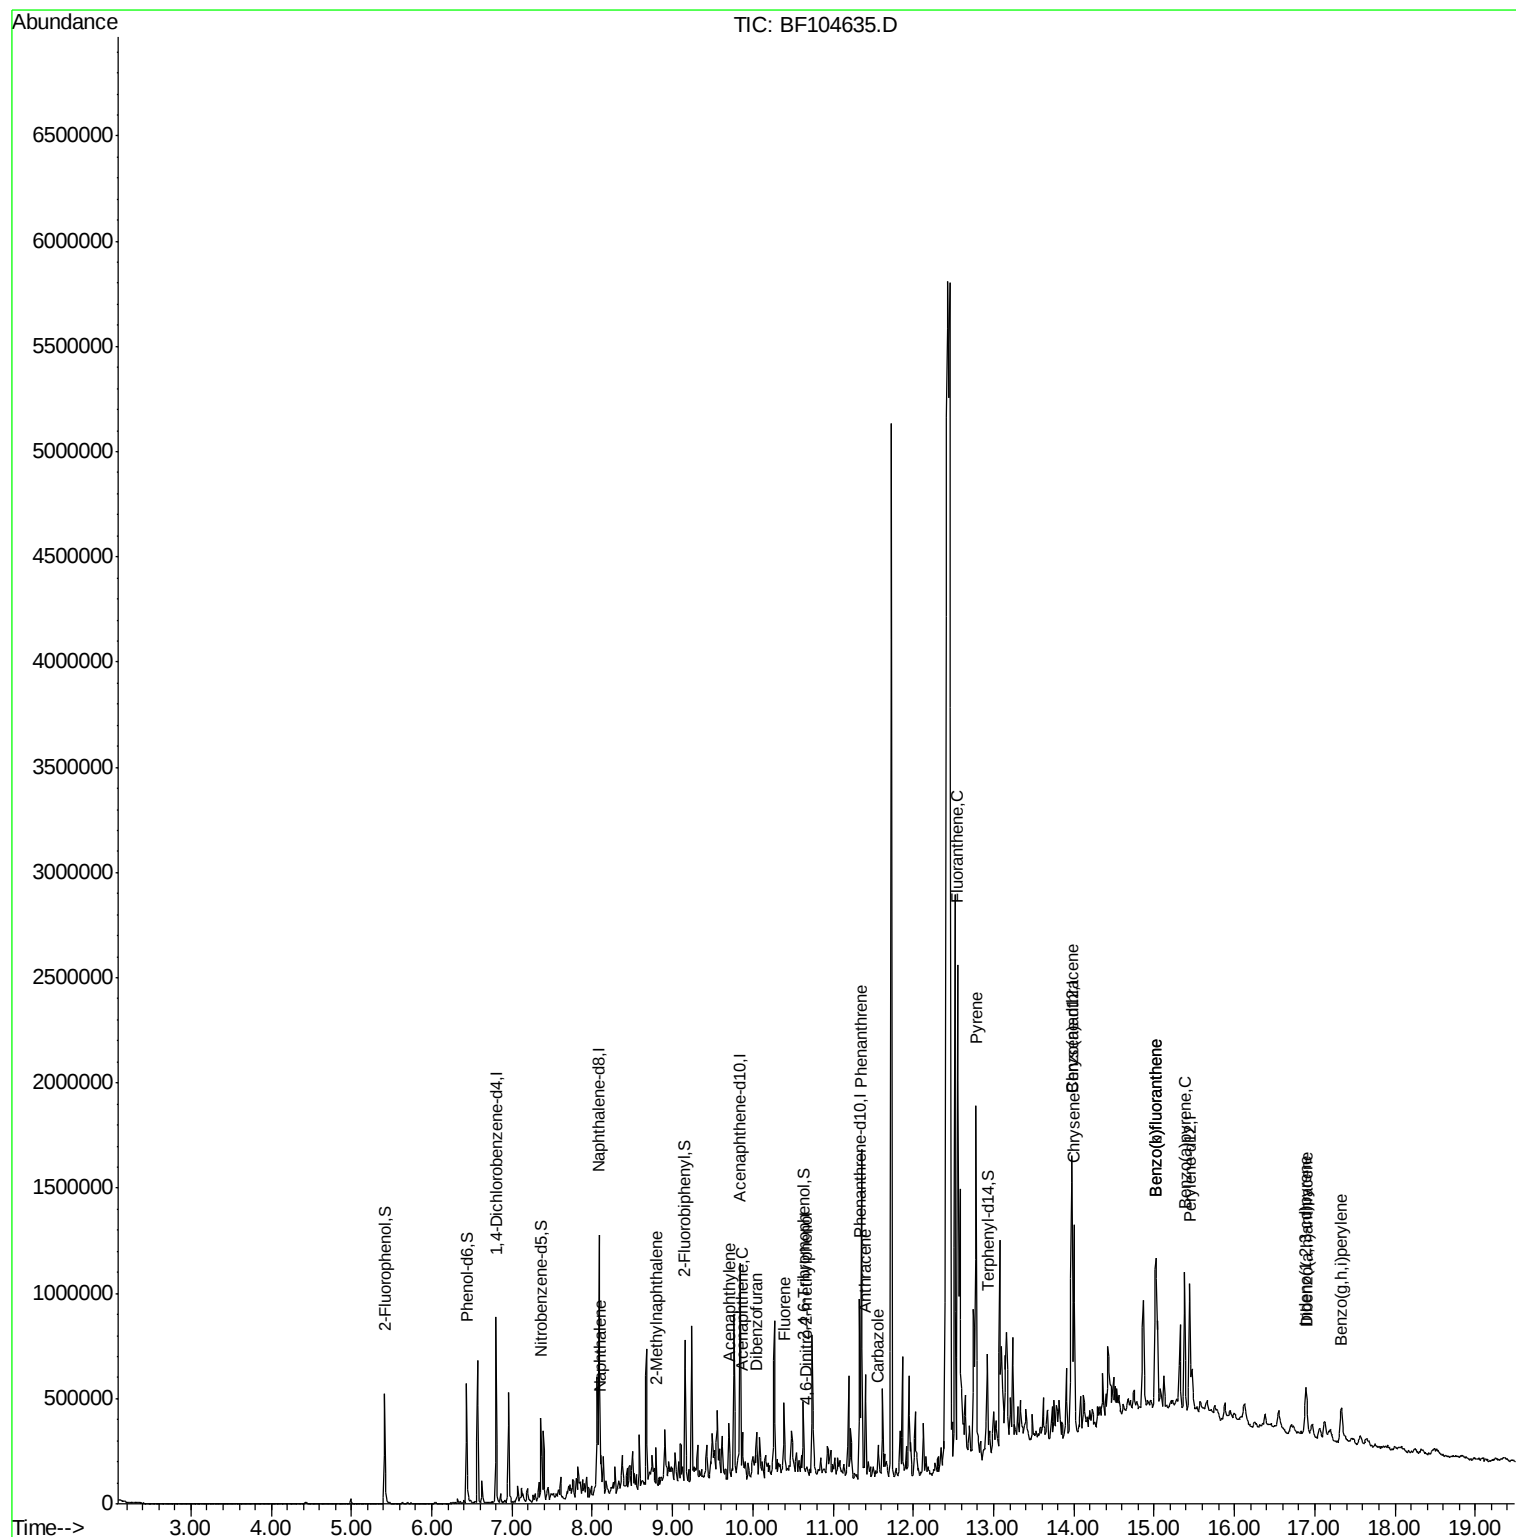

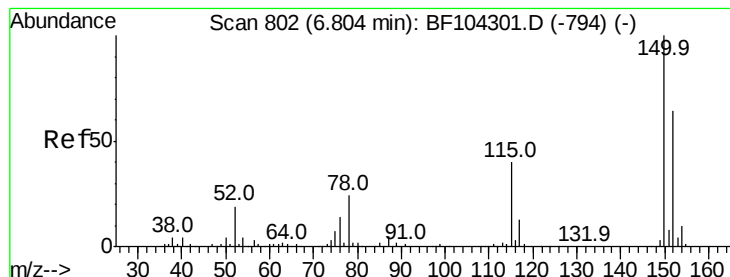


#1




1,4-Dichlorobenzene-d4
 Concen: 20.000 ng
 RT: 6.80 min Scan# 802
 Delta R.T. 0.00 min
 Lab File: BF104635.D
 Acq: 19 Apr 2018 18:32

Instrument :
 BNA_F
 ClientSampleId :

Tot Ion:152 Resp: 129146
 Ion Ratio Lower Upper
 152 100
 150 157.4 124.6 186.8
 115 61.0 50.1 75.1

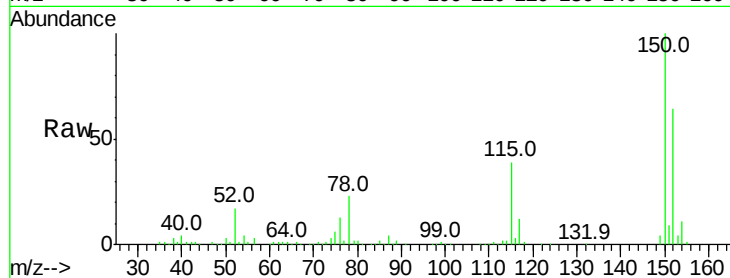


Abundance Ion 152.00 (151.70 to 152.70): E
 Ion 150.00 (149.70 to 150.70): E
 Ion 115.00 (114.70 to 115.70): E

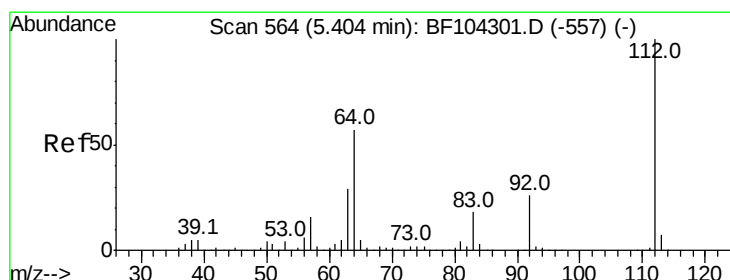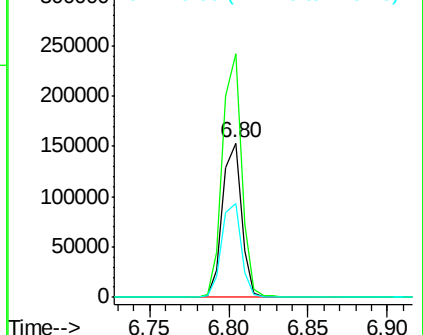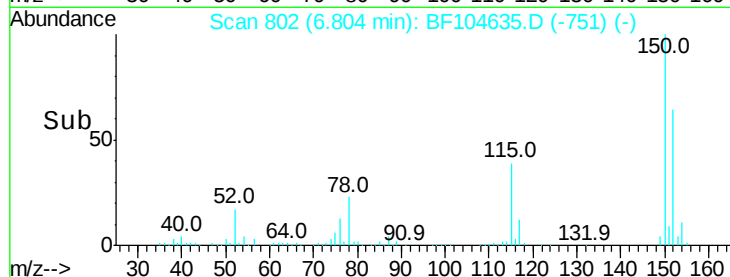



#5

2-Fluorophenol
 Concen: 19.716 ng
 RT: 5.41 min Scan# 565
 Delta R.T. -0.01 min
 Lab File: BF104635.D
 Acq: 19 Apr 2018 18:32

Tgt Ion:112 Resp: 166525
 Ion Ratio Lower Upper
 112 100
 64 56.4 47.9 71.9
 63 27.1 23.7 35.5

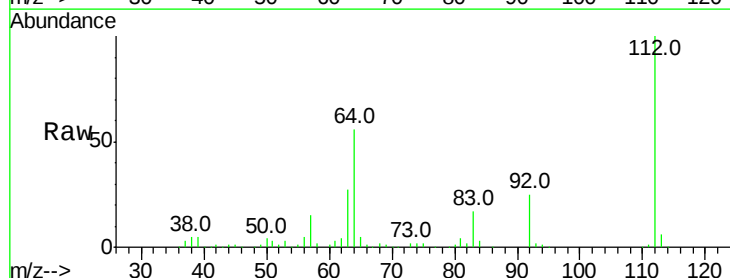

Abundance Ion 112.00 (111.70 to 112.70): E
 Ion 64.00 (63.70 to 64.70): BF1
 Ion 63.00 (62.70 to 63.70): BF1

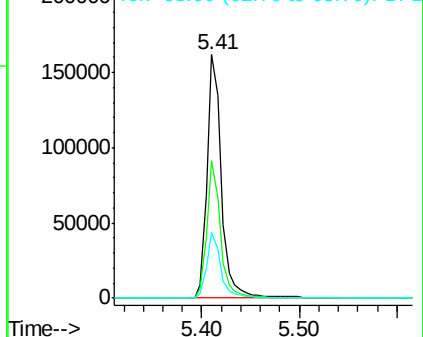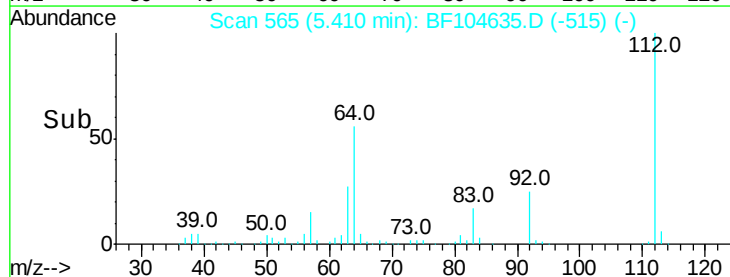



#7

Phenol-d6

Concen: 19.042 ng

RT: 6.43 min Scan# 739

Delta R.T. -0.01 min

Lab File: BF104635.D

Acq: 19 Apr 2018 18:32

Instrument :

BNA_F

ClientSampleId :


Tot Ion: 99 Resp: 197608

Ion Ratio Lower Upper




99 100

42 15.5 14.5 21.7

71 30.3 25.4 38.0

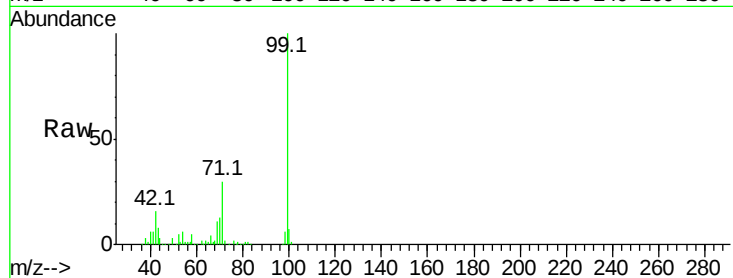

Abundance Ion 99.00 (98.70 to 99.70): BF1
Ion 42.00 (41.70 to 42.70): BF1
Ion 71.00 (70.70 to 71.70): BF1

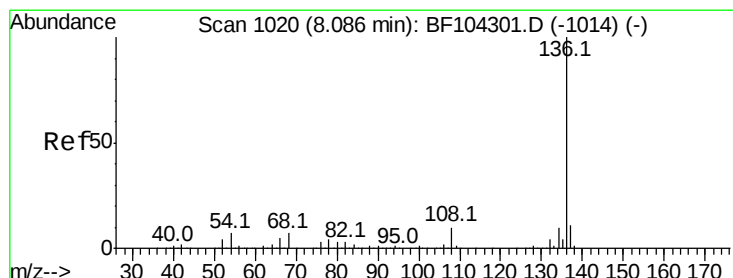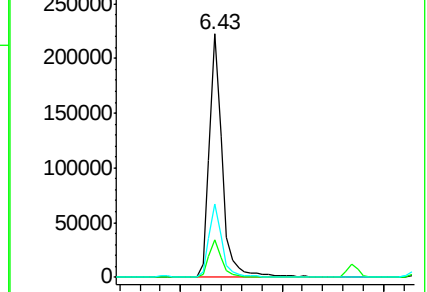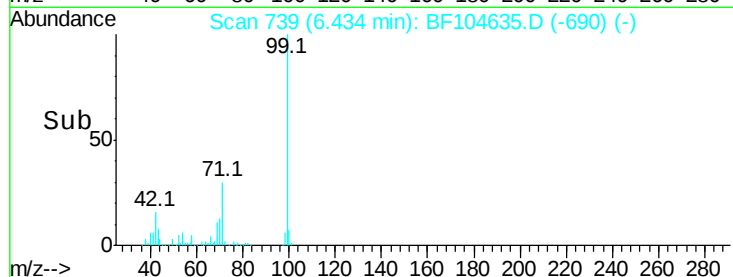

#21

Naphthalene-d8

Concen: 20.000 ng

RT: 8.09 min Scan# 1020

Delta R.T. -0.01 min

Lab File: BF104635.D

Acq: 19 Apr 2018 18:32

Tgt Ion: 136 Resp: 492228


Ion Ratio Lower Upper

136 100



137 10.9 8.9 13.3


54 6.8 6.6 9.8

68 6.1 5.0 7.4

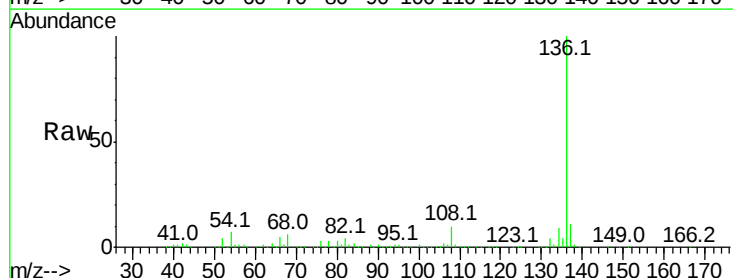

Abundance Ion 136.00 (135.70 to 136.70): E
Ion 137.00 (136.70 to 137.70): E
Ion 54.00 (53.70 to 54.70): BF1
Ion 68.00 (67.70 to 68.70): BF1

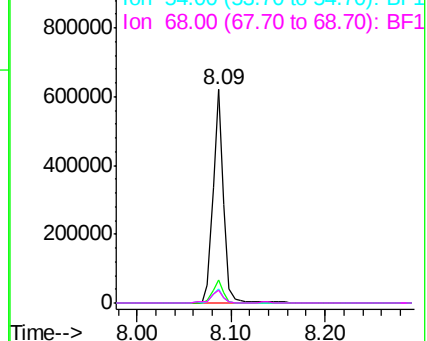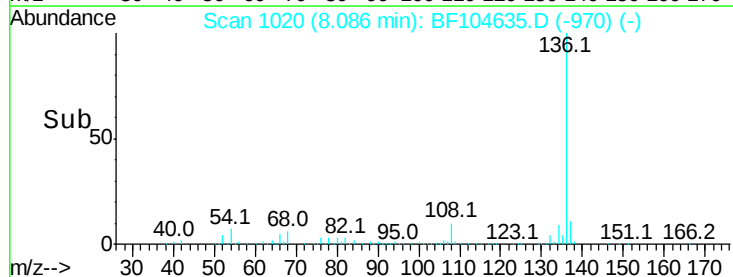







#23
Nitrobenzene-d5
Concen: 14.718 ng
RT: 7.36 min Scan# 897
Delta R.T. -0.02 min
Lab File: BF104635.D
Acq: 19 Apr 2018 18:32

Instrument :
BNA_F
ClientSampleId :

Tot Ion: 82 Resp: 110950
Ion Ratio Lower Upper
82 100
128 45.3 36.1 54.1
54 44.1 41.4 62.2

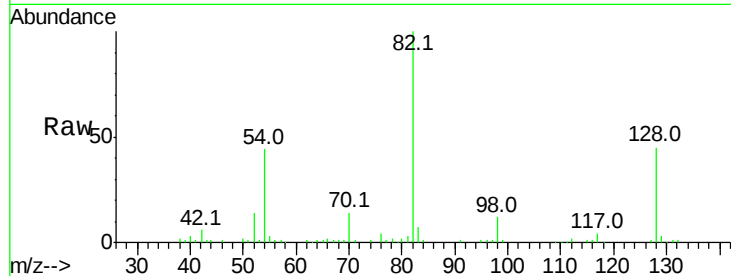


Abundance Ion 82.00 (81.70 to 82.70): BF1
Ion 128.00 (127.70 to 128.70): BF1
Ion 54.00 (53.70 to 54.70): BF1

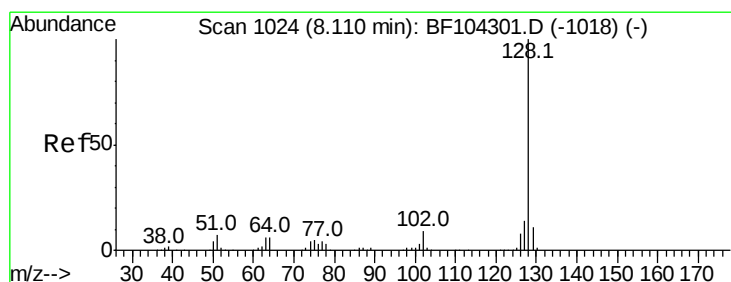
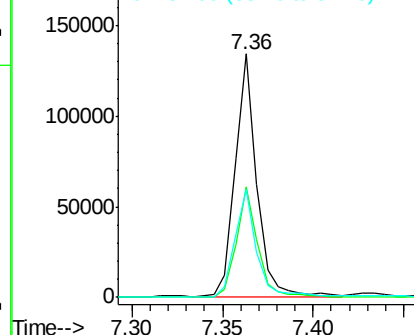



#31
Naphthalene
Concen: 2.121 ng
RT: 8.11 min Scan# 1024
Delta R.T. -0.01 min
Lab File: BF104635.D
Acq: 19 Apr 2018 18:32

Tgt Ion:128 Resp: 51992
Ion Ratio Lower Upper
128 100
129 12.7 8.8 13.2
127 13.2 10.9 16.3



Abundance Ion 128.00 (127.70 to 128.70): BF1
Ion 129.00 (128.70 to 129.70): BF1
Ion 127.00 (126.70 to 127.70): BF1




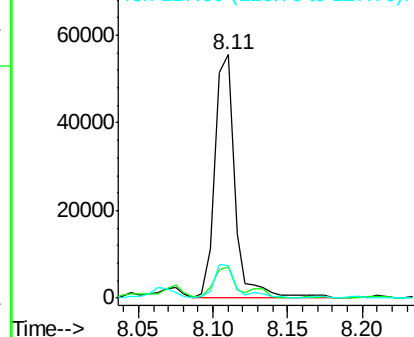




#37
 2-Methylnaphthalene
 Concen: 2.563 ng
 RT: 8.80 min Scan# 1141
 Delta R.T. -0.01 min
 Lab File: BF104635.D
 Acq: 19 Apr 2018 18:32




Instrument :
 BNA_F
 ClientSampleId :


Tot Ion	Ratio	Lower	Upper
142	100		
141	89.1	70.8	106.2
115	34.9	26.1	39.1

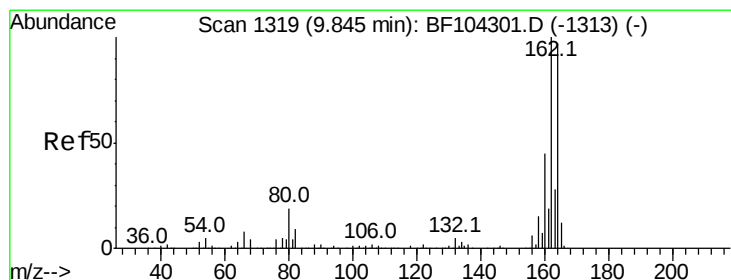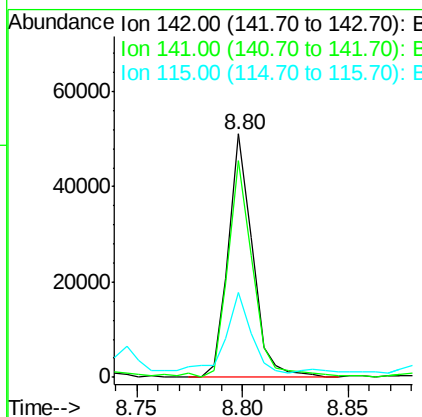

#38
 Acenaphthene-d10
 Concen: 20.000 ng
 RT: 9.84 min Scan# 1318
 Delta R.T. -0.01 min
 Lab File: BF104635.D
 Acq: 19 Apr 2018 18:32

Tgt Ion	Ratio	Lower	Upper
164	100		
162	104.5	86.1	129.1
160	45.8	38.3	57.5

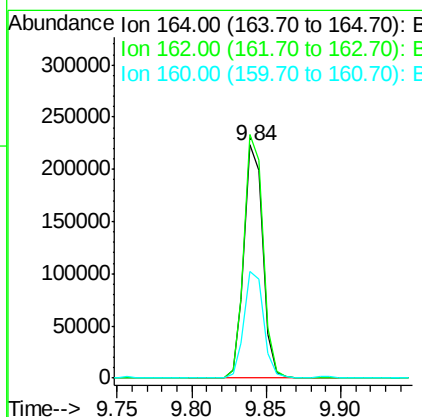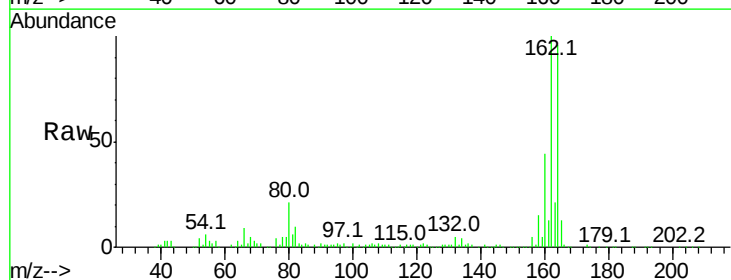


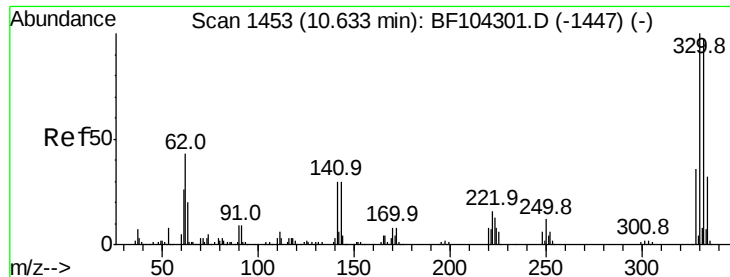




#41
 2,4,6-Tribromophenol
 Concen: 17.471 ng
 RT: 10.63 min Scan# 1453
 Delta R.T. -0.01 min
 Lab File: BF104635.D
 Acq: 19 Apr 2018 18:32

Instrument :
 BNA_F
 ClientSampleId :

Tot Ion:330 Resp: 35794
 Ion Ratio Lower Upper
 330 100
 332 94.4 77.0 115.6
 141 34.9 29.9 44.9

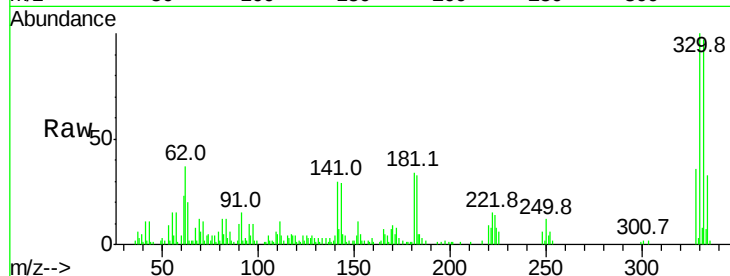


Abundance Ion 329.80 (329.50 to 330.50): E
 Ion 331.80 (331.50 to 332.50): E
 Ion 141.00 (140.70 to 141.70): E

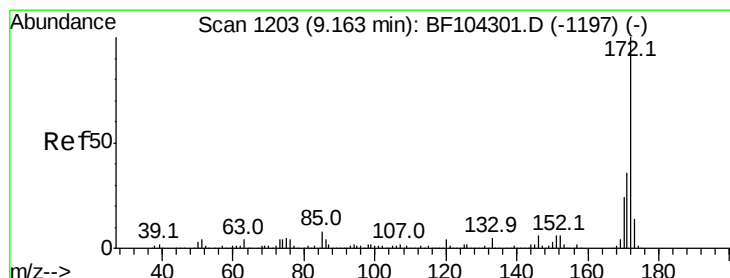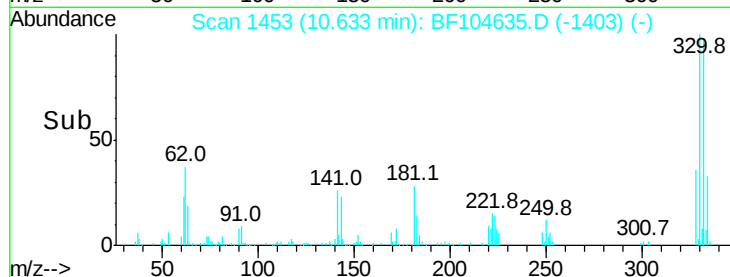
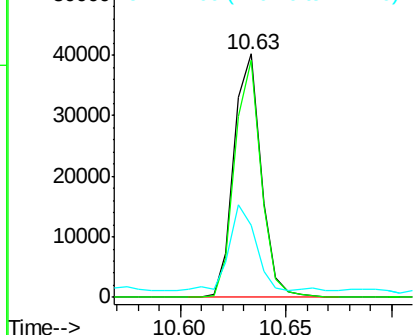



#44
 2-Fluorobiphenyl
 Concen: 15.508 ng
 RT: 9.16 min Scan# 1202
 Delta R.T. -0.01 min
 Lab File: BF104635.D
 Acq: 19 Apr 2018 18:32

Tgt Ion:172 Resp: 193885
 Ion Ratio Lower Upper
 172 100
 171 35.1 29.7 44.5
 170 22.6 19.6 29.4

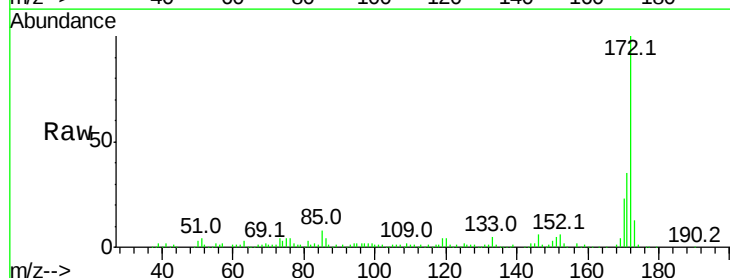

Abundance Ion 172.00 (171.70 to 172.70): E
 Ion 171.00 (170.70 to 171.70): E
 Ion 170.00 (169.70 to 170.70): E

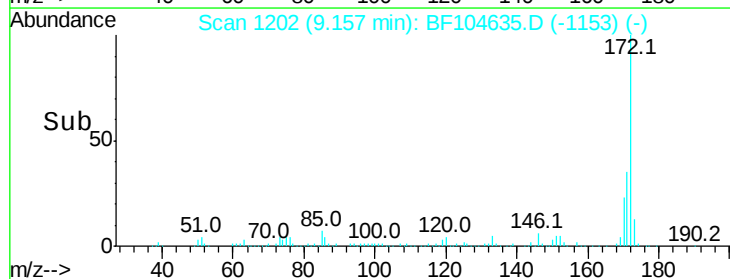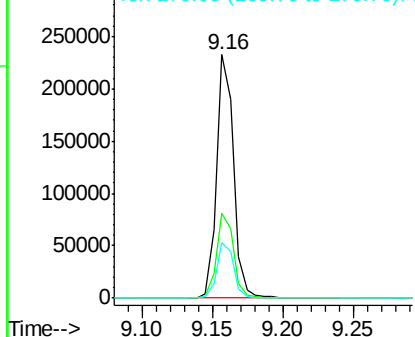



#48

Acenaphthylene

Concen: 3.952 ng

RT: 9.70 min Scan# 1295

Delta R.T. -0.01 min

Lab File: BF104635.D

Acq: 19 Apr 2018 18:32

Instrument :

BNA_F

ClientSampleId :


Tot Ion:152 Resp: 81260

Ion Ratio Lower Upper

152 100

151 21.3 16.3 24.5




153 14.1 10.7 16.1



Abundance Ion 152.00 (151.70 to 152.70): E

Ion 151.00 (150.70 to 151.70): E

Ion 153.00 (152.70 to 153.70): E

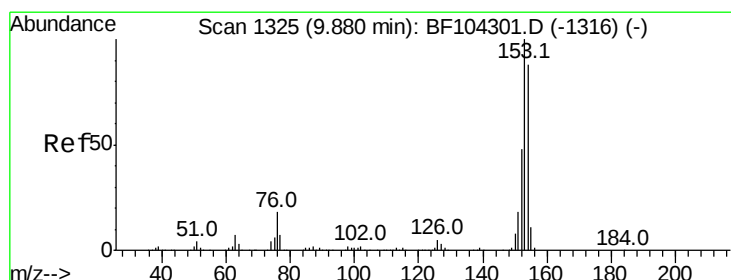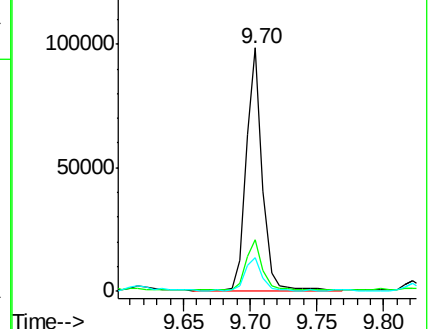

#51

Acenaphthene

Concen: 2.459 ng

RT: 9.87 min Scan# 1324

Delta R.T. -0.01 min

Lab File: BF104635.D

Acq: 19 Apr 2018 18:32


Tgt Ion:154 Resp: 30854

Ion Ratio Lower Upper

154 100

153 114.3 91.2 136.8



152 57.8 43.8 65.8




Abundance Ion 154.00 (153.70 to 154.70): E

Ion 153.00 (152.70 to 153.70): E

Ion 152.00 (151.70 to 152.70): E

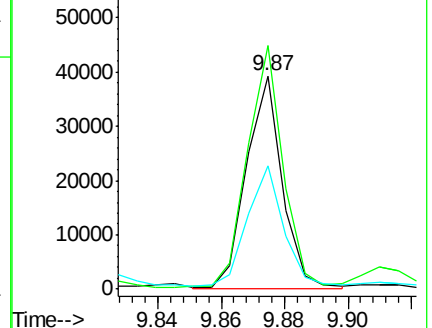



#54

Dibenzenofuran

Concen: 2.821 ng

RT: 10.05 min Scan# 1353

Delta R.T. -0.01 min

Lab File: BF104635.D

Acq: 19 Apr 2018 18:32

Instrument :

BNA_F

ClientSampleId :


Tot Ion:168 Resp: 49329

Ion Ratio Lower Upper

168 100

139 40.4 30.1 45.1




169 17.8 10.9 16.3#



Abundance Ion 168.00 (167.70 to 168.70): E

Ion 139.00 (138.70 to 139.70): E

Ion 169.00 (168.70 to 169.70): E

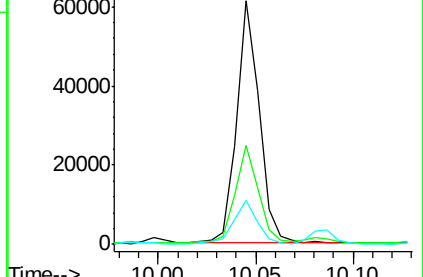

#57

Fluorene

Concen: 7.265 ng

RT: 10.39 min Scan# 1411

Delta R.T. -0.01 min

Lab File: BF104635.D

Acq: 19 Apr 2018 18:32


Tgt Ion:166 Resp: 92458

Ion Ratio Lower Upper

166 100

165 99.4 79.8 119.8



167 14.9 10.6 16.0




Abundance Ion 166.00 (165.70 to 166.70): E

Ion 165.00 (164.70 to 165.70): E

Ion 167.00 (166.70 to 167.70): E




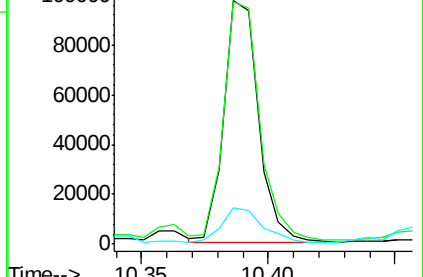


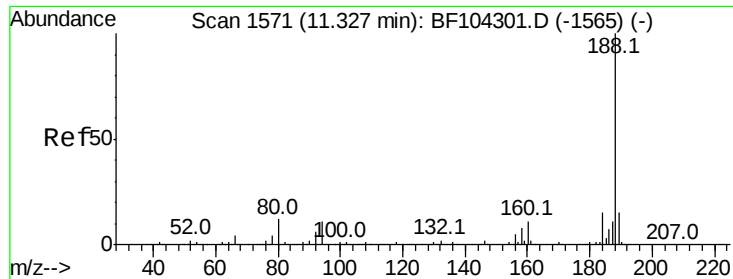

#63
Phenanthrene-d10
Concen: 20.000 ng
RT: 11.33 min Scan# 1572
Delta R.T. 0.00 min
Lab File: BF104635.D
Acq: 19 Apr 2018 18:32




Instrument :
BNA_F
ClientSampled :


Tot Ion:188 Resp: 306852
Ion Ratio Lower Upper
188 100
94 9.4 8.5 12.7
80 9.9 9.2 13.8

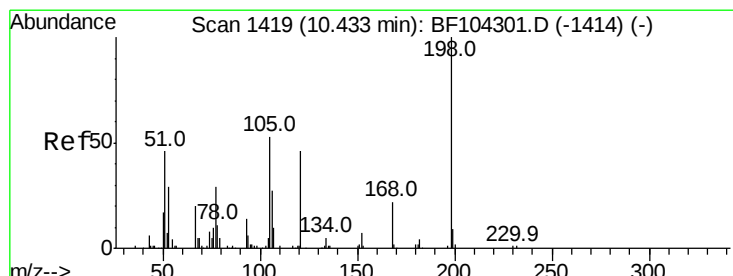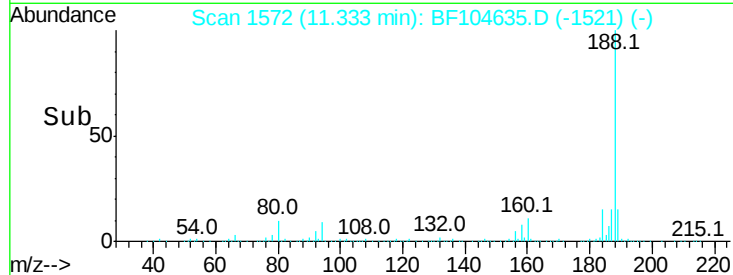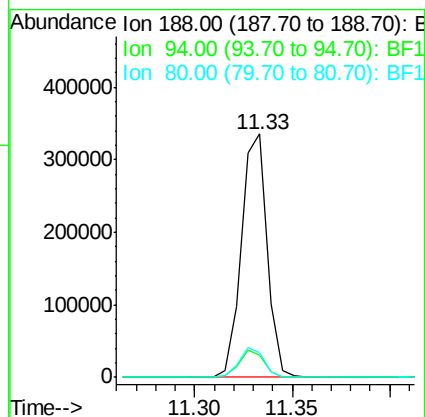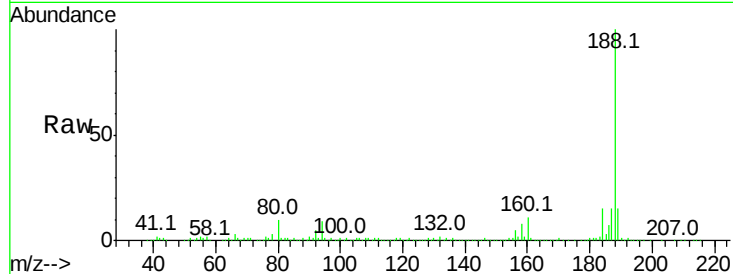

#64
4,6-Dinitro-2-methylphenol
Concen: 7.417 ng
RT: 10.66 min Scan# 1458
Delta R.T. 0.21 min
Lab File: BF104635.D
Acq: 19 Apr 2018 18:32

Tgt Ion:198 Resp: 124
Ion Ratio Lower Upper
198 100
51 161.8 37.7 77.7#
105 1000.3 36.3 76.3#

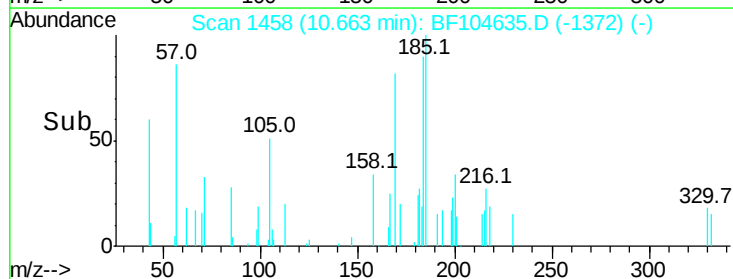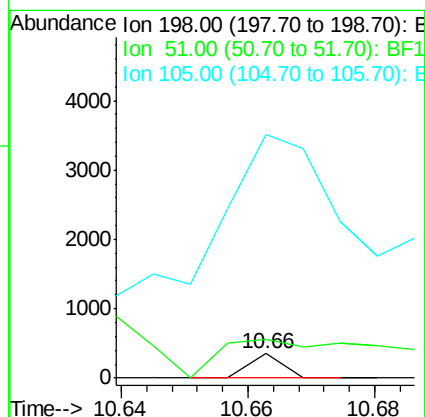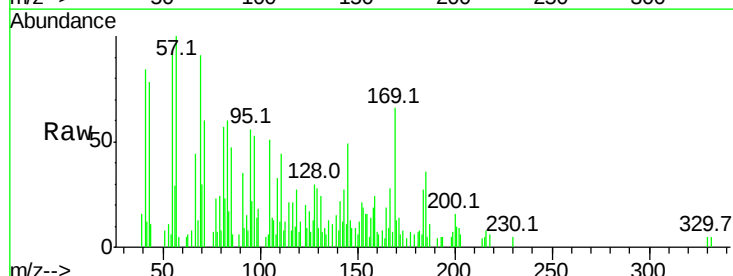

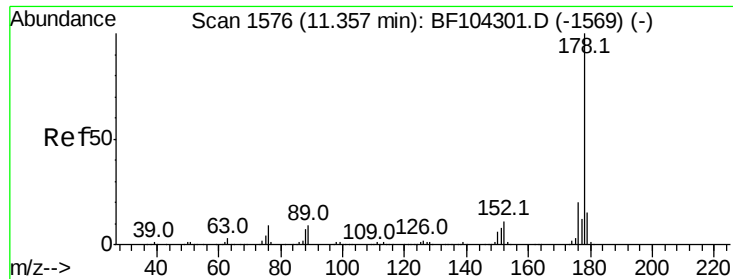

#70

Phenanthrene

Concen: 32.090 ng

RT: 11.36 min Scan# 1576

Delta R.T. -0.01 min

Lab File: BF104635.D

Acq: 19 Apr 2018 18:32

Instrument :

BNA_F

ClientSampleId :


Tot Ion:178 Resp: 548370

Ion Ratio Lower Upper

178 100

176 19.9 15.8 23.8




179 15.8 13.0 19.6

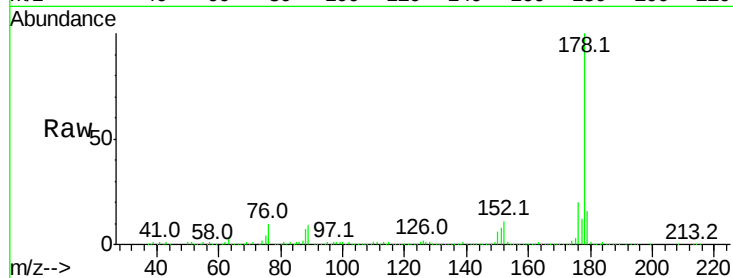

Abundance Ion 178.00 (177.70 to 178.70): E

Ion 176.00 (175.70 to 176.70): E

Ion 179.00 (178.70 to 179.70): E

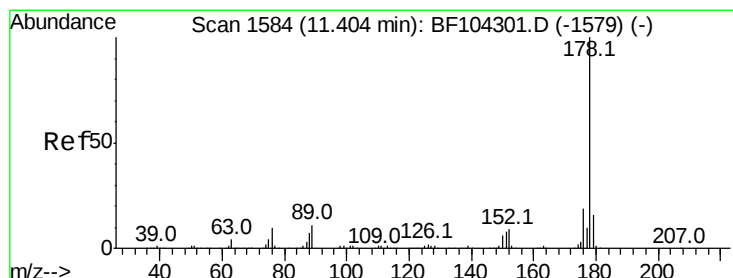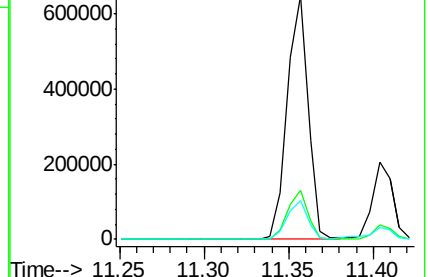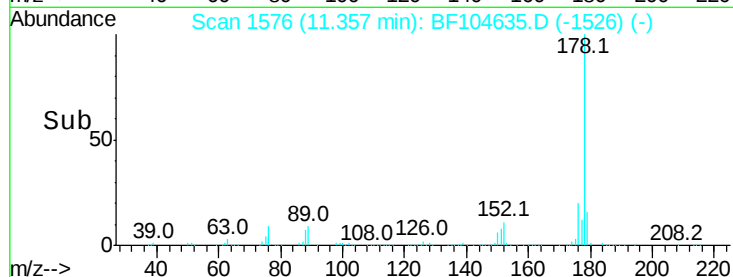

#71

Anthracene

Concen: 9.594 ng

RT: 11.40 min Scan# 1584

Delta R.T. -0.01 min

Lab File: BF104635.D

Acq: 19 Apr 2018 18:32


Tgt Ion:178 Resp: 166651

Ion Ratio Lower Upper

178 100

176 18.3 15.4 23.2



179 15.2 12.6 19.0

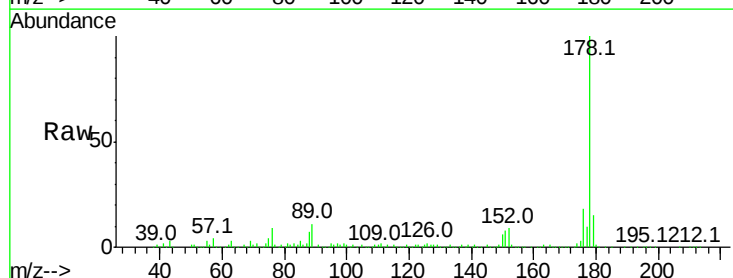


Abundance Ion 178.00 (177.70 to 178.70): E

Ion 176.00 (175.70 to 176.70): E

Ion 179.00 (178.70 to 179.70): E

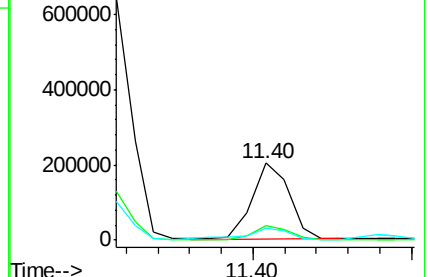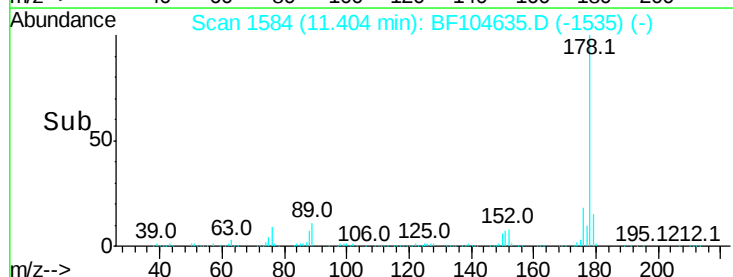



#72

Carbazole

Concen: 2.376 ng

RT: 11.56 min Scan# 1611

Delta R.T. -0.01 min

Lab File: BF104635.D

Acq: 19 Apr 2018 18:32

Instrument :

BNA_F

ClientSampleId :


Tot Ion:167 Resp: 40322

Ion Ratio Lower Upper

167 100

166 22.6 17.6 26.4




139 14.0 10.9 16.3

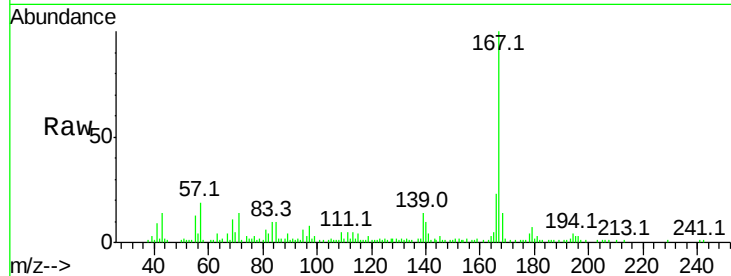

Abundance Ion 167.00 (166.70 to 167.70): E

Ion 166.00 (165.70 to 166.70): E

Ion 139.00 (138.70 to 139.70): E

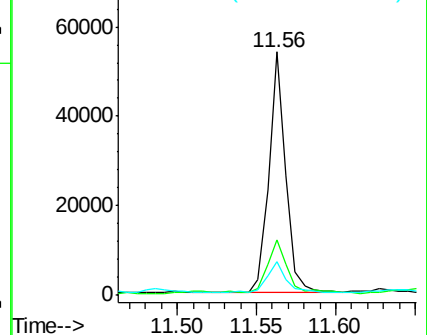

#74

Fluoranthene

Concen: 41.985 ng

RT: 12.55 min Scan# 1779

Delta R.T. 0.00 min

Lab File: BF104635.D

Acq: 19 Apr 2018 18:32


Tgt Ion:202 Resp: 749611

Ion Ratio Lower Upper

202 100

101 12.5 0.0 34.1



203 17.9 0.0 38.1




Abundance Ion 202.00 (201.70 to 202.70): E

Ion 101.00 (100.70 to 101.70): E

Ion 203.00 (202.70 to 203.70): E

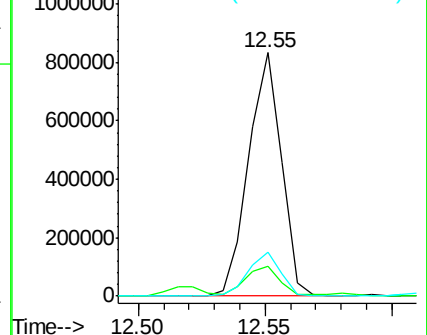



#75

Chrysene-d12

Concen: 20.000 ng

RT: 13.98 min Scan# 2022

Delta R.T. -0.01 min

Lab File: BF104635.D

Acq: 19 Apr 2018 18:32

Instrument :

BNA_F

ClientSampleId :


Tot Ion:240 Resp: 275639

Ion Ratio Lower Upper

240 100

120 12.4 9.5 14.3




236 26.5 20.7 31.1

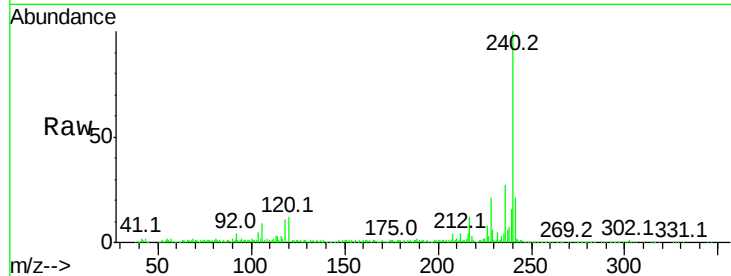

Abundance Ion 240.00 (239.70 to 240.70): E

Ion 120.00 (119.70 to 120.70): E

Ion 236.00 (235.70 to 236.70): E

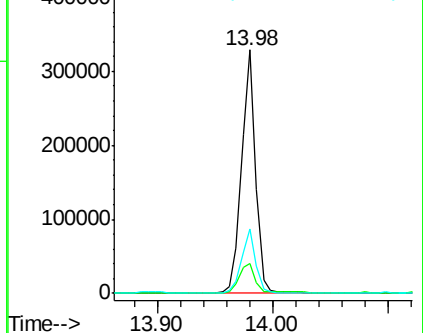

#77

Pyrene

Concen: 35.152 ng

RT: 12.78 min Scan# 1818

Delta R.T. 0.00 min

Lab File: BF104635.D

Acq: 19 Apr 2018 18:32


Tgt Ion:202 Resp: 718200

Ion Ratio Lower Upper

202 100

200 21.6 17.4 26.2



203 17.9 14.3 21.5




Abundance Ion 202.00 (201.70 to 202.70): E

Ion 200.00 (199.70 to 200.70): E

Ion 203.00 (202.70 to 203.70): E

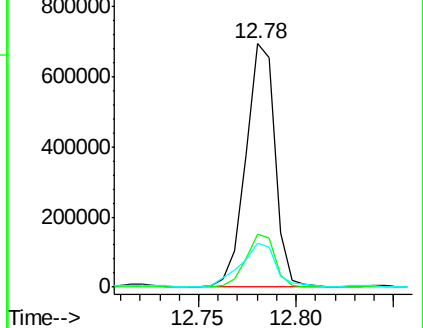



#78

Terphenyl-d14

Concen: 12.151 ng

RT: 12.92 min Scan# 1842

Delta R.T. 0.00 min

Lab File: BF104635.D

Acq: 19 Apr 2018 18:32

Instrument :

BNA_F

ClientSampled :


Tot Ion:244 Resp: 146912

Ion Ratio Lower Upper

244 100

212 6.7 5.4 8.0




122 11.6 11.0 16.4



Abundance Ion 244.00 (243.70 to 244.70): E

Ion 212.00 (211.70 to 212.70): E

Ion 122.00 (121.70 to 122.70): E

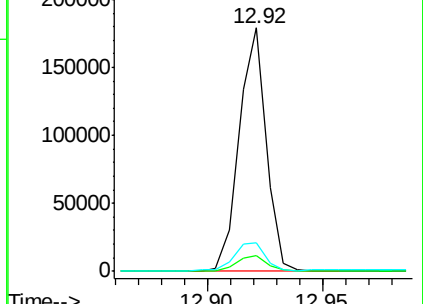

#80

Benzo(a)anthracene

Concen: 25.619 ng

RT: 13.97 min Scan# 2020

Delta R.T. -0.01 min

Lab File: BF104635.D

Acq: 19 Apr 2018 18:32


Tgt Ion:228 Resp: 421860

Ion Ratio Lower Upper

228 100

226 31.4 22.6 33.8



229 20.8 15.8 23.6




Abundance Ion 228.00 (227.70 to 228.70): E

Ion 226.00 (225.70 to 226.70): E

Ion 229.00 (228.70 to 229.70): E




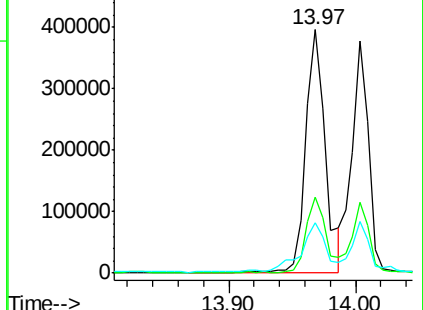




#82
Chrysene
Concen: 20.297 ng
RT: 14.00 min Scan# 2026
Delta R.T. -0.01 min
Lab File: BF104635.D
Acq: 19 Apr 2018 18:32




Instrument :
BNA_F
ClientSampleId :


Tot Ion:228 Resp: 343300
Ion Ratio Lower Upper
228 100
226 30.4 25.0 37.6
229 22.1 16.2 24.4

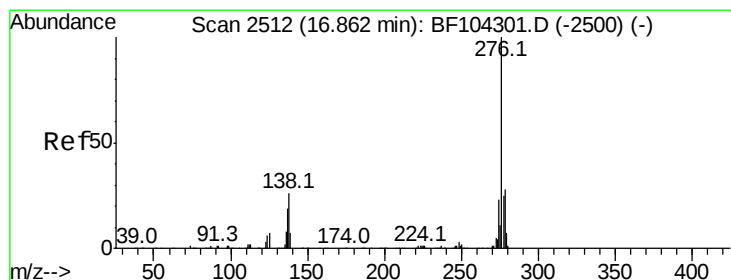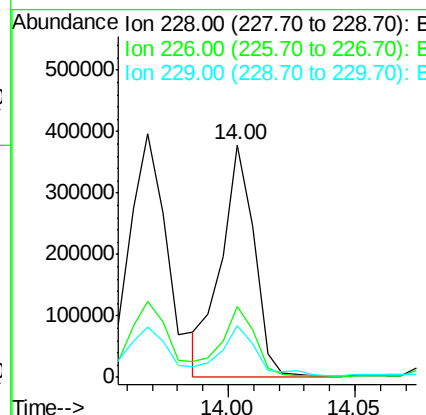

#85
Indeno(1,2,3-cd)pyrene
Concen: 9.804 ng
RT: 16.89 min Scan# 2517
Delta R.T. -0.02 min
Lab File: BF104635.D
Acq: 19 Apr 2018 18:32

Tgt Ion:276 Resp: 140869
Ion Ratio Lower Upper
276 100
138 26.0 25.0 37.6
277 25.9 20.1 30.1

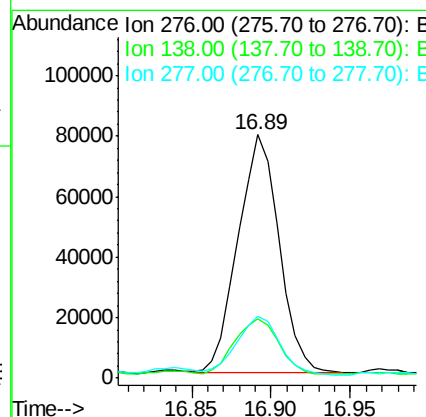



#86

Pervlene-d12

Concen: 20.000 ng

RT: 15.44 min Scan# 2271

Delta R.T. 0.00 min

Lab File: BF104635.D

Acq: 19 Apr 2018 18:32

Instrument :

BNA_F

ClientSampleId :


Tot Ion:264 Resp: 258218

Ion Ratio Lower Upper

264 100

260 24.6 19.2 28.8




265 22.5 17.5 26.3

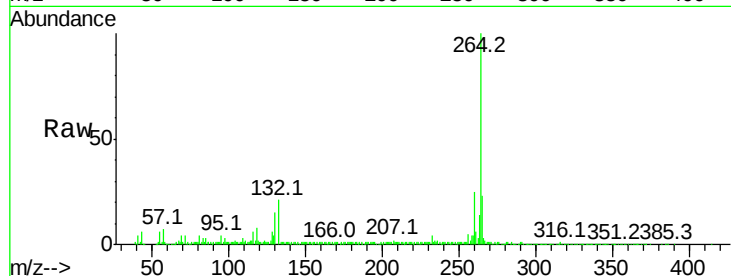

Abundance Ion 264.00 (263.70 to 264.70): E

Ion 260.00 (259.70 to 260.70): E

Ion 265.00 (264.70 to 265.70): E

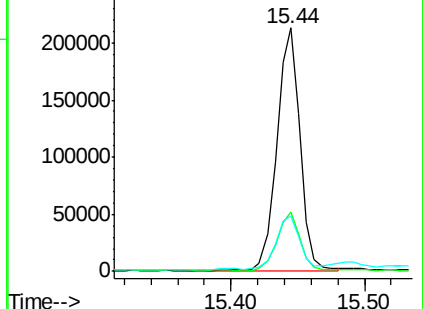

#87

Benzo(b)fluoranthene

Concen: 35.295 ng

RT: 15.02 min Scan# 2199

Delta R.T. -0.01 min

Lab File: BF104635.D

Acq: 19 Apr 2018 18:32


Tgt Ion:252 Resp: 575620

Ion Ratio Lower Upper

252 100

253 23.1 17.0 25.6



125 13.6 9.0 13.6#




Abundance Ion 252.00 (251.70 to 252.70): E

Ion 253.00 (252.70 to 253.70): E

Ion 125.00 (124.70 to 125.70): E




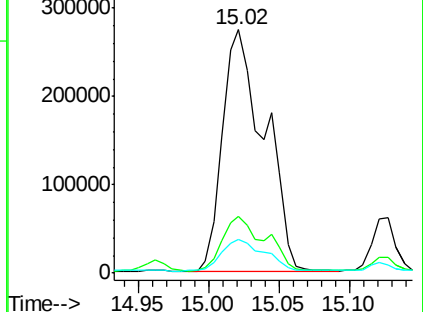


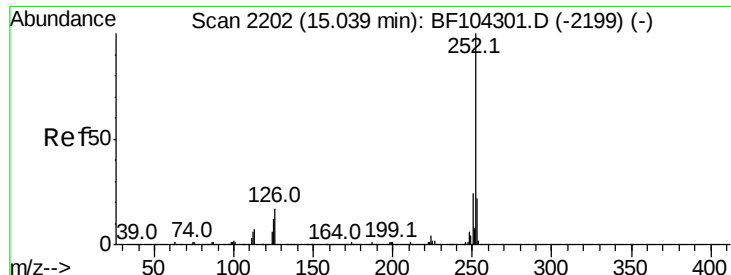

#88
Benzo(k)fluoranthene
Concen: 37.386 ng
RT: 15.02 min Scan# 2199
Delta R.T. -0.04 min
Lab File: BF104635.D
Acq: 19 Apr 2018 18:32




Instrument :
BNA_F
ClientSampleId :


Tot Ion	Ratio	Lower	Upper
252	100		
253	23.1	17.9	26.9
125	13.6	10.2	15.2

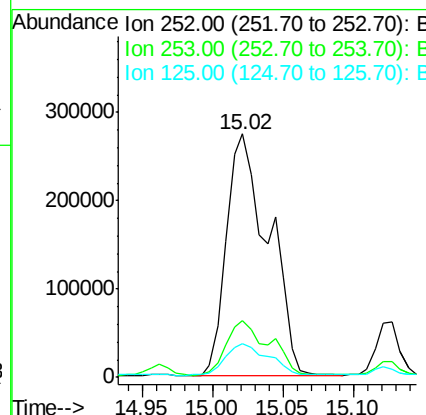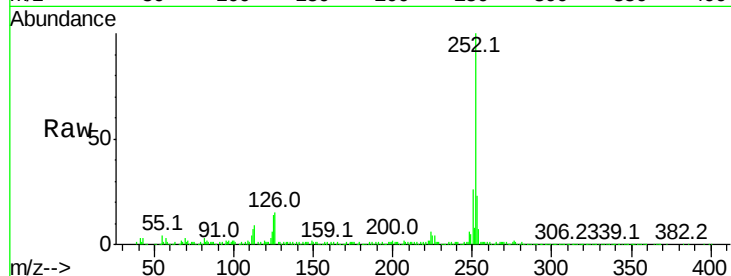

#89
Benzo(a)pyrene
Concen: 20.493 ng
RT: 15.38 min Scan# 2260
Delta R.T. -0.01 min
Lab File: BF104635.D
Acq: 19 Apr 2018 18:32

Tgt Ion	Ratio	Lower	Upper
252	100		
253	23.4	17.1	25.7
125	14.9	9.8	14.6

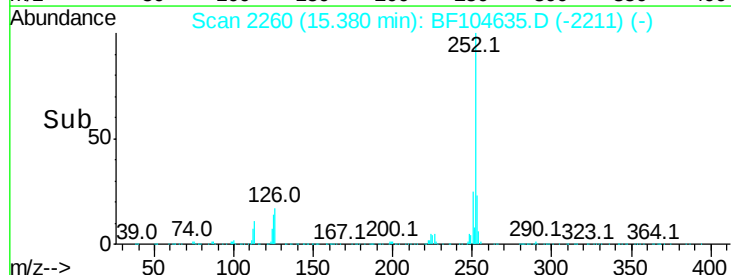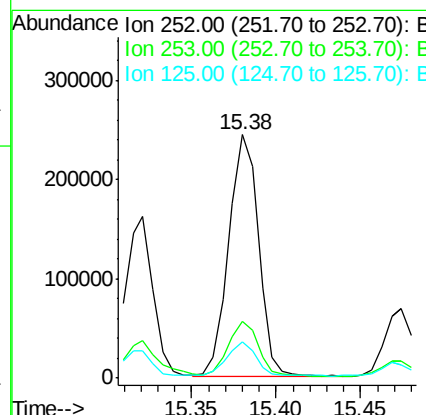



#90

Dibenzo(a,h)anthracene

Concen: 3.401 ng

RT: 16.90 min Scan# 2519

Delta R.T. -0.02 min

Lab File: BF104635.D

Acq: 19 Apr 2018 18:32

Instrument :

BNA_F

ClientSampleId :


Tot Ion:278 Resp: 40759

Ion Ratio Lower Upper

278 100

139 23.7 15.9 23.9




279 30.8 19.0 28.4#

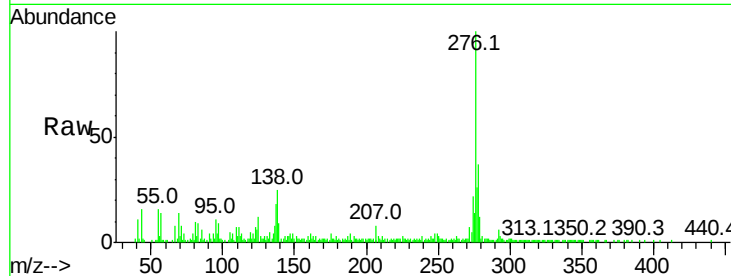

Abundance Ion 278.00 (277.70 to 278.70): E

Ion 139.00 (138.70 to 139.70): E

Ion 279.00 (278.70 to 279.70): E

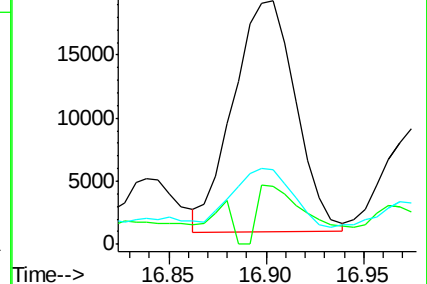

#91

Benzo(g,h,i)perylene

Concen: 11.412 ng

RT: 17.33 min Scan# 2592

Delta R.T. -0.02 min

Lab File: BF104635.D

Acq: 19 Apr 2018 18:32


Tgt Ion:276 Resp: 132507

Ion Ratio Lower Upper

276 100

277 24.7 17.9 26.9

138 25.1 21.8 32.8



Abundance Ion 276.00 (275.70 to 276.70): E

Ion 277.00 (276.70 to 277.70): E

Ion 138.00 (137.70 to 138.70): E

