
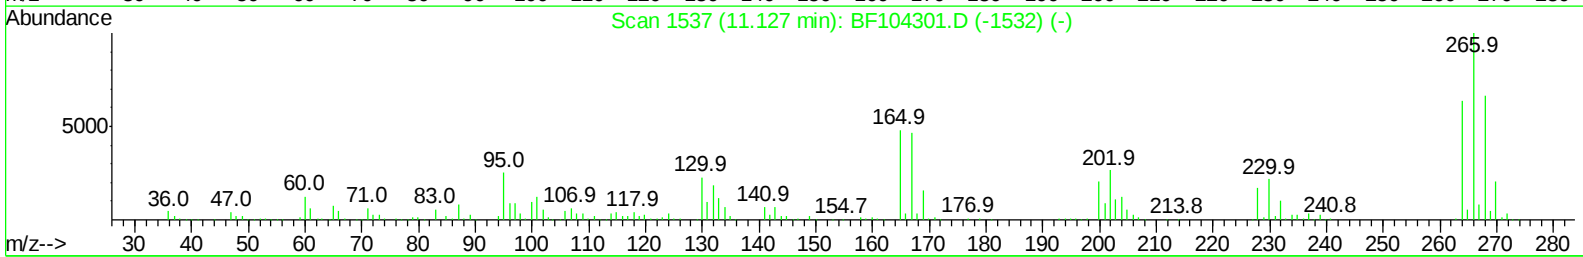
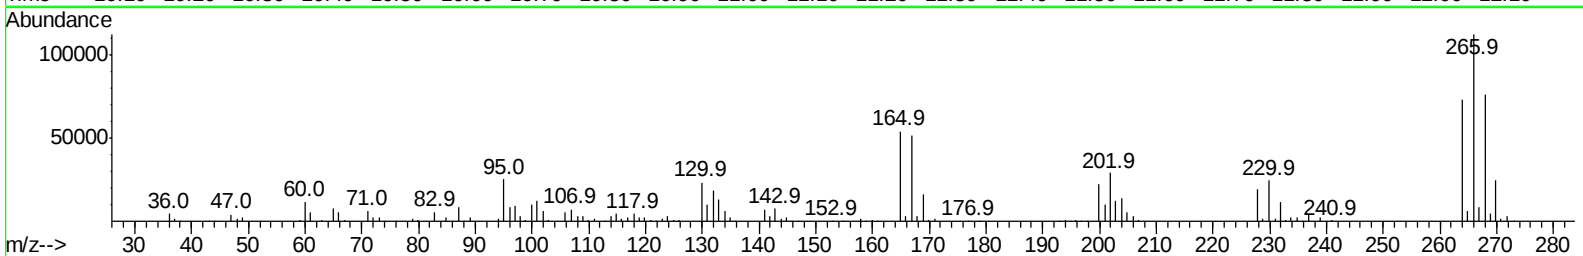


Data Path : Z:\HPCHEM1\BNA F\DATA\BF041918\
Data File : BF104631.D
Acq On : 19 Apr 2018 16:40
Operator : JU/SJ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Apr 20 06:41:34 2018
Quant Method : Z:\HPCHEM1\BNA F\METHODS\8270-BF040618.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Apr 19 14:44:03 2018
Response via : Initial Calibration

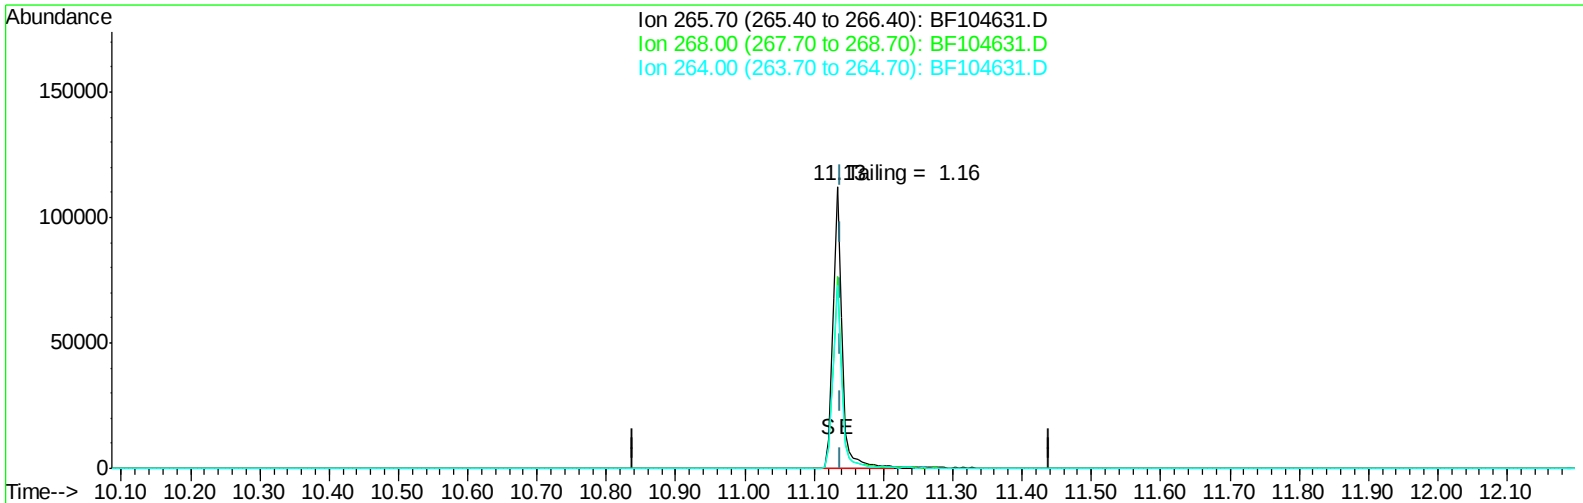

TIC: BF104631.D

(69) Pentachlorophenol (C)




11.133min (-0.006) 39673.96ng

response 102523

Ion	Exp%	Act%
265.70	100	100
268.00	63.90	68.16
264.00	61.90	65.09
0.00	0.00	0.00

Data Path : Z:\HPCHEM1\BNA F\DATA\BF041918\
Data File : BF104631.D
Acq On : 19 Apr 2018 16:40
Operator : JU/SJ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Apr 20 06:41:34 2018
Quant Method : Z:\HPCHEM1\BNA F\METHODS\8270-BF040618.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Apr 19 14:44:03 2018
Response via : Initial Calibration

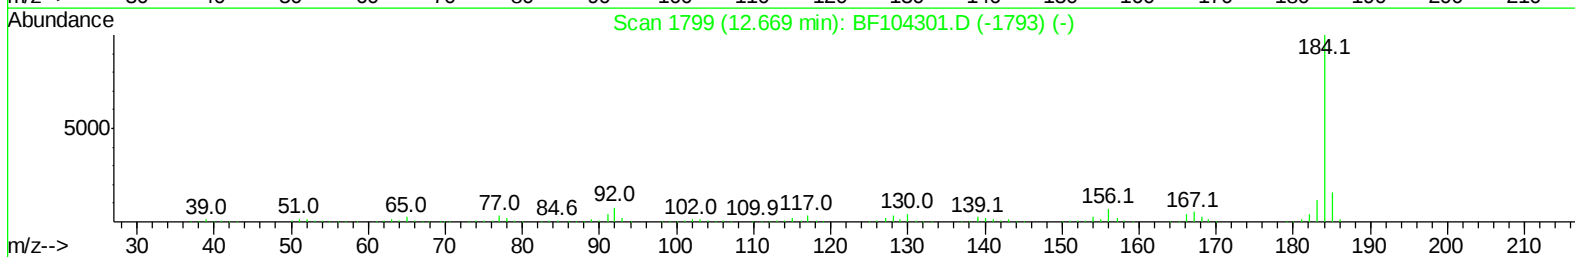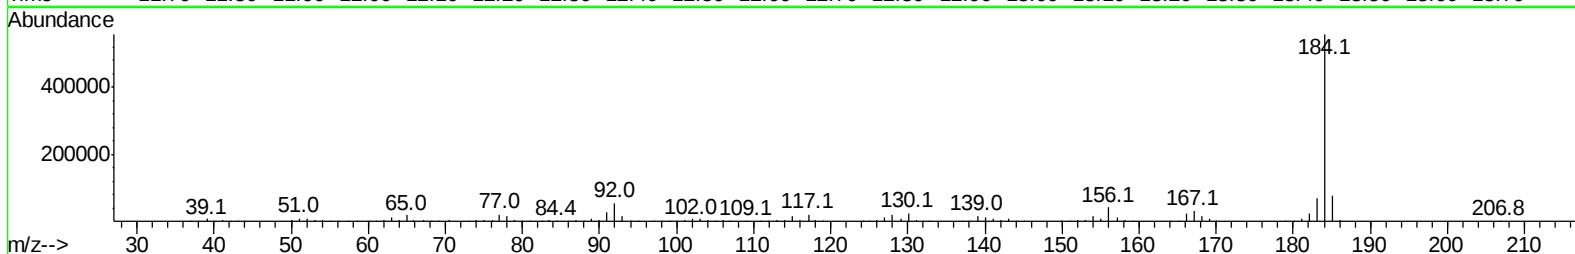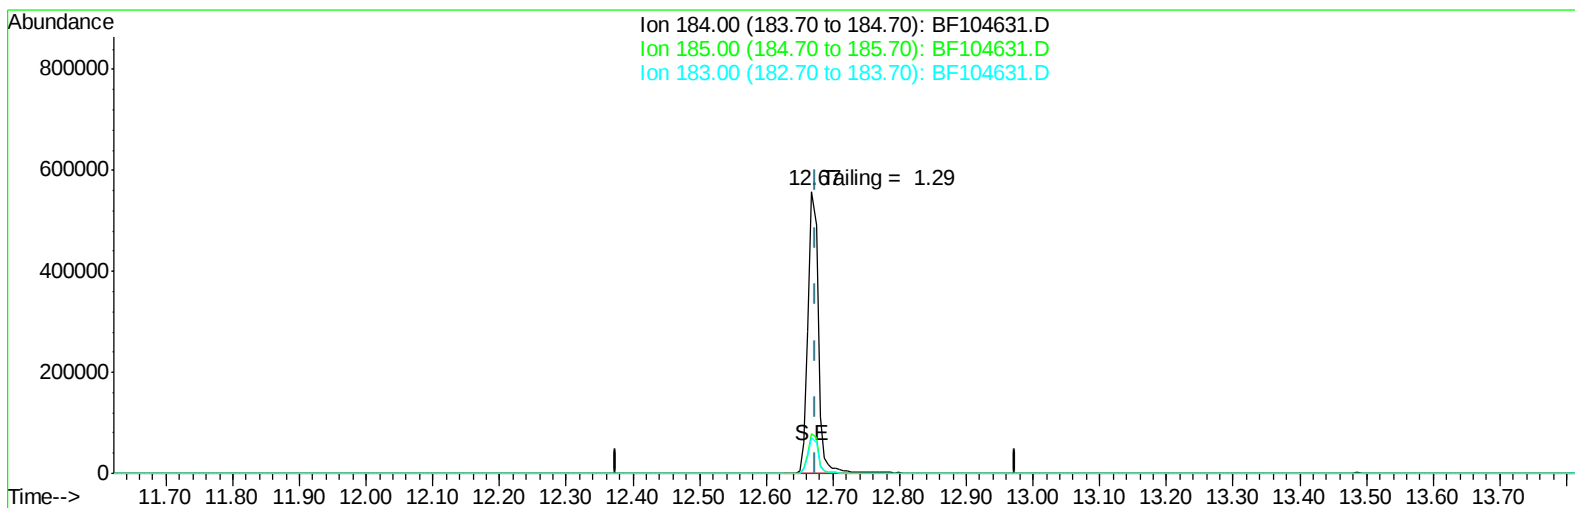

TIC: BF104631.D

(76) Benzidine

12.669min (-0.006) 0.00ng

response 575225

Ion	Exp%	Act%
184.00	100	100
185.00	15.70	14.02
183.00	11.60	12.53
0.00	0.00	0.00