
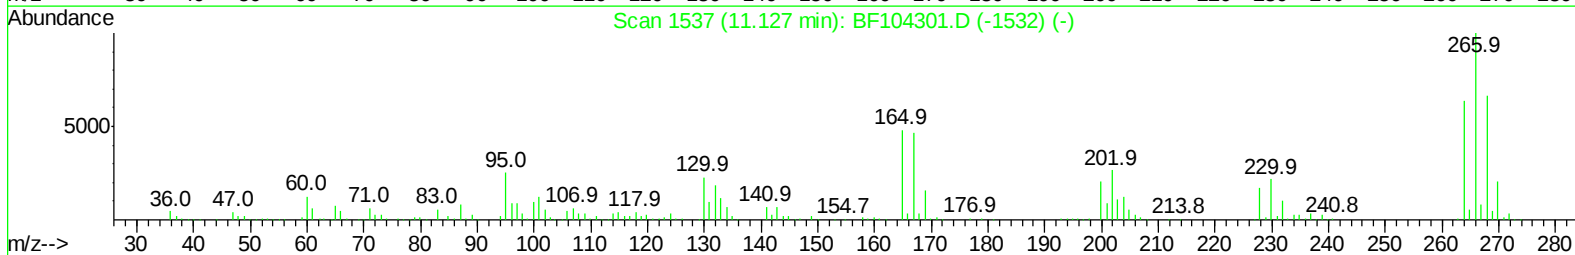
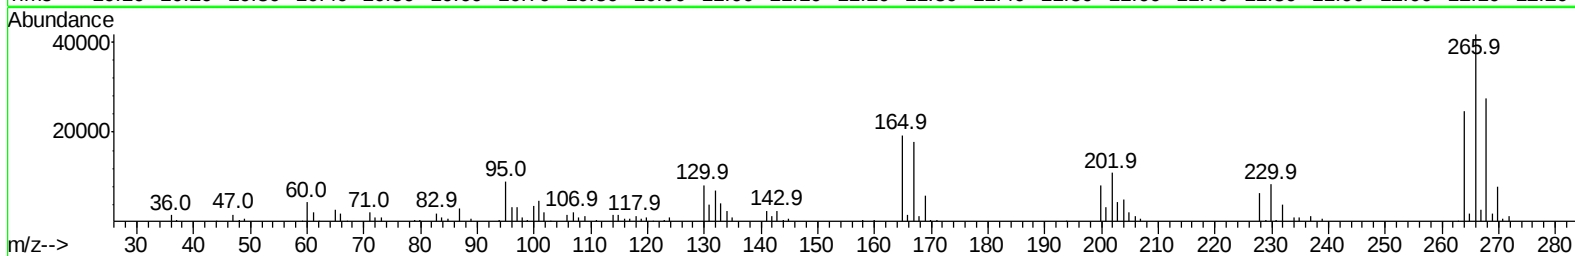


Data Path : Z:\HPCHEM1\BNA F\DATA\BF041918\
Data File : BF104659.D
Acq On : 20 Apr 2018 5:59
Operator : JU/SJ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Apr 20 06:42:36 2018
Quant Method : Z:\HPCHEM1\BNA F\METHODS\8270-BF040618.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Apr 19 14:44:03 2018
Response via : Initial Calibration

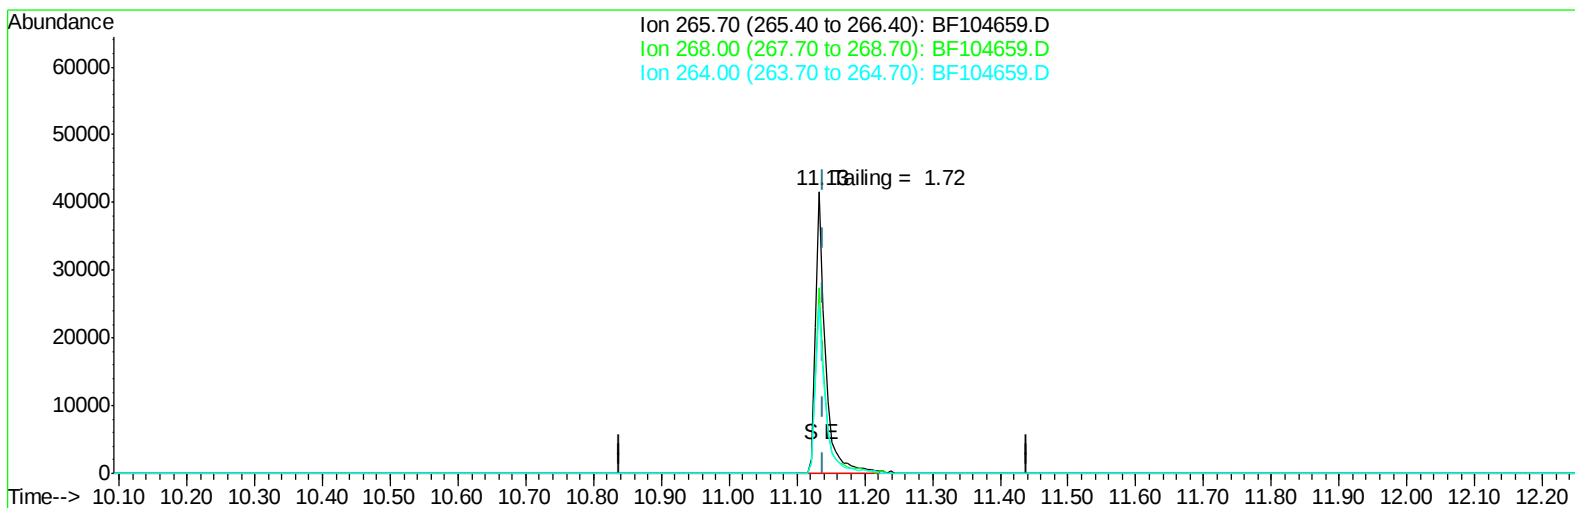

TIC: BF104659.D

(69) Pentachlorophenol (C)




11.133min (-0.006) 45071.82ng

response 42050

Ion	Exp%	Act%
265.70	100	100
268.00	63.90	66.13
264.00	61.90	59.50
0.00	0.00	0.00

Data Path : Z:\HPCHEM1\BNA F\DATA\BF041918\
Data File : BF104659.D
Acq On : 20 Apr 2018 5:59
Operator : JU/SJ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Apr 20 06:42:36 2018
Quant Method : Z:\HPCHEM1\BNA F\METHODS\8270-BF040618.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Apr 19 14:44:03 2018
Response via : Initial Calibration

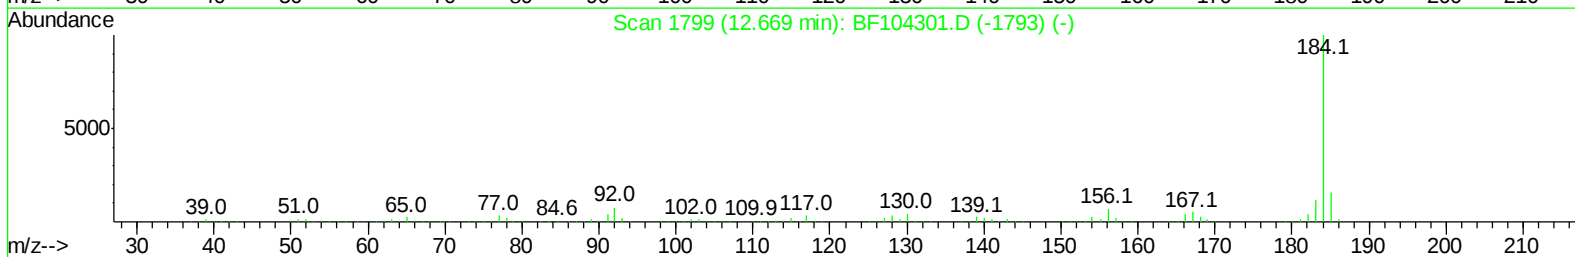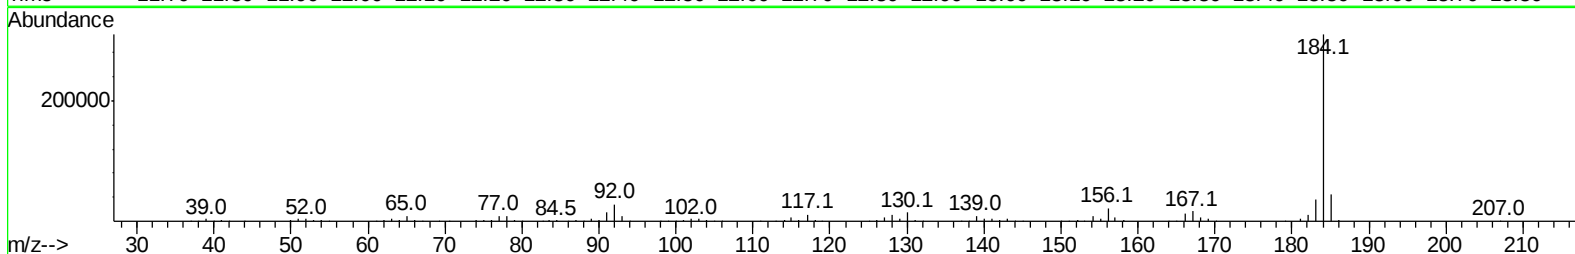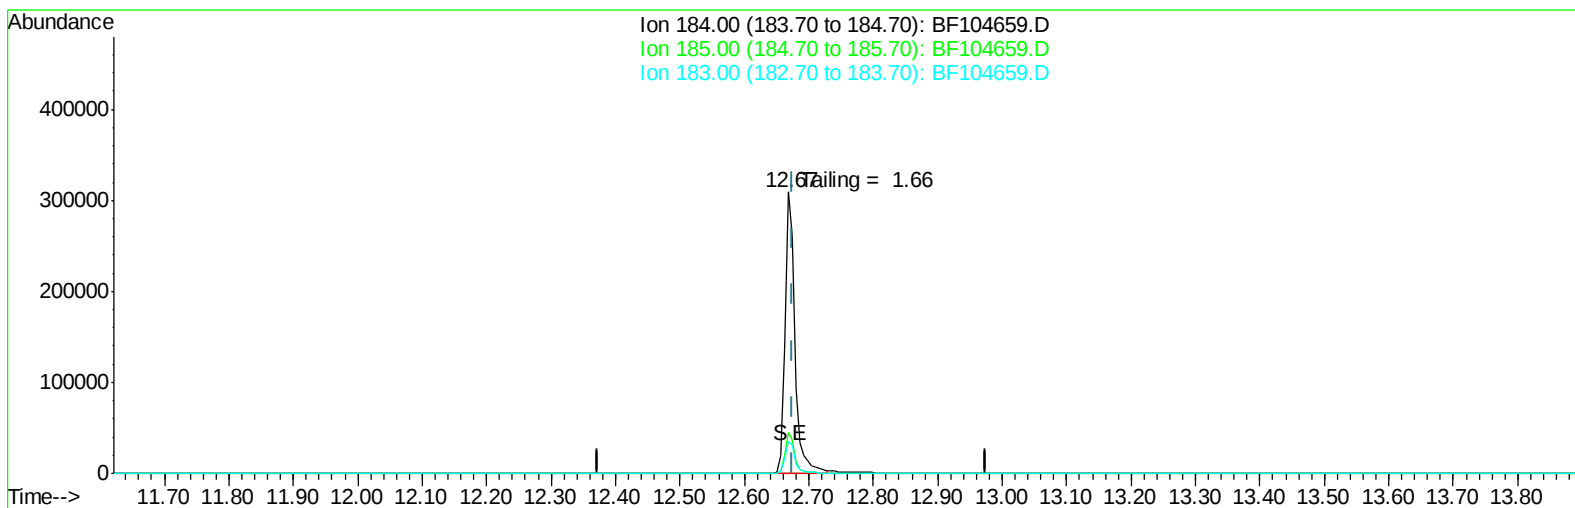

TIC: BF104659.D

(76) Benzidine

12.668min (-0.006) 0.00ng

response 331080

Ion	Exp%	Act%
184.00	100	100
185.00	15.70	14.62
183.00	11.60	11.51
0.00	0.00	0.00