


Data Path : Z:\HPCHEM1\BNA F\Data\BF041918\
 Data File : BF104631.D
 Acq On : 19 Apr 2018 16:40
 Operator : JU/SJ
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF040618.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Thu Apr 19 14:44:03 2018

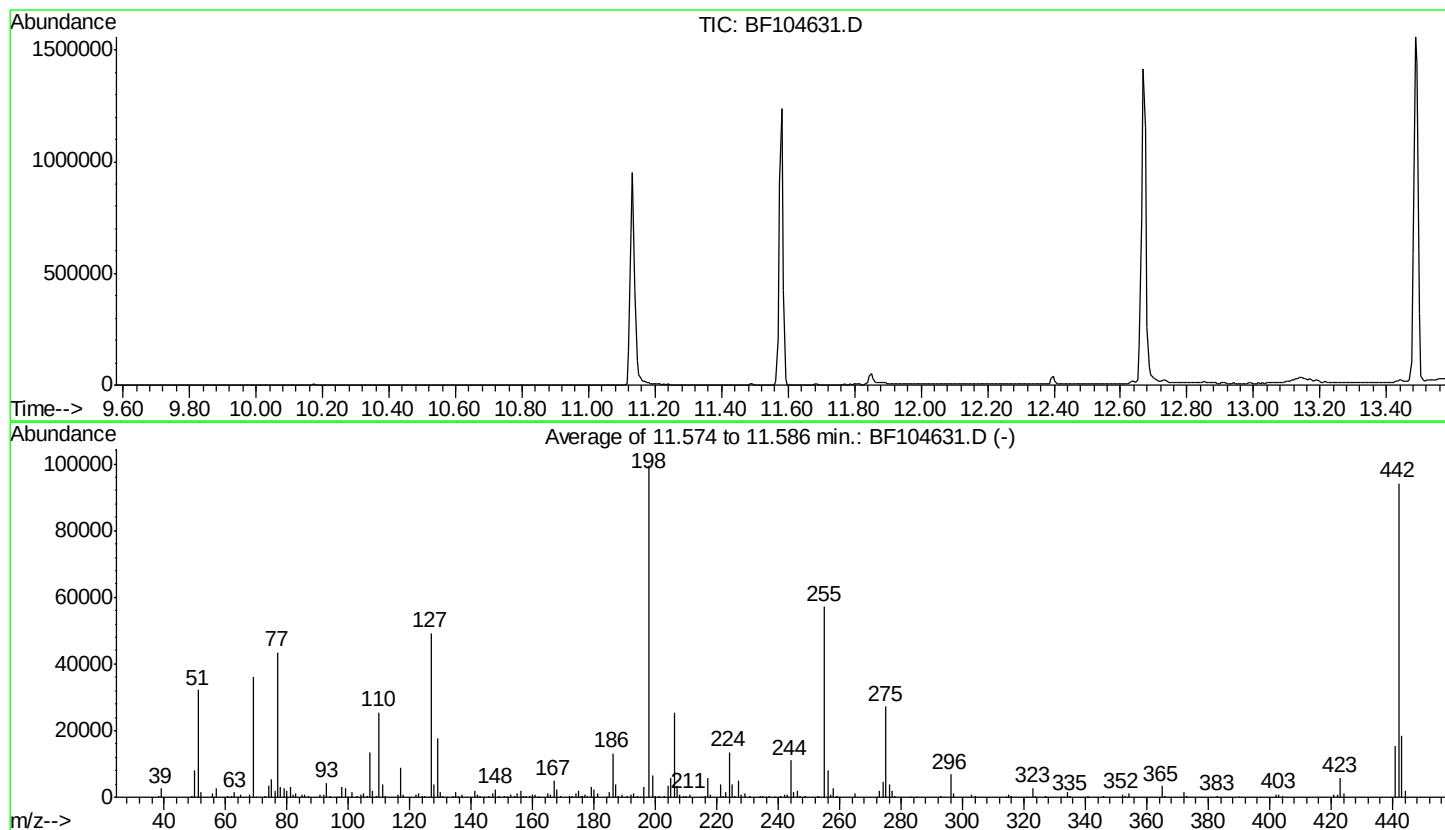

AutoFind: Scans 1613, 1614, 1615; Background Corrected with Scan 1607

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	32.3	32142	PASS
68	69	0.00	2	2.0	709	PASS
69	198	0.00	100	36.1	35925	PASS
70	69	0.00	2	0.4	128	PASS
127	198	10	80	49.6	49325	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	99493	PASS
199	198	5	9	6.5	6485	PASS
275	198	10	60	27.3	27189	PASS
365	198	1	100	3.4	3367	PASS
441	443	0.01	100	83.3	15313	PASS
442	198	50	100	94.8	94293	PASS
443	442	15	24	19.5	18390	PASS