


Data Path : Z:\HPCHEM1\BNA_F\Data\BF041918\
 Data File : BF104659.D
 Acq On : 20 Apr 2018 5:59
 Operator : JU/SJ
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF040618.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Thu Apr 19 14:44:03 2018

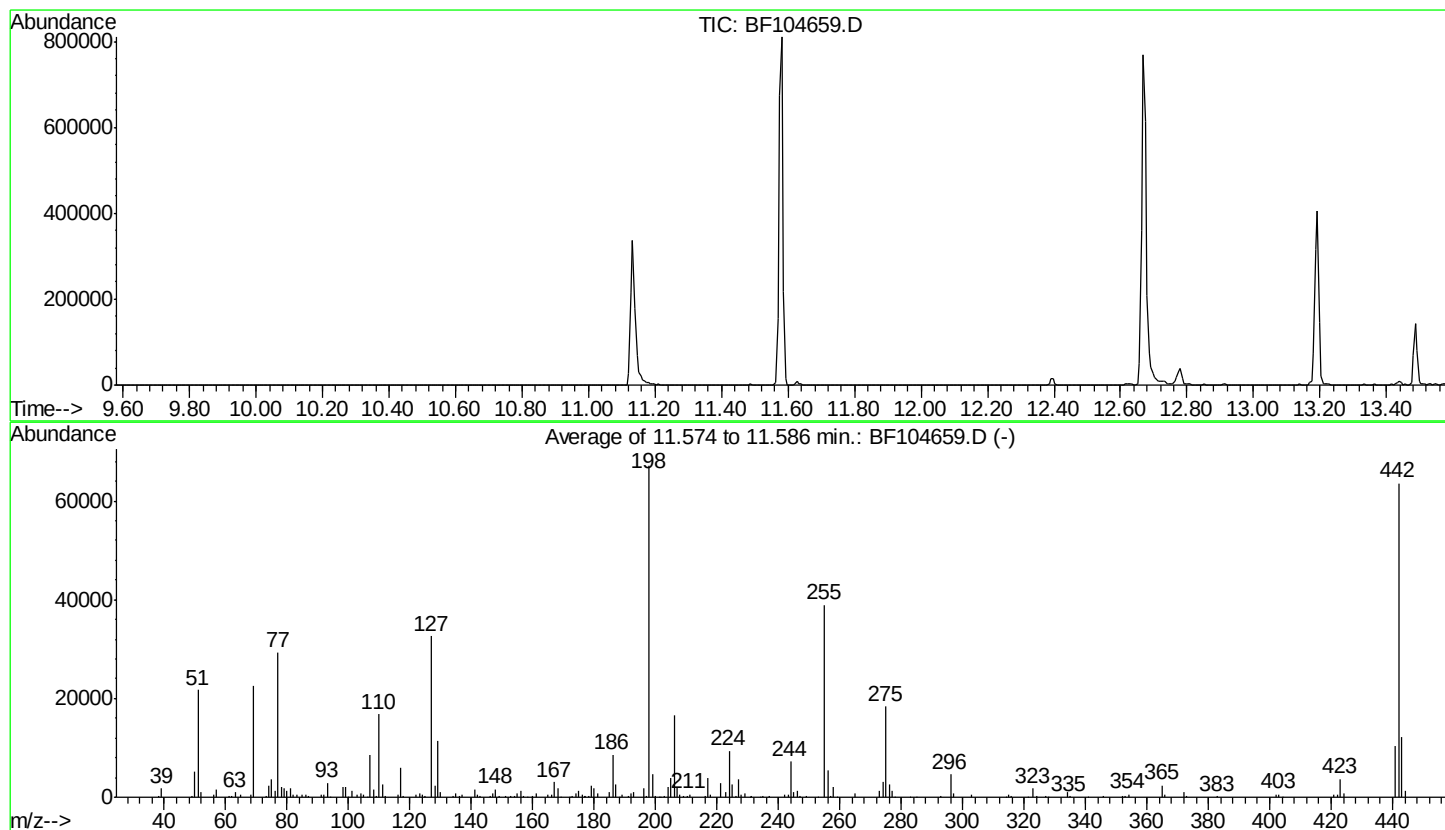

AutoFind: Scans 1613, 1614, 1615; Background Corrected with Scan 1608

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	32.3	21684	PASS
68	69	0.00	2	1.8	408	PASS
69	198	0.00	100	33.5	22500	PASS
70	69	0.00	2	0.0	0	PASS
127	198	10	80	48.6	32663	PASS
197	198	0.00	2	0.4	272	PASS
198	198	100	100	100.0	67160	PASS
199	198	5	9	6.8	4595	PASS
275	198	10	60	27.3	18329	PASS
365	198	1	100	3.6	2411	PASS
441	443	0.01	100	84.6	10409	PASS
442	198	50	100	94.7	63568	PASS
443	442	15	24	19.4	12305	PASS