


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF041921\
 Data File : BF123615.D
 Acq On : 19 Apr 2021 10:33
 Operator : JU/CG
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF041521.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Fri Apr 16 10:31:33 2021

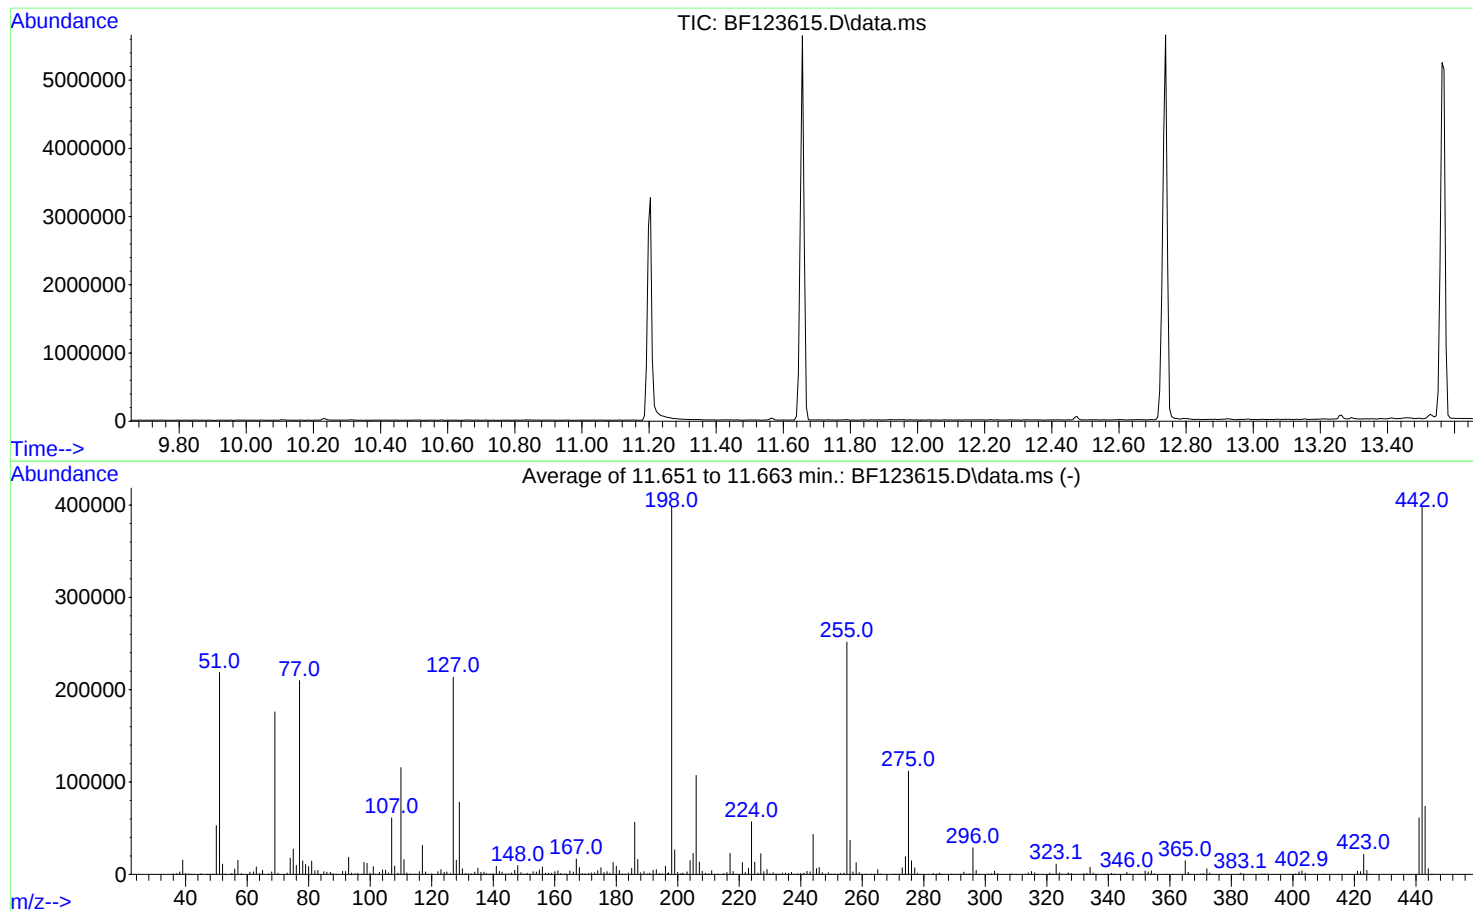




AutoFind: Scans 1626, 1627, 1628; Background Corrected with Scan 1620

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	54.9	218676	PASS
68	69	0.00	2	1.5	2562	PASS
69	198	0.00	100	44.2	175917	PASS
70	69	0.00	2	0.7	1203	PASS
127	198	10	80	53.6	213579	PASS
197	198	0.00	2	0.5	1829	PASS
198	198	100	100	100.0	398400	PASS
199	198	5	9	6.7	26500	PASS
275	198	10	60	28.1	111835	PASS
365	198	1	100	3.7	14789	PASS
441	198	0.01	100	15.3	61139	PASS
442	442	50	100	100.0	397632	PASS
443	442	15	24	18.6	73781	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF041921\
 Data File : BF123615.D
 Acq On : 19 Apr 2021 10:33
 Operator : JU/CG
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Quant Time: Apr 19 11:18:33 2021
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF041521.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Apr 16 10:31:33 2021
 Response via : Initial Calibration

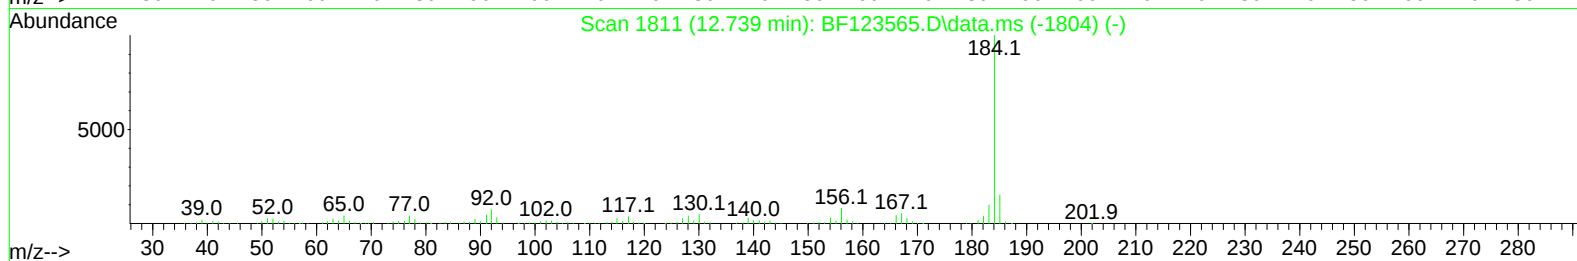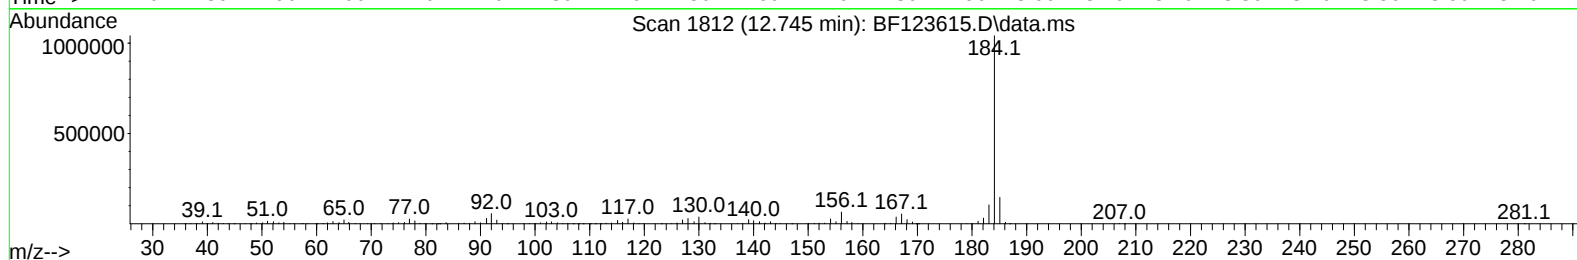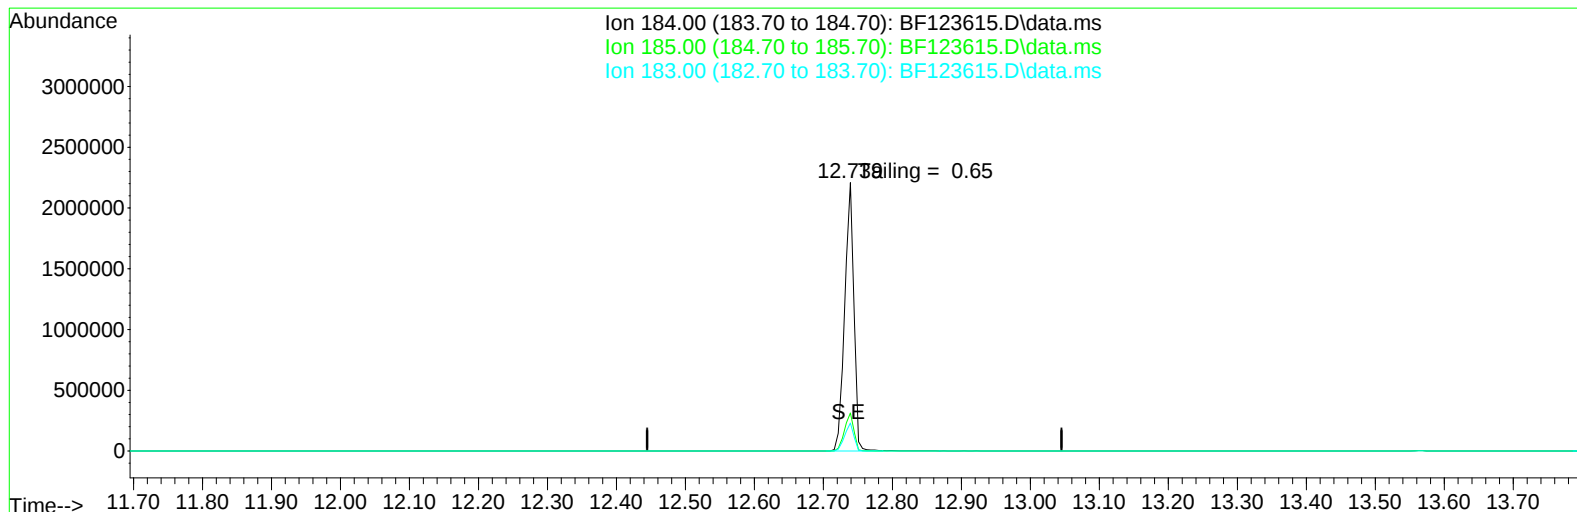

TIC: BF123615.D\data.ms

(77) Benzidine

12.745min (-12.745) 0.00 ng




response 0

Ion	Exp%	Act%
184.00	100.00	0.00
185.00	15.10	0.00#
183.00	9.80	0.00#
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF041921\
 Data File : BF123615.D
 Acq On : 19 Apr 2021 10:33
 Operator : JU/CG
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Quant Time: Apr 19 11:18:33 2021
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF041521.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Apr 16 10:31:33 2021
 Response via : Initial Calibration

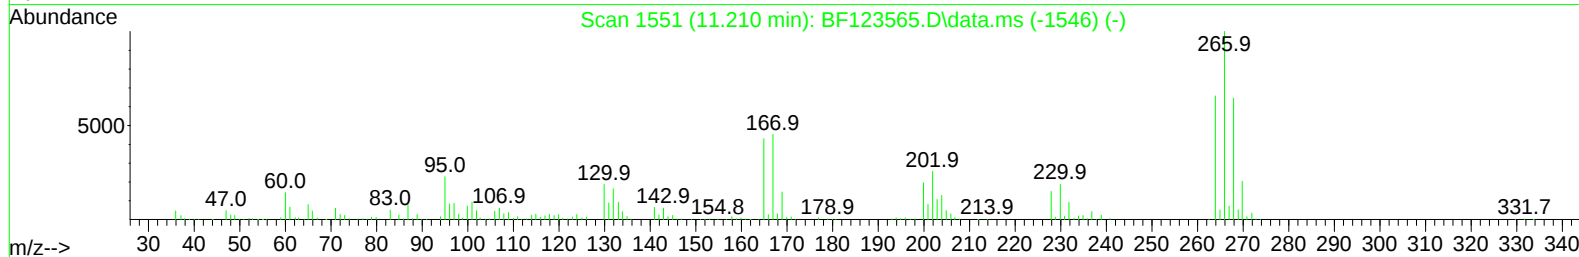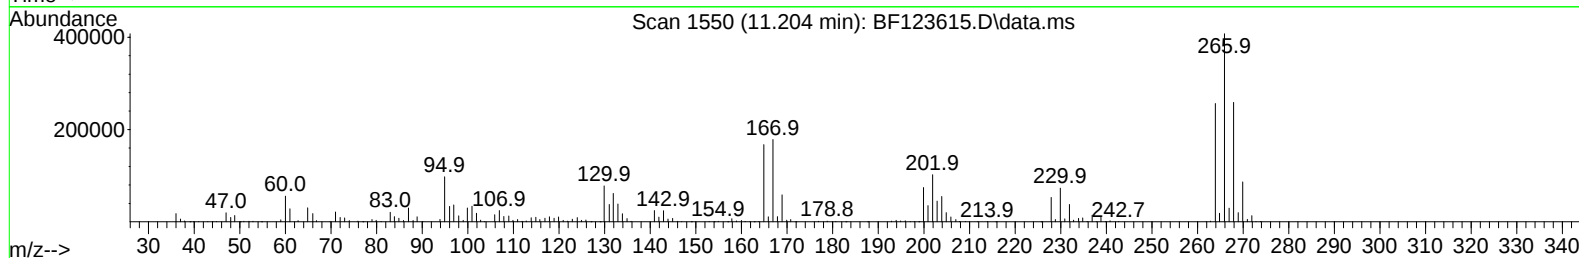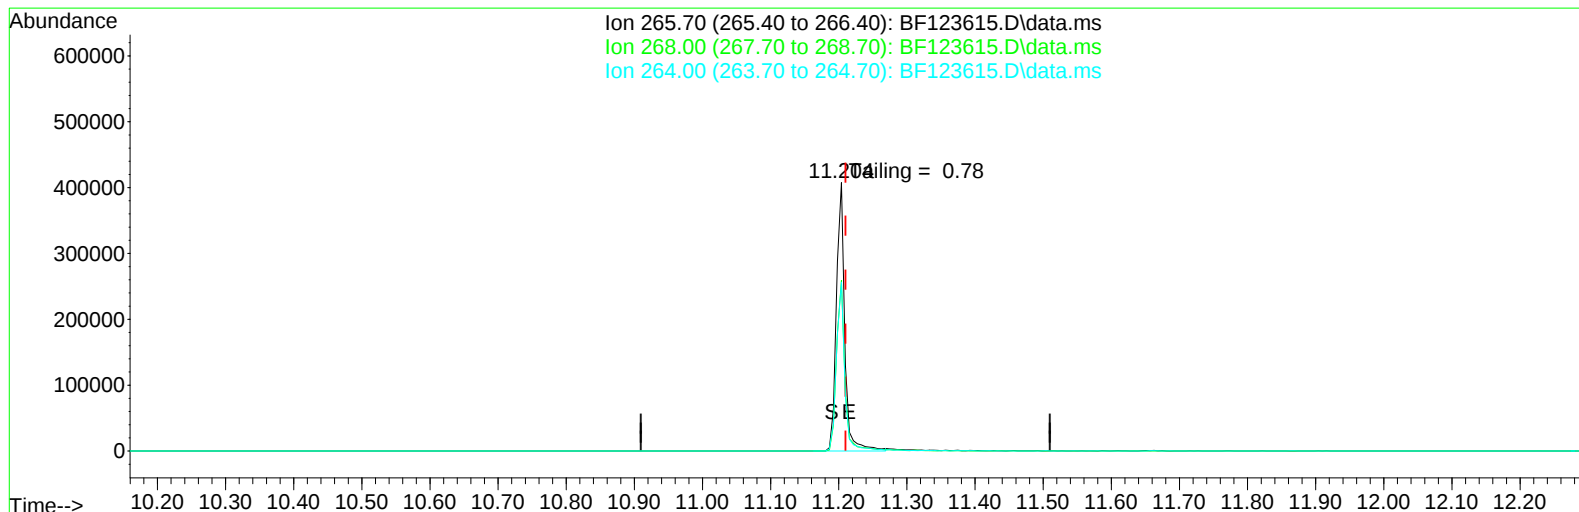

TIC: BF123615.D\data.ms

(70) Pentachlorophenol (C)

11.204min (-0.006) 510059.16 ng

response 351667

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	64.50	63.49
264.00	65.70	62.89
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
4/19/2021	BNA_F	BF123615.D
Compound Name	Response	Retention Time
DDT	914296	13.56
DDD	10393	13.26
DDE	1497	12.92
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
11890	926186	1.28

Instrument :
BNA_F
ClientSampleId :
DFTPP