
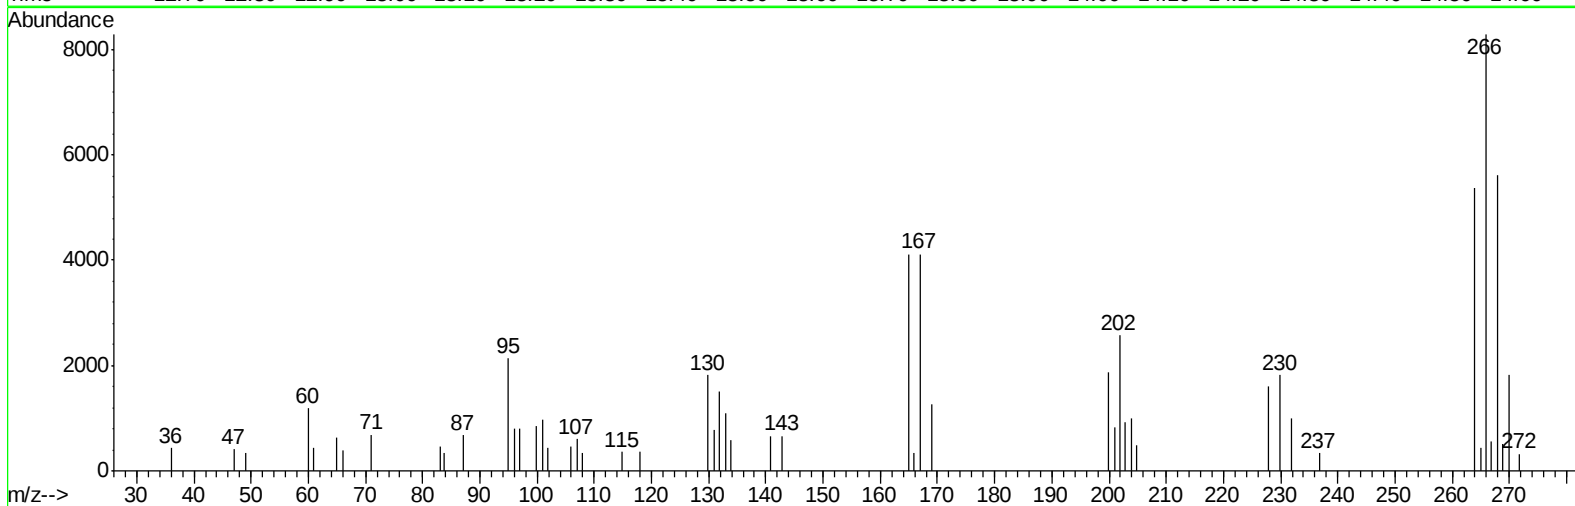


Data Path : Z:\HPCHEM1\BNA_F\DATA\BF042015\
Data File : BF078645.D
Acq On : 20 Apr 2015 14:50
Operator : TP/IZ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Apr 21 07:27:24 2015
Quant Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF040115.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Apr 21 03:43:19 2015
Response via : Initial Calibration

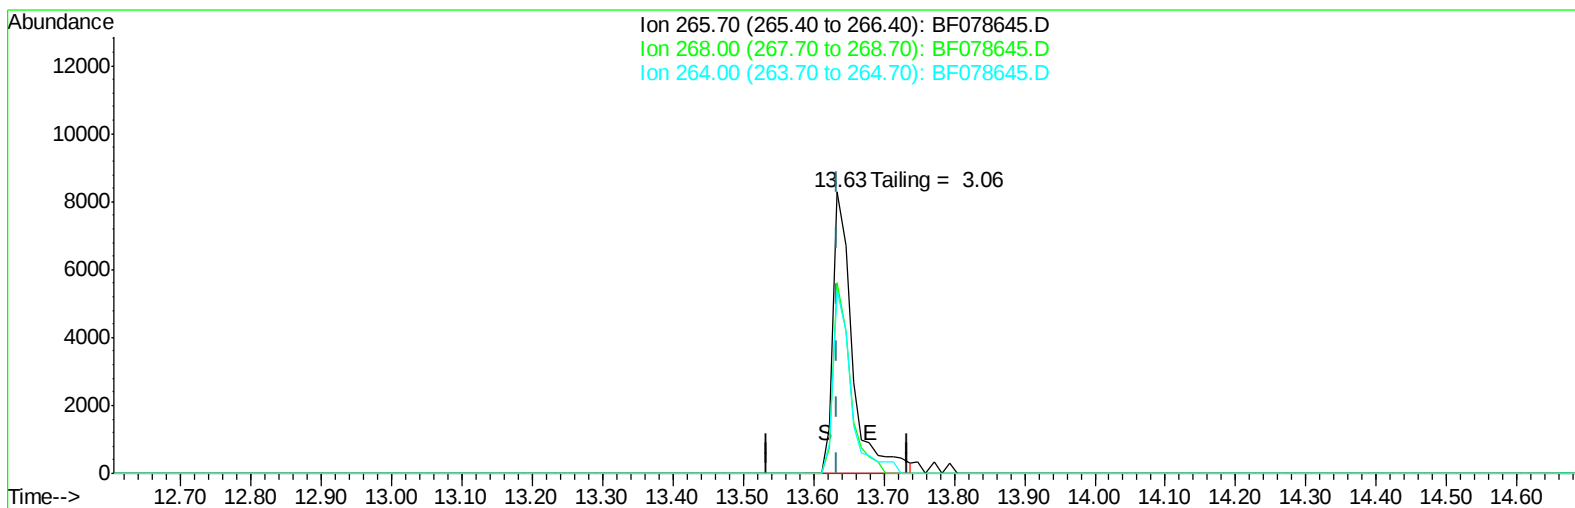

TIC: BF078645.D

(69) Pentachlorophenol (C)



13.634min (-0.000) 0.00ng

response 14709

Ion	Exp%	Act%
265.70	100	100
268.00	62.60	67.62
264.00	62.50	64.89
0.00	0.00	0.00

Data Path : Z:\HPCHEM1\BNA_F\DATA\BF042015\
Data File : BF078645.D
Acq On : 20 Apr 2015 14:50
Operator : TP/IZ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Apr 21 07:27:24 2015
Quant Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF040115.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Apr 21 03:43:19 2015
Response via : Initial Calibration

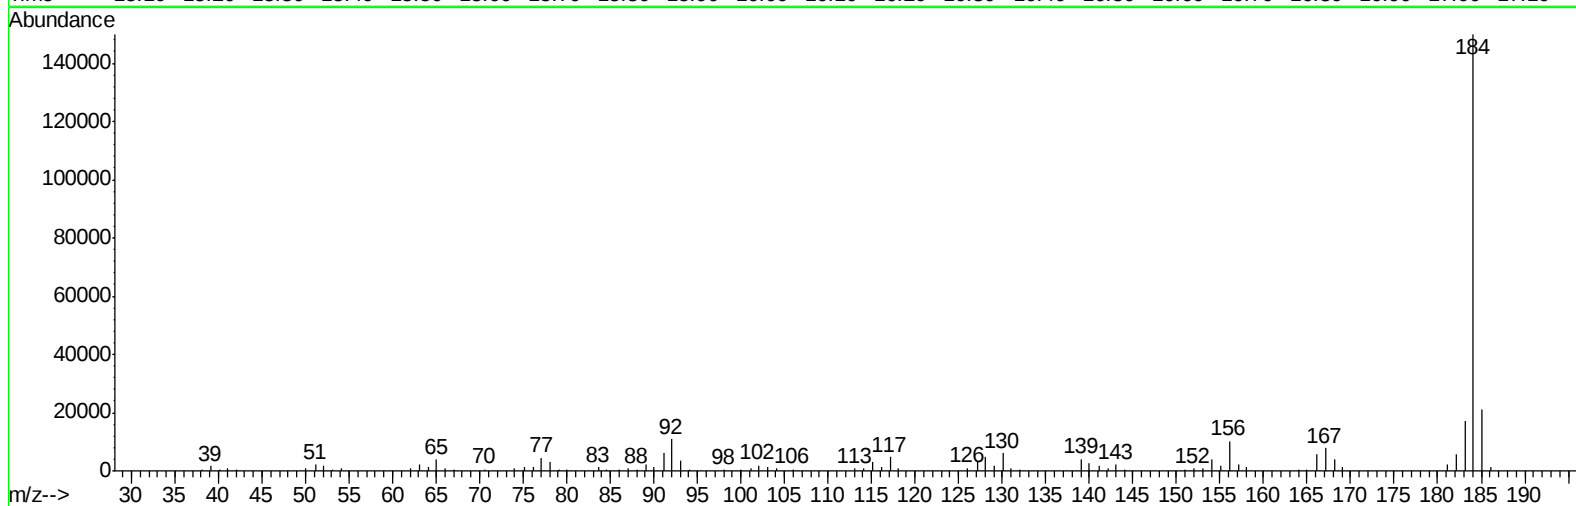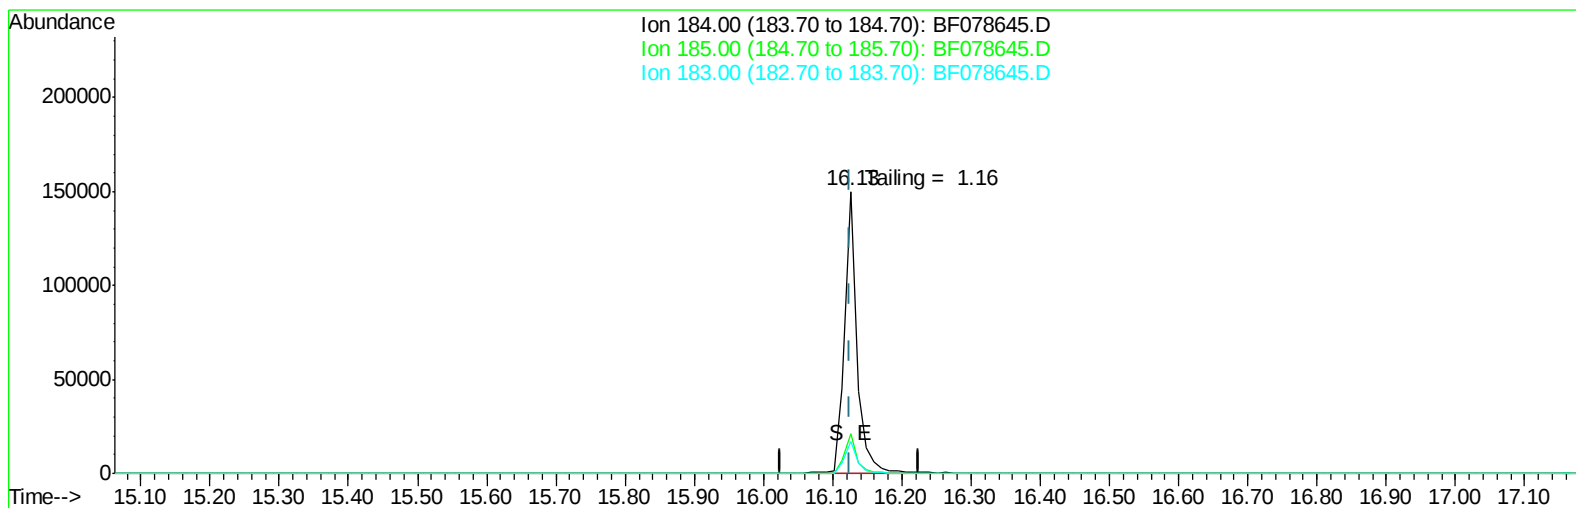

TIC: BF078645.D

(76) Benzidine

16.125min (-0.000) 0.00ng

response 182415

Ion	Exp%	Act%
184.00	100	100
185.00	15.20	14.03
183.00	11.90	11.51
0.00	0.00	0.00