
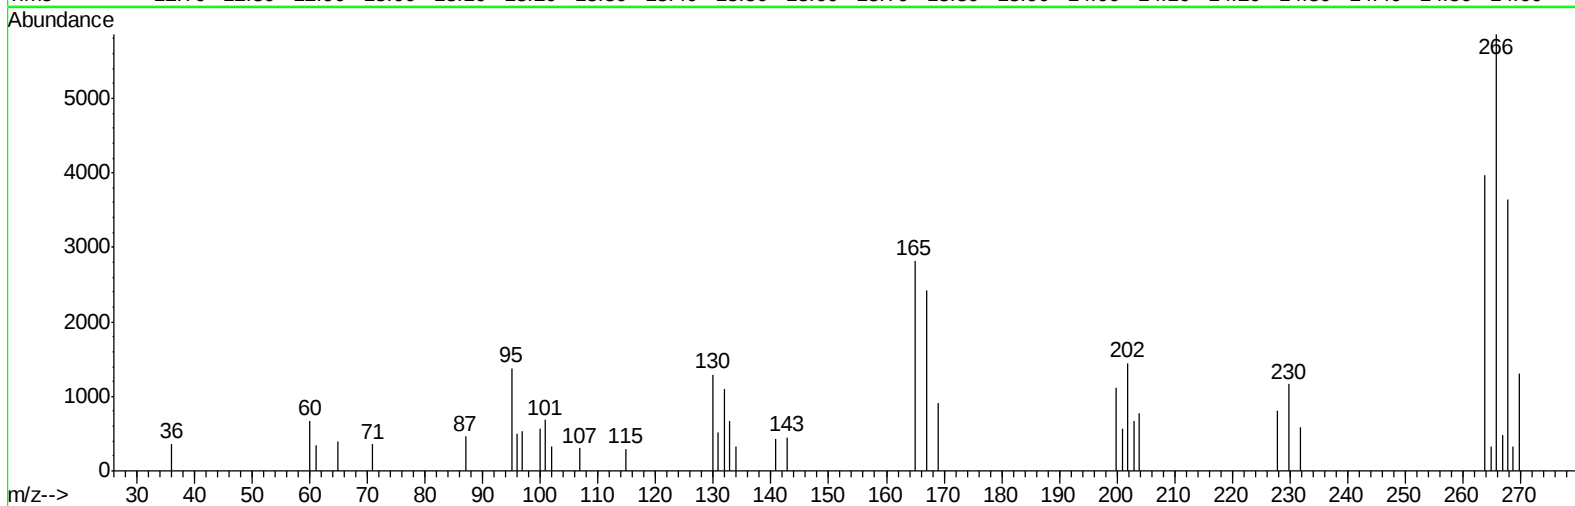


Data Path : Z:\HPCHEM1\BNA_F\DATA\BF042015\
Data File : BF078662.D
Acq On : 21 Apr 2015 1:45
Operator : TP/IZ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Apr 21 07:28:39 2015
Quant Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF040115.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Apr 21 03:43:19 2015
Response via : Initial Calibration

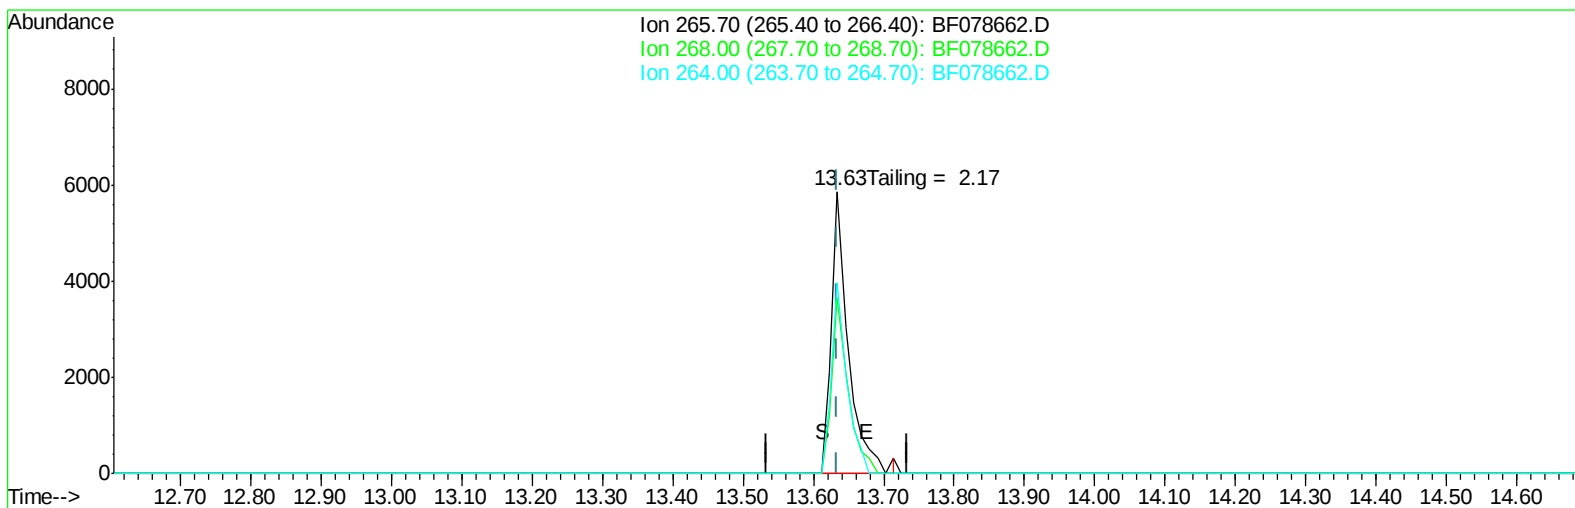

TIC: BF078662.D

(69) Pentachlorophenol (C)



13.634min (+0.000) 0.00ng

response 9664

Ion	Exp%	Act%
265.70	100	100
268.00	62.60	62.27
264.00	62.50	67.87
0.00	0.00	0.00

Data Path : Z:\HPCHEM1\BNA_F\DATA\BF042015\
Data File : BF078662.D
Acq On : 21 Apr 2015 1:45
Operator : TP/IZ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Apr 21 07:28:39 2015
Quant Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF040115.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Apr 21 03:43:19 2015
Response via : Initial Calibration

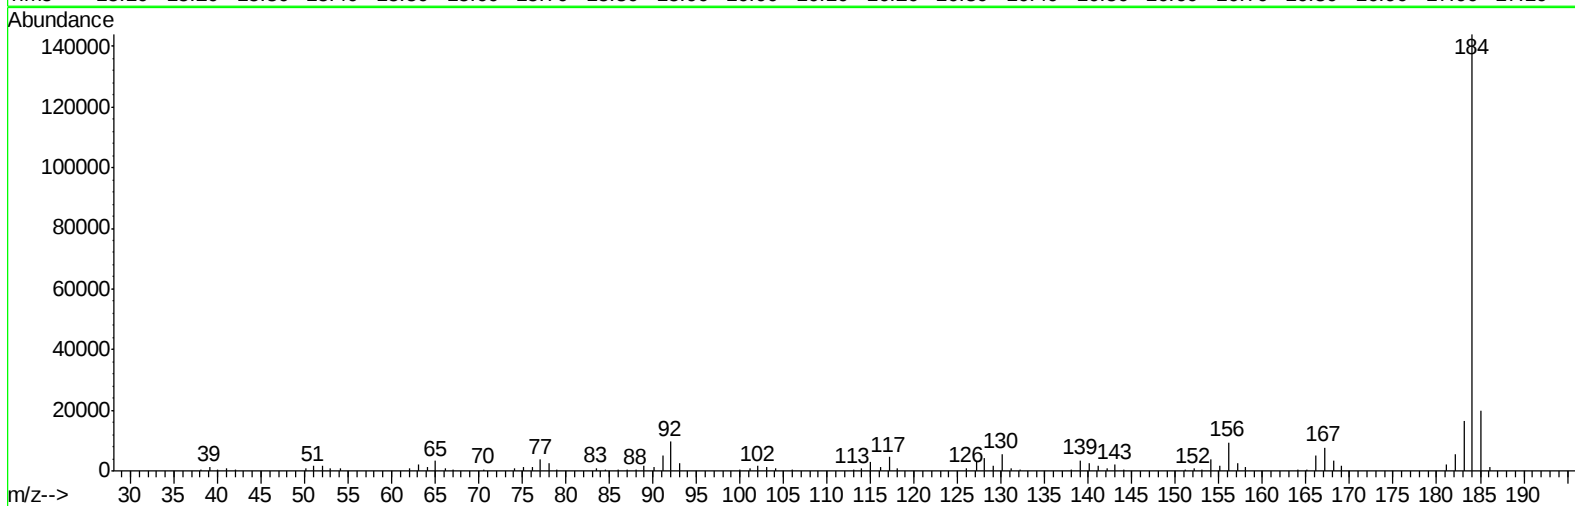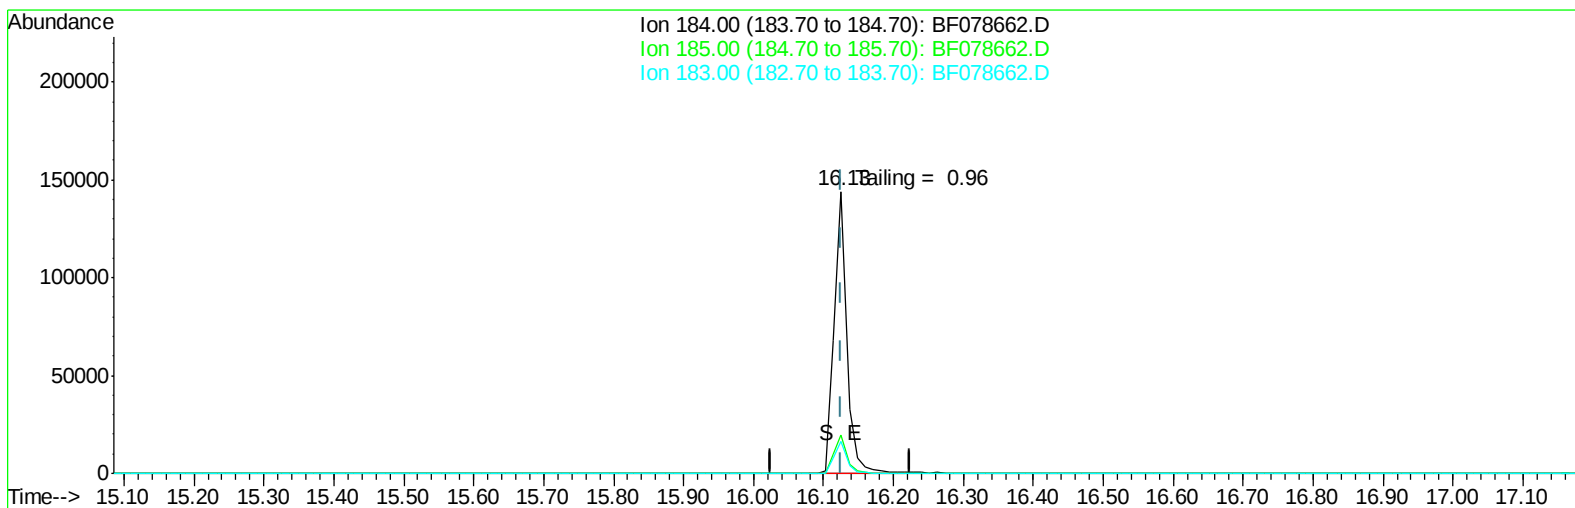

TIC: BF078662.D

(76) Benzidine

16.126min (+0.000) 0.00ng

response 177998

Ion	Exp%	Act%
184.00	100	100
185.00	15.20	13.77
183.00	11.90	11.51
0.00	0.00	0.00