


Data Path : Z:\HPCHEM1\BNA F\DATA\BF042015\
 Data File : BF078645.D
 Acq On : 20 Apr 2015 14:50
 Operator : TP/IZ
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA F\METHODS\8270-BF040115.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Tue Mar 31 14:58:34 2015

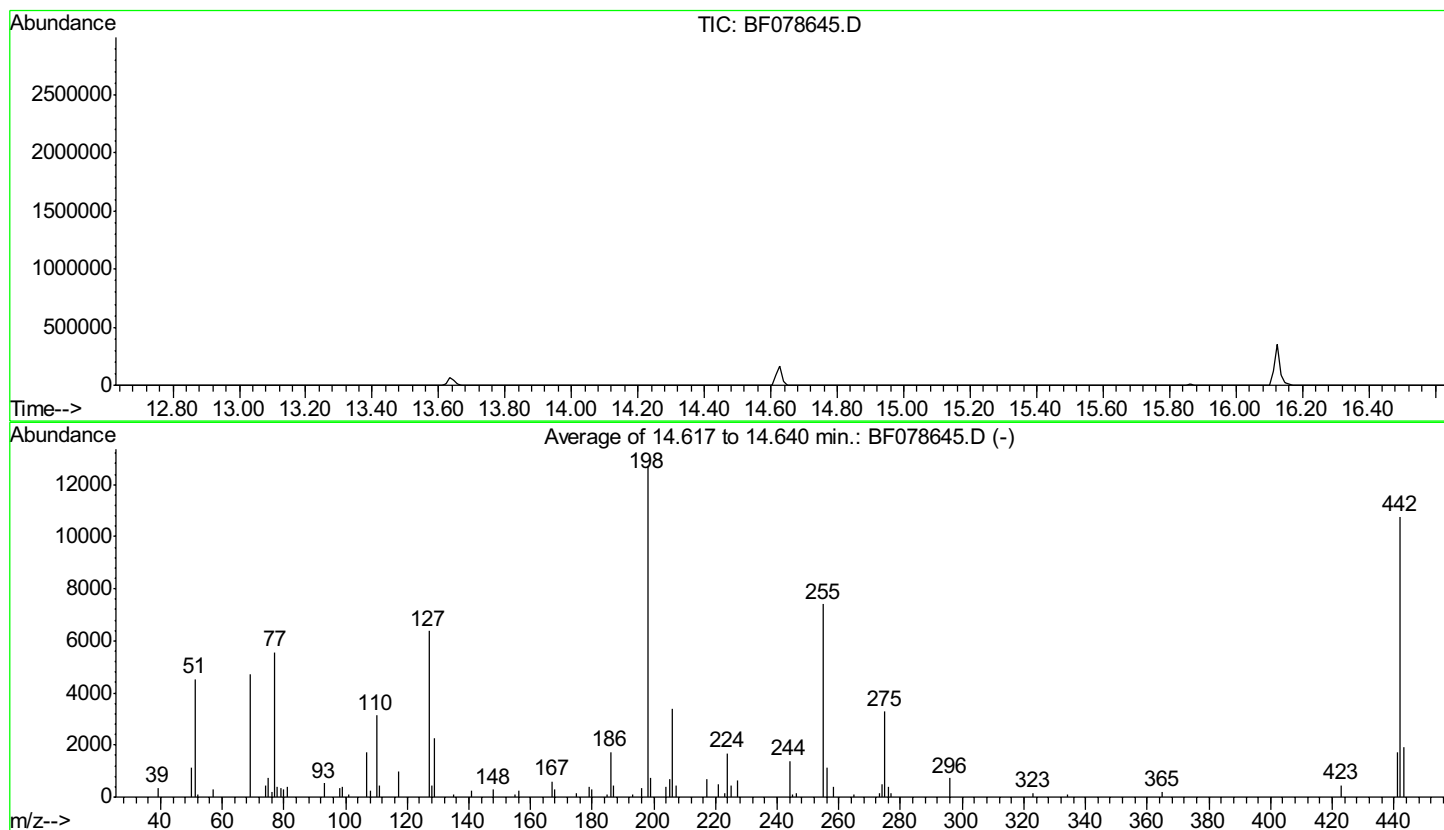

AutoFind: Scans 1175, 1176, 1177; Background Corrected with Scan 1171

Target	Rel. to	Lower	Upper	Rel.	Raw	Result
Mass	Mass	Limit%	Limit%	Abn%	Abn	Pass/Fail
51	198	10	80	35.6	4535	PASS
68	69	0.00	2	0.0	0	PASS
69	198	0.00	100	37.2	4731	PASS
70	69	0.00	2	0.0	0	PASS
127	198	10	80	50.2	6385	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	12724	PASS
199	198	5	9	5.9	756	PASS
275	198	10	60	25.8	3281	PASS
365	198	1	100	1.7	222	PASS
441	442	0.01	24	16.1	1736	PASS
442	198	50	100	84.6	10769	PASS
443	442	15	24	18.0	1941	PASS