


Data Path : Z:\HPCHEM1\BNA F\DATA\BF042015\  
Data File : BF078662.D  
Acq On : 21 Apr 2015 1:45  
Operator : TP/IZ  
Sample : DFTPP  
Misc :  
ALS Vial : 1 Sample Multiplier: 1

Instrument :  
BNA\_F  
ClientSampleId :  
DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA F\METHODS\8270-BF040115.M  
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION  
Last Update : Tue Mar 31 14:58:34 2015

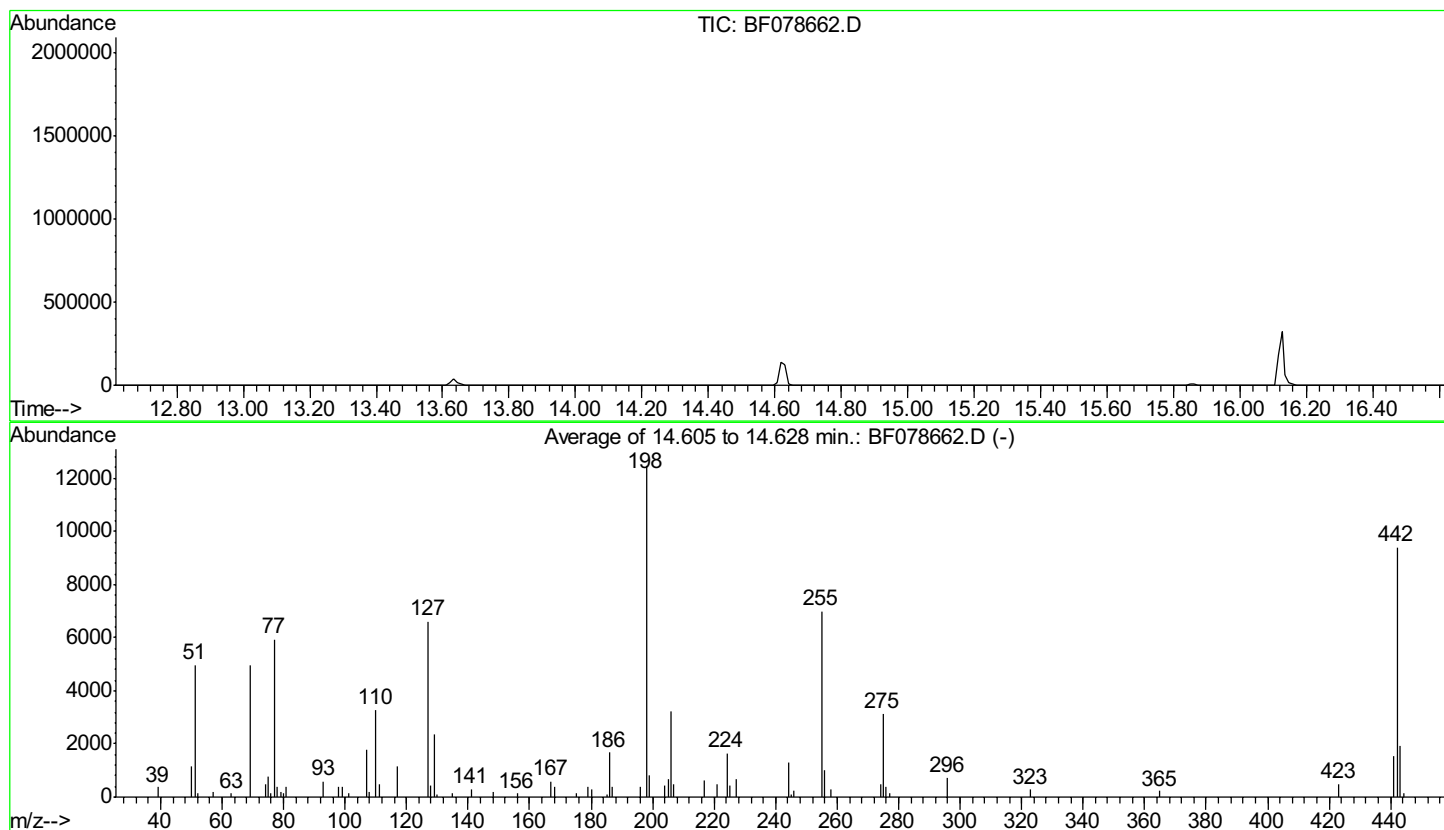

AutoFind: Scans 1174, 1175, 1176; Background Corrected with Scan 1171

| Target | Rel. to | Lower  | Upper  | Rel.  | Raw   | Result    |
|--------|---------|--------|--------|-------|-------|-----------|
| Mass   | Mass    | Limit% | Limit% | Abn%  | Abn   | Pass/Fail |
| 51     | 198     | 10     | 80     | 39.8  | 4961  | PASS      |
| 68     | 69      | 0.00   | 2      | 0.0   | 0     | PASS      |
| 69     | 198     | 0.00   | 100    | 39.8  | 4962  | PASS      |
| 70     | 69      | 0.00   | 2      | 0.0   | 0     | PASS      |
| 127    | 198     | 10     | 80     | 53.0  | 6612  | PASS      |
| 197    | 198     | 0.00   | 2      | 0.0   | 0     | PASS      |
| 198    | 198     | 100    | 100    | 100.0 | 12472 | PASS      |
| 199    | 198     | 5      | 9      | 6.5   | 816   | PASS      |
| 275    | 198     | 10     | 60     | 25.2  | 3141  | PASS      |
| 365    | 198     | 1      | 100    | 1.9   | 237   | PASS      |
| 441    | 442     | 0.01   | 24     | 16.2  | 1527  | PASS      |
| 442    | 198     | 50     | 100    | 75.4  | 9399  | PASS      |
| 443    | 442     | 15     | 24     | 20.3  | 1908  | PASS      |