


Data Path : Z:\HPCHEM1\BNA F\DATA\BF042016\
 Data File : BF086319.D
 Acq On : 20 Apr 2016 20:12
 Operator : UM/SJ
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF042016.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Wed Apr 20 15:45:26 2016

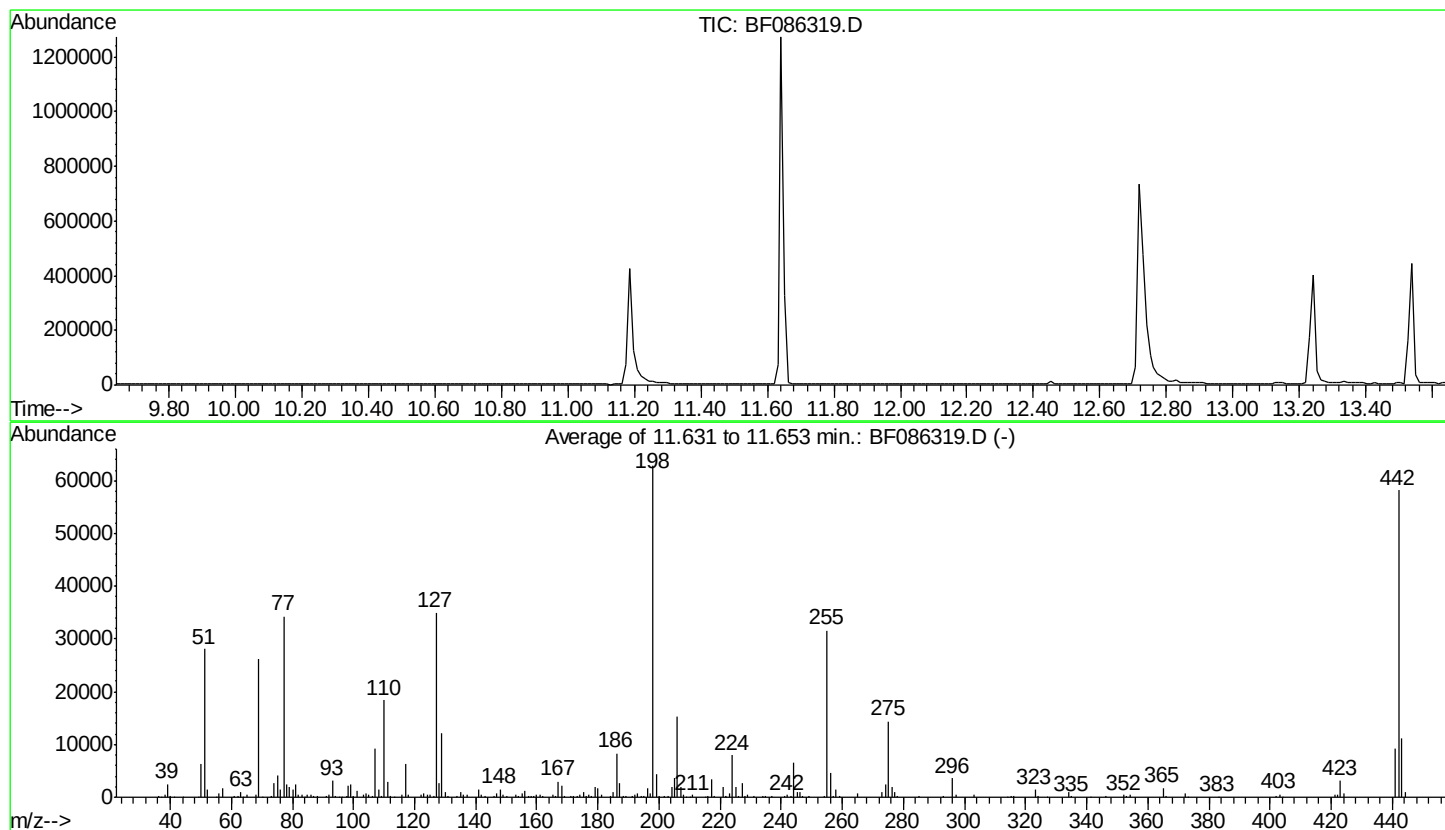

AutoFind: Scans 835, 836, 837; Background Corrected with Scan 832

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	44.7	28099	PASS
68	69	0.00	2	1.6	411	PASS
69	198	0.00	100	41.7	26219	PASS
70	69	0.00	2	0.4	117	PASS
127	198	10	80	55.8	35066	PASS
197	198	0.00	2	1.1	702	PASS
198	198	100	100	100.0	62869	PASS
199	198	5	9	6.9	4326	PASS
275	198	10	60	23.0	14438	PASS
365	198	1	100	2.8	1735	PASS
441	442	0.01	24	15.9	9277	PASS
442	198	50	100	92.5	58176	PASS
443	442	15	24	19.2	11191	PASS