
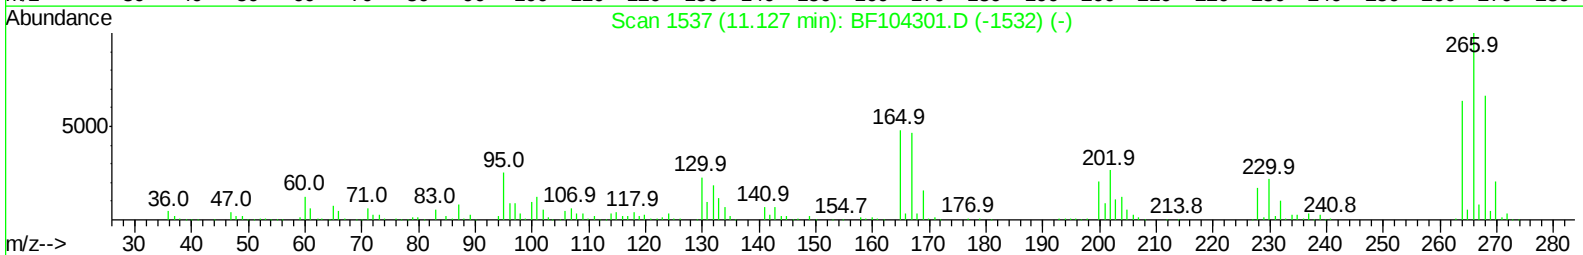
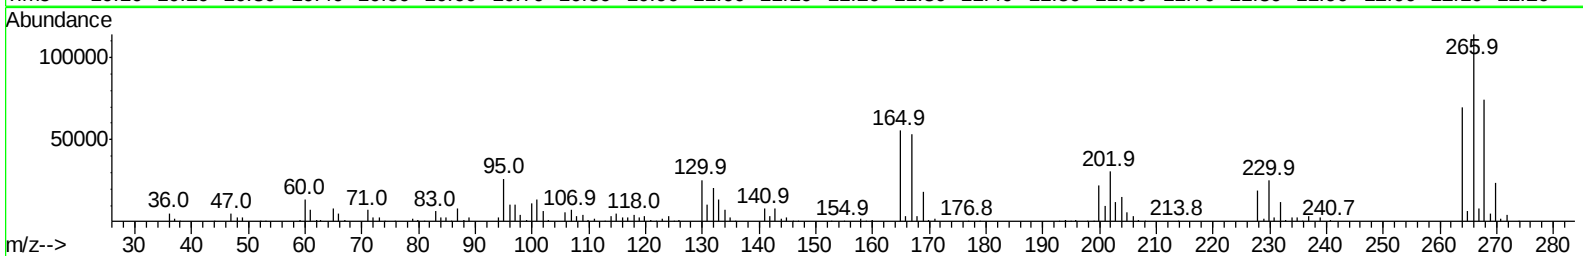


Data Path : Z:\HPCHEM1\BNA F\Data\BF042018\
Data File : BF104665.D
Acq On : 20 Apr 2018 10:53
Operator : JU/SJ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Apr 23 01:23:34 2018
Quant Method : Z:\HPCHEM1\BNA F\METHODS\8270-BF040618.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Apr 20 14:49:55 2018
Response via : Initial Calibration

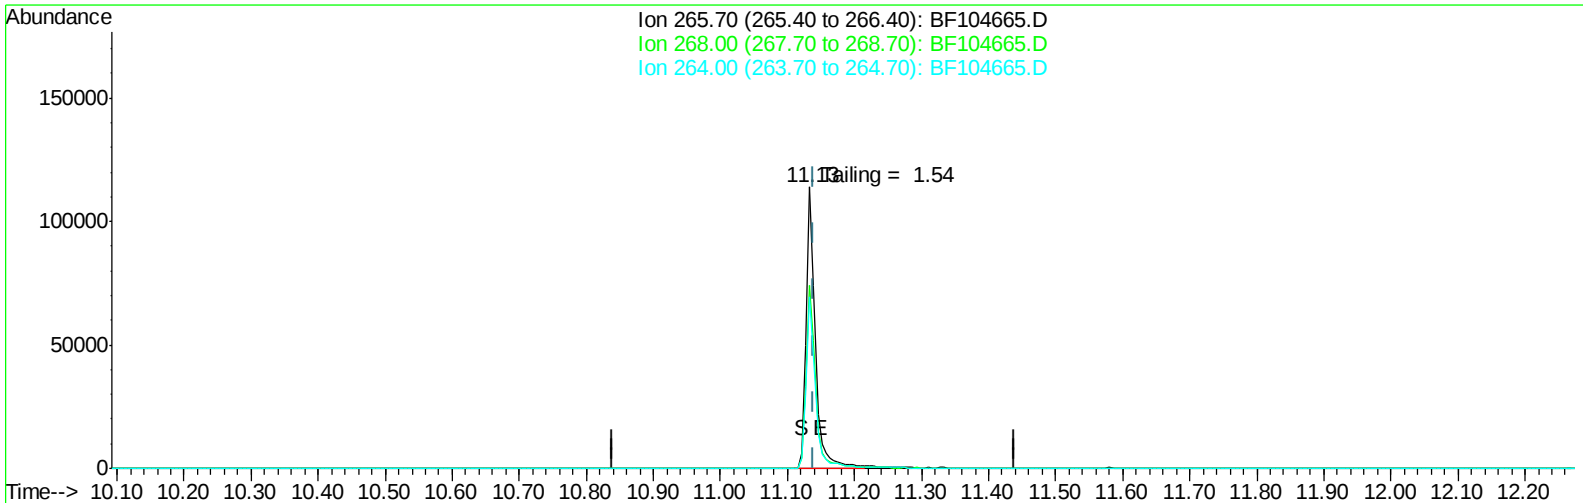

TIC: BF104665.D

(69) Pentachlorophenol (C)




11.133min (-0.006) 36814.08ng

response 108762

Ion	Exp%	Act%
265.70	100	100
268.00	63.90	64.91
264.00	61.90	60.97
0.00	0.00	0.00

Data Path : Z:\HPCHEM1\BNA F\Data\BF042018\
 Data File : BF104665.D
 Acq On : 20 Apr 2018 10:53
 Operator : JU/SJ
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Quant Time: Apr 23 01:23:34 2018
 Quant Method : Z:\HPCHEM1\BNA F\METHODS\8270-BF040618.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Apr 20 14:49:55 2018
 Response via : Initial Calibration

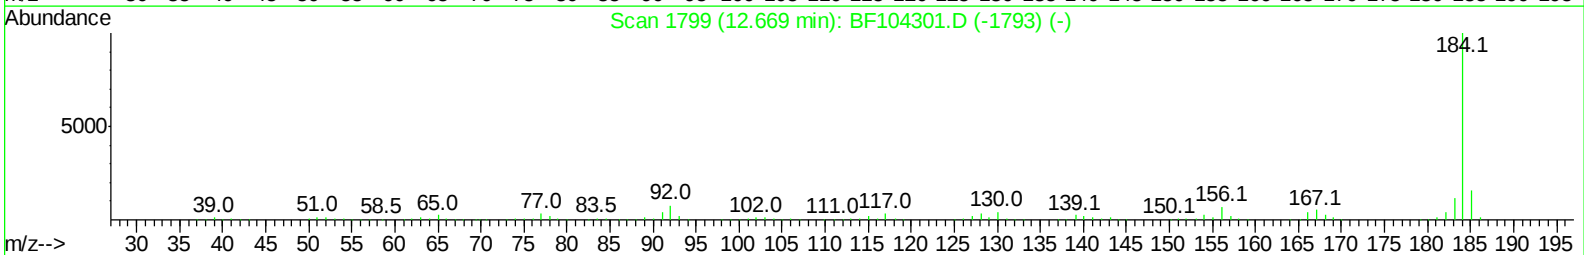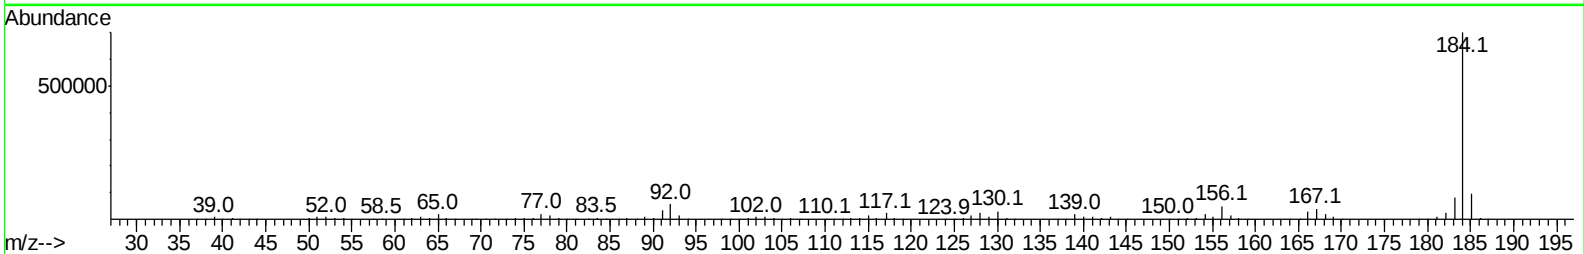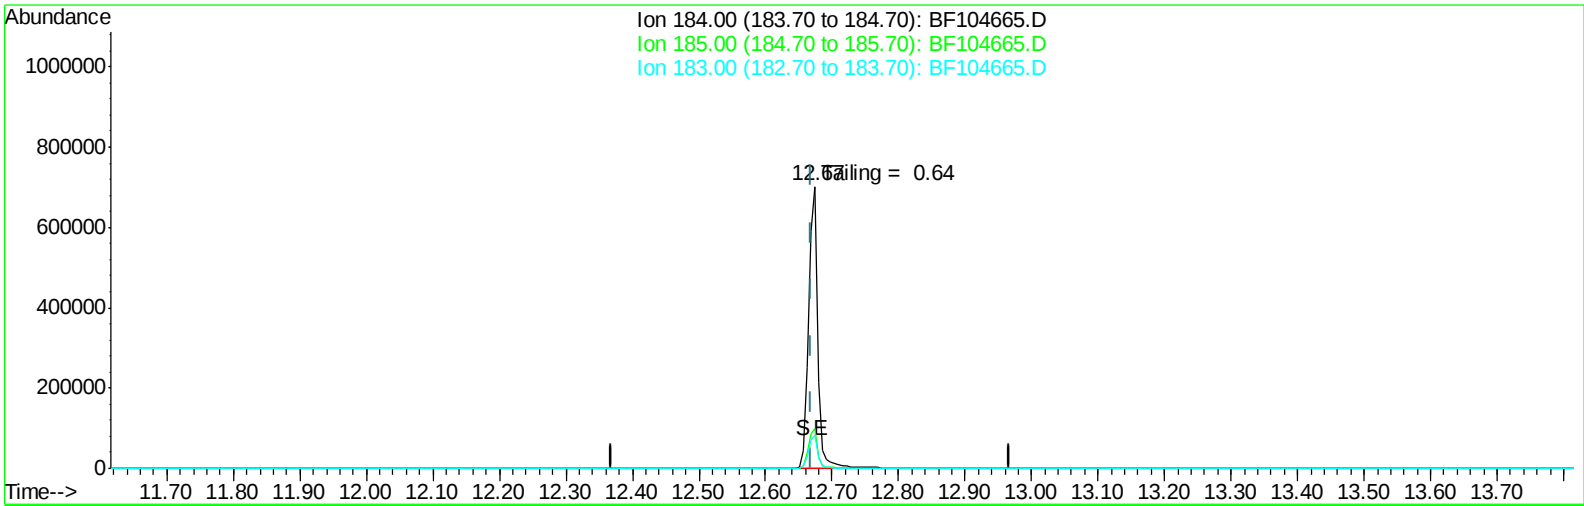

TIC: BF104665.D

(76) Benzidine

12.674min (+0.006) 0.00ng

response 687828

Ion	Exp%	Act%
184.00	100	100
185.00	15.70	14.00
183.00	11.60	11.99
0.00	0.00	0.00