


Data Path : Z:\HPCHEM1\BNA F\Data\BF042018\
 Data File : BF104665.D
 Acq On : 20 Apr 2018 10:53
 Operator : JU/SJ
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF040618.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Fri Apr 20 14:49:55 2018

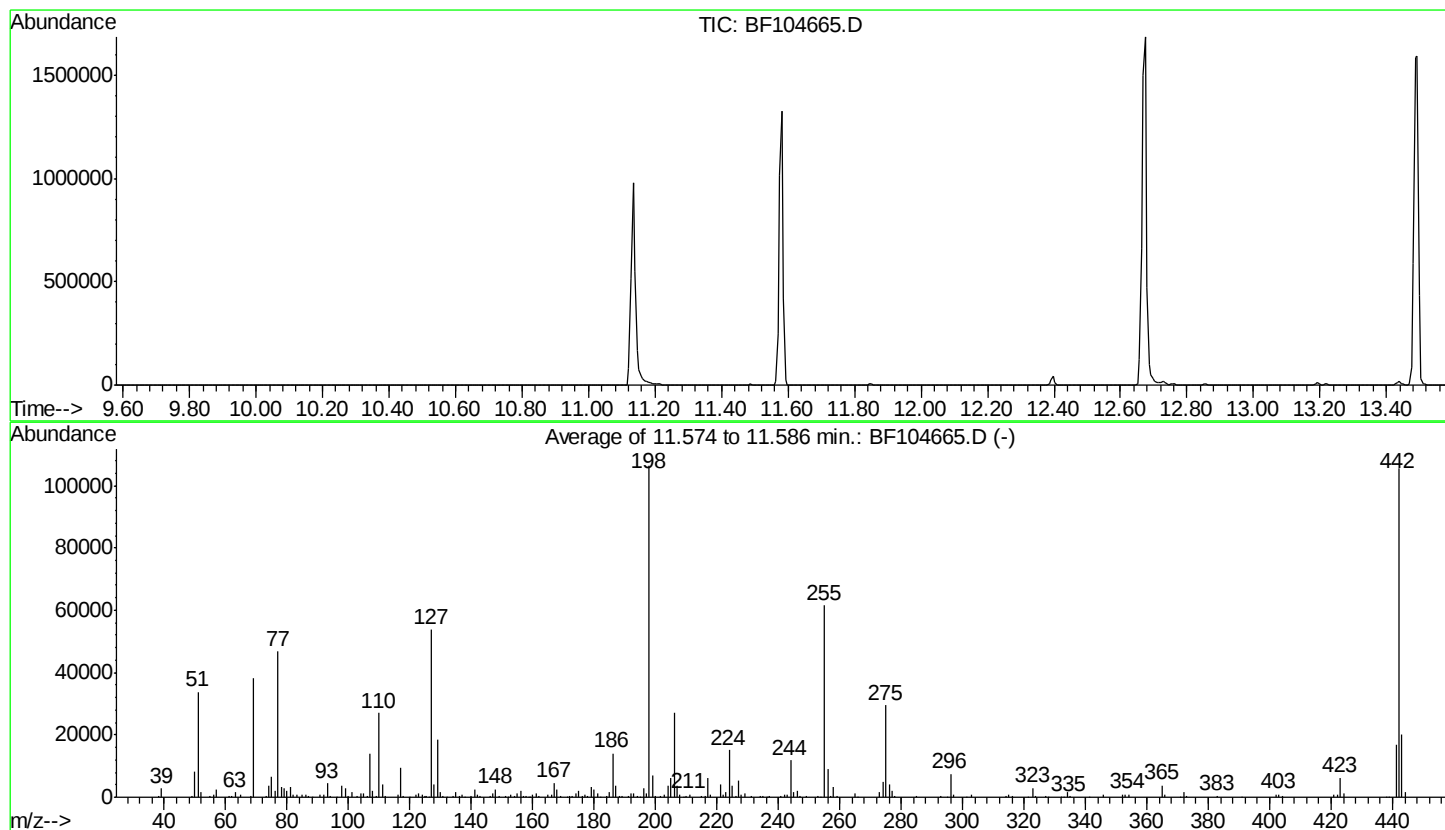

AutoFind: Scans 1613, 1614, 1615; Background Corrected with Scan 1608

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	31.7	33749	PASS
68	69	0.00	2	1.6	601	PASS
69	198	0.00	100	35.8	38101	PASS
70	69	0.00	2	0.0	0	PASS
127	198	10	80	50.5	53789	PASS
197	198	0.00	2	1.1	1160	PASS
198	198	100	100	100.0	106416	PASS
199	198	5	9	6.6	6987	PASS
275	198	10	60	27.7	29456	PASS
365	198	1	100	3.5	3756	PASS
441	443	0.01	100	84.4	16828	PASS
442	198	50	100	99.3	105677	PASS
443	442	15	24	18.9	19945	PASS