

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF042021\
 Data File : BF123654.D
 Acq On : 20 Apr 2021 21:22
 Operator : JU/CG
 Sample : M2076-15
 Misc :
 ALS Vial : 18 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 SB-17-14.5-15.0

Manual Integrations
 APPROVED

mohammad
 4/21/2021 11:25:30 AM

Quant Time: Apr 21 01:22:20 2021
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF041521.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue Apr 20 15:49:40 2021
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Dichlorobenzene-d4	6.851	152	235254	20.00	ng	0.00
21) Naphthalene-d8	8.134	136	909406	20.00	ng	# 0.00
39) Acenaphthene-d10	9.892	164	443243	20.00	ng	0.00
64) Phenanthrene-d10	11.380	188	826236	20.00	ng	0.00
76) Chrysene-d12	14.027	240	522863	20.00	ng	0.00
86) Perylene-d12	15.504	264	527962	20.00	ng	0.00
System Monitoring Compounds						
5) 2-Fluorophenol	5.475	112	1488916	102.29	ng	0.00
7) Phenol-d6	6.487	99	1890051	93.71	ng	0.00
23) Nitrobenzene-d5	7.410	82	1343272	67.90	ng	0.00
42) 2,4,6-Tribromophenol	10.680	330	522510	104.10	ng	0.00
45) 2-Fluorobiphenyl	9.210	172	2001771	67.32	ng	0.00
79) Terphenyl-d14	12.974	244	1842178	68.48	ng	0.00
Target Compounds						Qvalue
50) Dimethylphthalate	9.604	163	93529	3.05	ng	99
71) Phenanthrene	11.404	178	115127	2.67	ng	100
75) Fluoranthene	12.598	202	216848	4.58	ng	97
78) Pyrene	12.821	202	196766	5.16	ng	98
81) Benzo(a)anthracene	14.015	228	124642	3.89	ng	100
83) Chrysene	14.051	228	116066m	3.61	ng	
87) Indeno(1,2,3-cd)pyrene	16.974	276	57369	2.04	ng	# 91
88) Benzo(b)fluoranthene	15.068	252	130887m	3.51	ng	
90) Benzo(a)pyrene	15.439	252	99949	3.37	ng	95

(#) = qualifier out of range (m) = manual integration (+) = signals summed


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF042021\
Data File : BF123654.D
Acq On : 20 Apr 2021 21:22
Operator : JU/CG
Sample : M2076-15
Misc :
ALS Vial : 18 Sample Multiplier: 1


Instrument :
BNA_F
ClientSampleId :
SB-17-14.5-15.0

Manual Integrations
APPROVED

mohammad
4/21/2021 11:25:30 AM

Quant Time: Apr 21 01:22:20 2021
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF041521.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Apr 20 15:49:40 2021
Response via : Initial Calibration

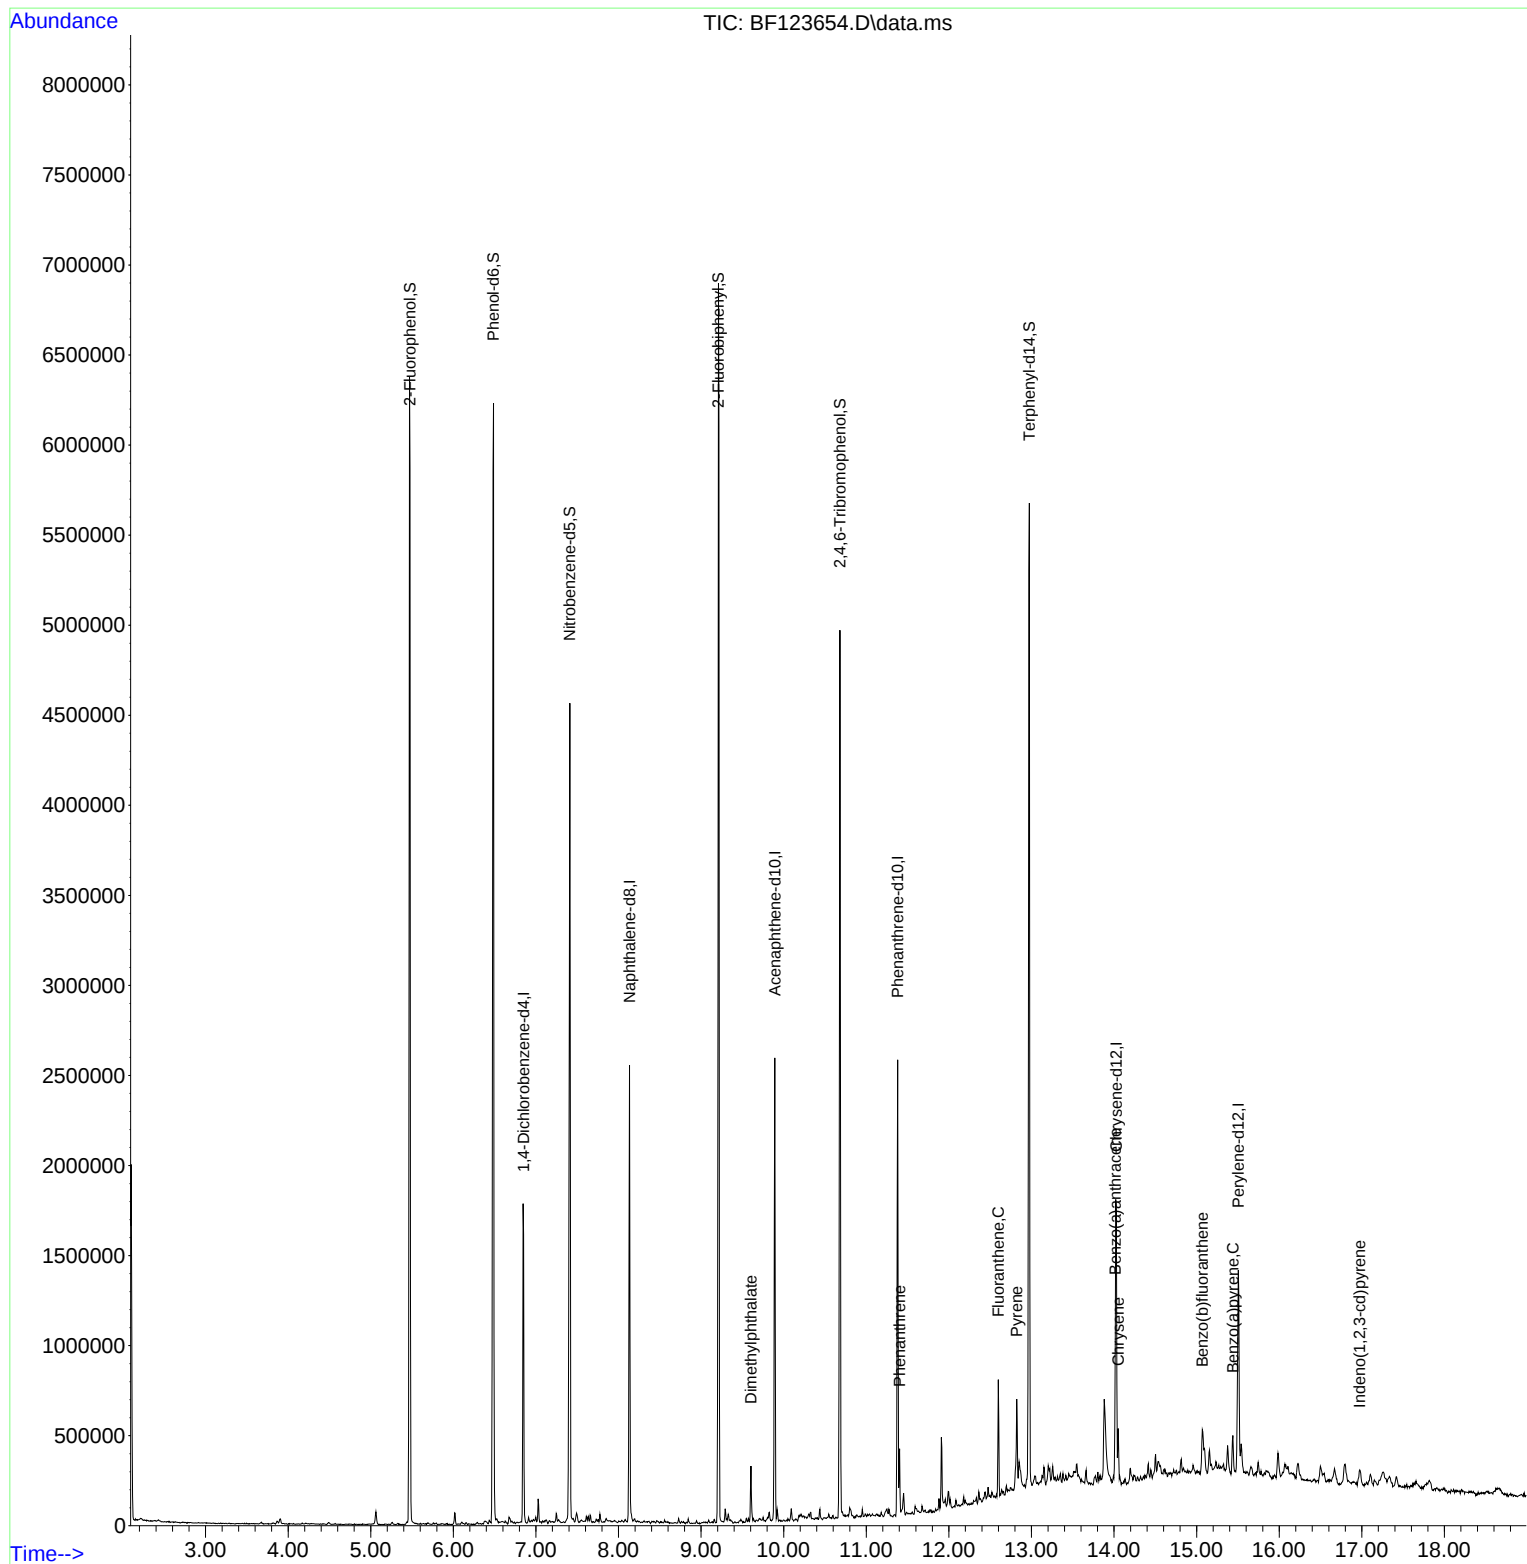







#1
1,4-Dichlorobenzene-d4
Concen: 20.00 ng
RT: 6.851 min Scan# 810
Delta R.T. 0.000 min
Lab File: BF123654.D
Acq: 20 Apr 2021 21:22

Tgt Ion:152 Resp: 235254
Ion Ratio Lower Upper
152 100
150 150.8 127.0 190.6
115 60.9 54.3 81.5

Instrument :
BNA_F
ClientSampleId :
SB-17-14.5-15.0




Manual Integrations
APPROVED


mohammad
4/21/2021 11:25:30 AM

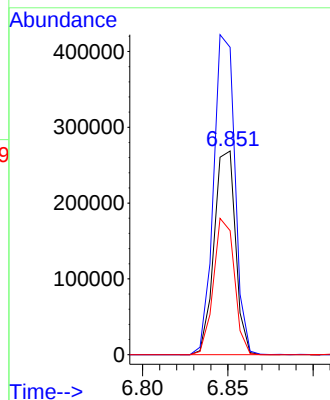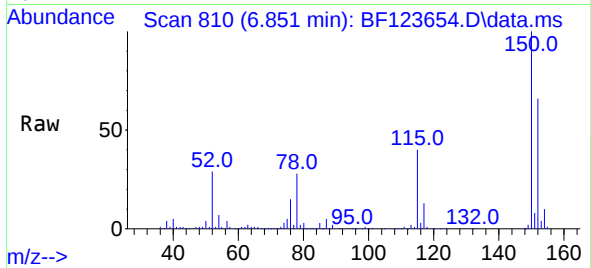

#5
2-Fluorophenol
Concen: 102.29 ng
RT: 5.475 min Scan# 576
Delta R.T. 0.006 min
Lab File: BF123654.D
Acq: 20 Apr 2021 21:22

Tgt Ion:112 Resp: 1488916
Ion Ratio Lower Upper
112 100
64 71.8 61.4 92.0
63 38.8 33.0 49.4

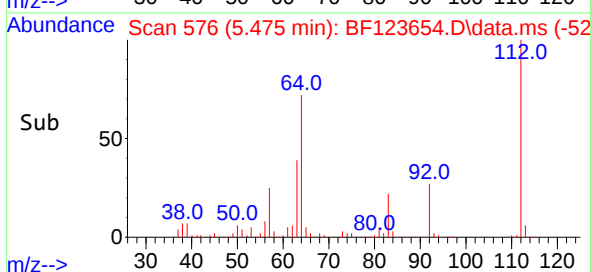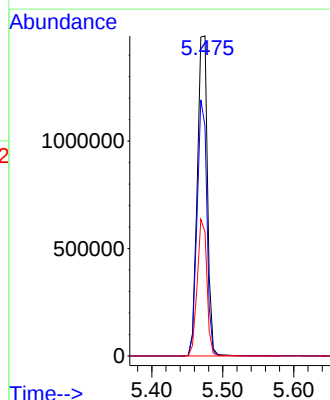



#7
Phenol-d6
Concen: 93.71 ng
RT: 6.487 min Scan# 748
Delta R.T. -0.006 min
Lab File: BF123654.D
Acq: 20 Apr 2021 21:22





Tgt Ion: 99 Resp: 1890051

Ion	Ratio	Lower	Upper
99	100		
42	23.7	19.8	29.8
71	38.7	31.1	46.7

Instrument :
BNA_F
ClientSampleId :
SB-17-14.5-15.0

Manual Integrations
APPROVED




mohammad
4/21/2021 11:25:30 AM

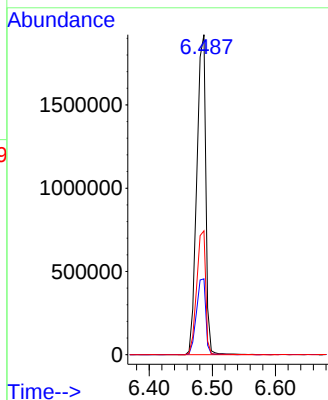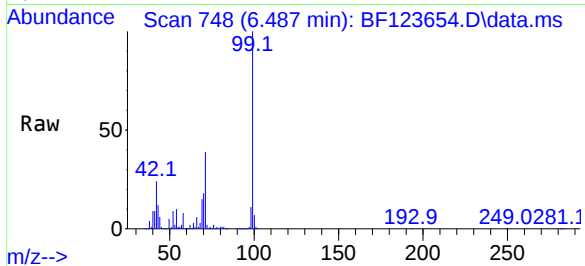


#21
Naphthalene-d8
Concen: 20.00 ng
RT: 8.134 min Scan# 1028
Delta R.T. -0.006 min
Lab File: BF123654.D
Acq: 20 Apr 2021 21:22

Tgt Ion: 136 Resp: 909406

Ion	Ratio	Lower	Upper
136	100		
137	11.1	8.7	13.1
54	11.8	9.8	14.6
68	6.2	4.1	6.1

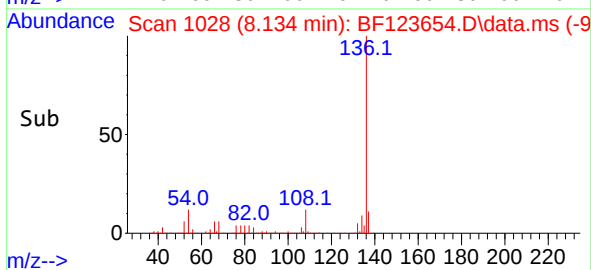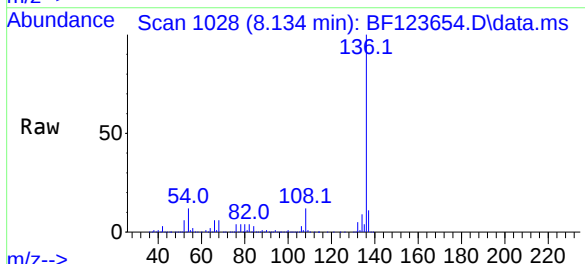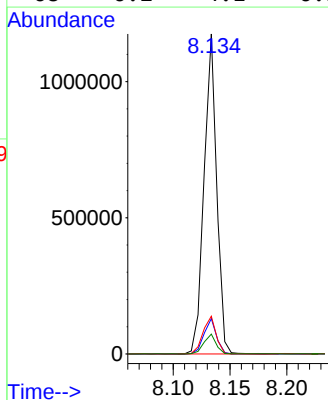

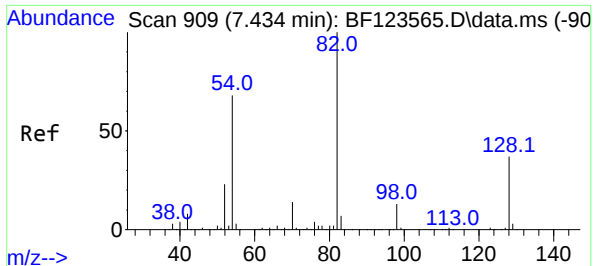

#23
Nitrobenzene-d5
Concen: 67.90 ng
RT: 7.410 min Scan# 905
Delta R.T. -0.006 min
Lab File: BF123654.D
Acq: 20 Apr 2021 21:22





Tgt Ion: 82 Resp: 1343272

Ion	Ratio	Lower	Upper
82	100		
128	38.0	29.4	44.2
54	64.2	54.1	81.1

Instrument :
BNA_F
ClientSampleId :
SB-17-14.5-15.0

Manual Integrations
APPROVED




mohammad
4/21/2021 11:25:30 AM

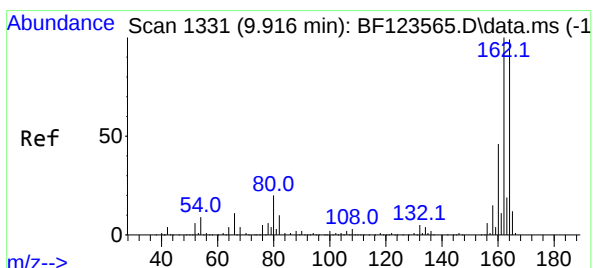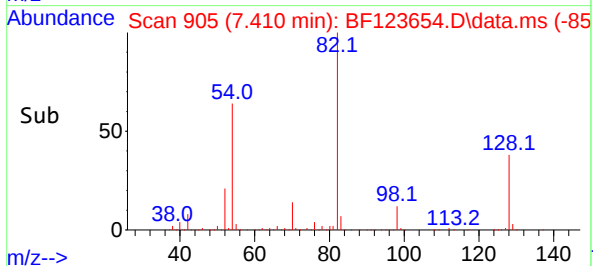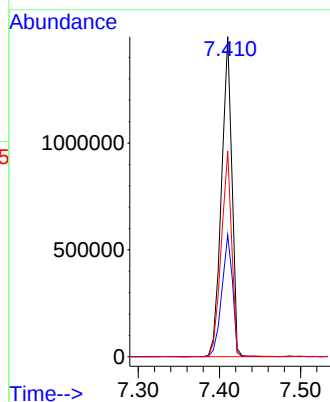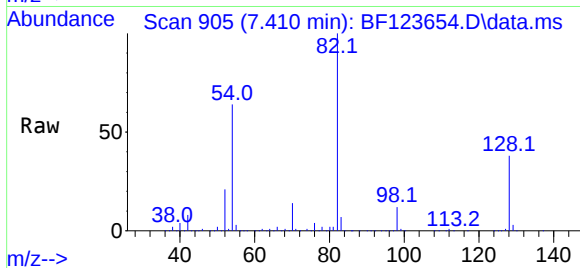

#39
Acenaphthene-d10
Concen: 20.00 ng
RT: 9.892 min Scan# 1327
Delta R.T. -0.006 min
Lab File: BF123654.D
Acq: 20 Apr 2021 21:22

Tgt Ion:164 Resp: 443243


Ion	Ratio	Lower	Upper
164	100		
162	102.2	80.7	121.1
160	46.0	37.3	55.9

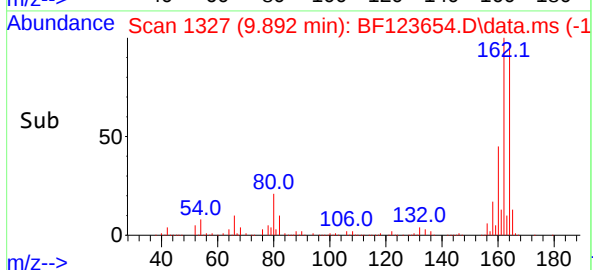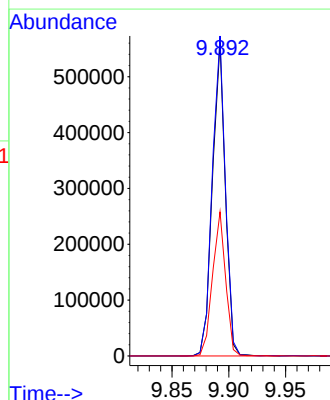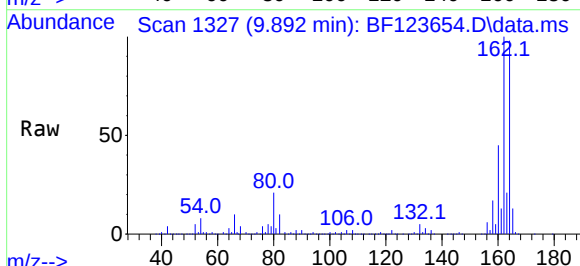



#42
2,4,6-Tribromophenol
Concen: 104.10 ng
RT: 10.680 min Scan# 1461
Delta R.T. -0.006 min
Lab File: BF123654.D
Acq: 20 Apr 2021 21:22




Instrument :
BNA_F
ClientSampleId :
SB-17-14.5-15.0

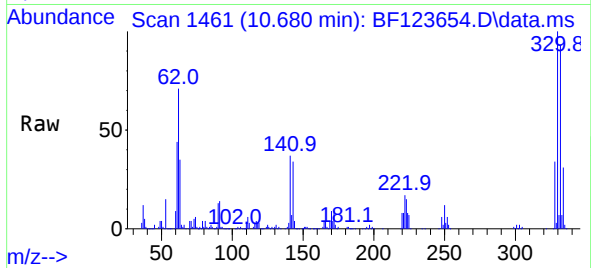

Tgt Ion:330 Resp: 522510
Ion Ratio Lower Upper
330 100
332 93.7 77.1 115.7
141 34.6 27.9 41.9




Manual Integrations
APPROVED


mohammad
4/21/2021 11:25:30 AM

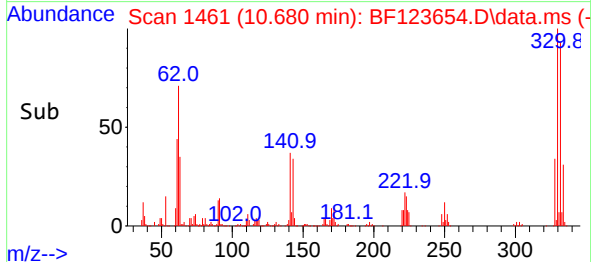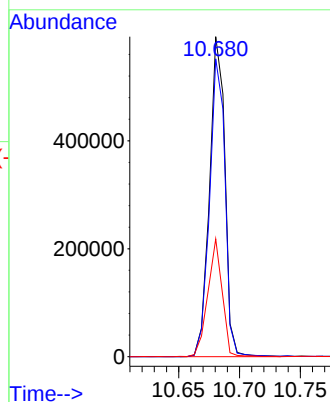


#45
2-Fluorobiphenyl
Concen: 67.32 ng
RT: 9.210 min Scan# 1211
Delta R.T. -0.006 min
Lab File: BF123654.D
Acq: 20 Apr 2021 21:22

Tgt Ion:172 Resp: 2001771
Ion Ratio Lower Upper
172 100
171 36.1 28.1 42.1
170 24.8 19.2 28.8

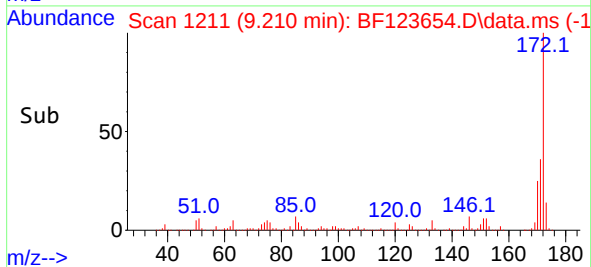
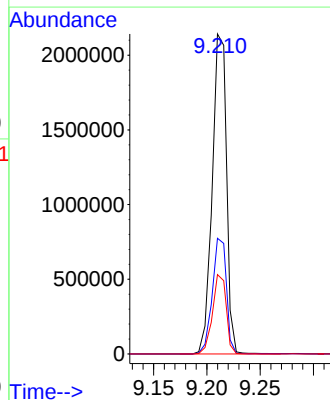
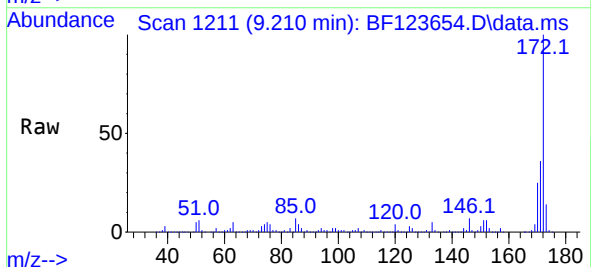





#50
Dimethylphthalate
Concen: 3.05 ng
RT: 9.604 min Scan# 1278
Delta R.T. -0.018 min
Lab File: BF123654.D
Acq: 20 Apr 2021 21:22

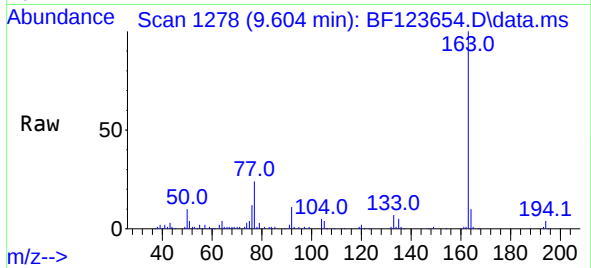



Tgt Ion:163 Resp: 93529
Ion Ratio Lower Upper
163 100
194 4.1 3.1 4.7
164 10.5 8.2 12.2

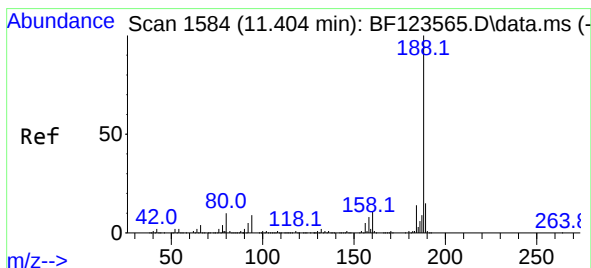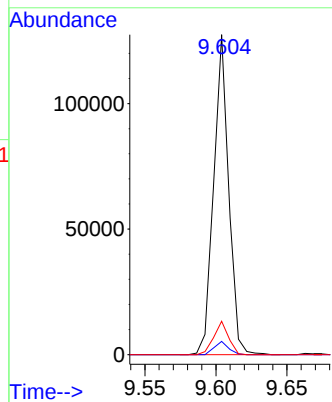

#64
Phenanthrene-d10
Concen: 20.00 ng
RT: 11.380 min Scan# 1580
Delta R.T. -0.006 min
Lab File: BF123654.D
Acq: 20 Apr 2021 21:22

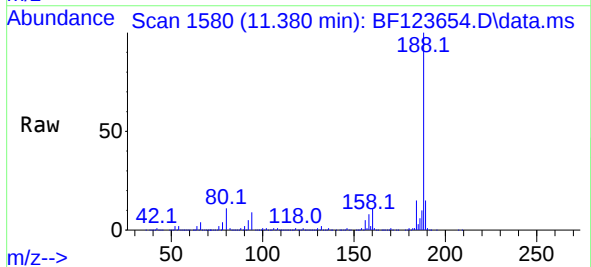


Tgt Ion:188 Resp: 826236
Ion Ratio Lower Upper
188 100
94 9.0 6.9 10.3
80 10.6 8.2 12.2

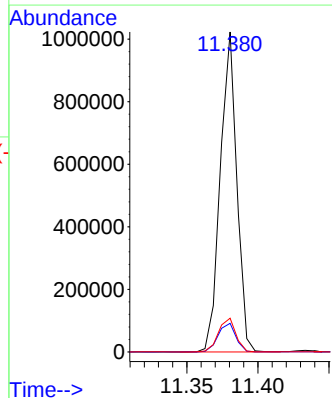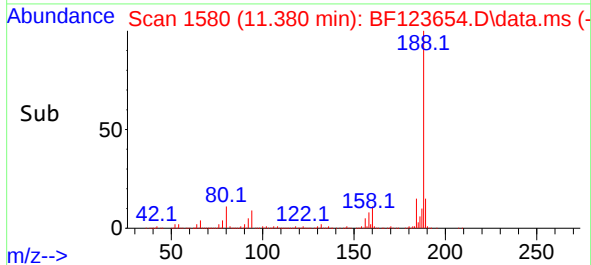

Instrument :
BNA_F
ClientSampleId :
SB-17-14.5-15.0


Manual Integrations
APPROVED

mohammad
4/21/2021 11:25:30 AM



#71
Phenanthrene
Concen: 2.67 ng
RT: 11.404 min Scan# 1584
Delta R.T. -0.006 min
Lab File: BF123654.D
Acq: 20 Apr 2021 21:22




Instrument :
BNA_F
ClientSampleId :
SB-17-14.5-15.0




Tgt Ion:178 Resp: 115127
Ion Ratio Lower Upper
178 100
176 19.4 15.6 23.4
179 15.4 12.5 18.7

Manual Integrations
APPROVED



mohammad
4/21/2021 11:25:30 AM

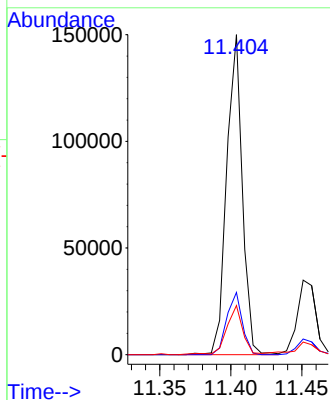


#75
Fluoranthene
Concen: 4.58 ng
RT: 12.598 min Scan# 1787
Delta R.T. -0.006 min
Lab File: BF123654.D
Acq: 20 Apr 2021 21:22



Tgt Ion:202 Resp: 216848
Ion Ratio Lower Upper
202 100
101 12.7 0.0 30.9
203 18.1 0.0 37.5

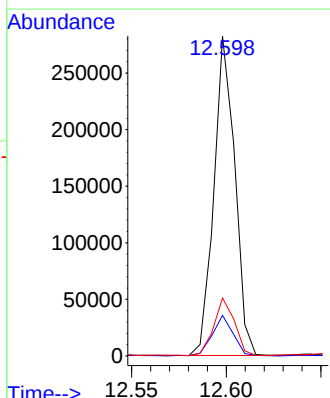







#76
Chrysene-d12
Concen: 20.00 ng
RT: 14.027 min Scan# 2030
Delta R.T. -0.006 min
Lab File: BF123654.D
Acq: 20 Apr 2021 21:22

Tgt Ion:240 Resp: 522863
Ion Ratio Lower Upper
240 100
120 9.3 7.2 10.8
236 23.6 19.0 28.4

Instrument :
BNA_F
ClientSampleId :
SB-17-14.5-15.0




Manual Integrations
APPROVED


mohammad
4/21/2021 11:25:30 AM

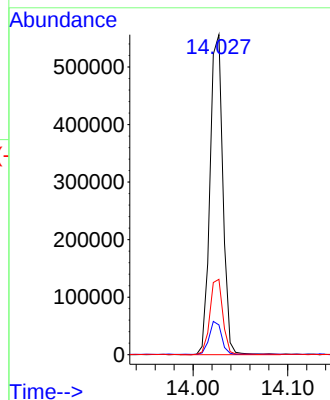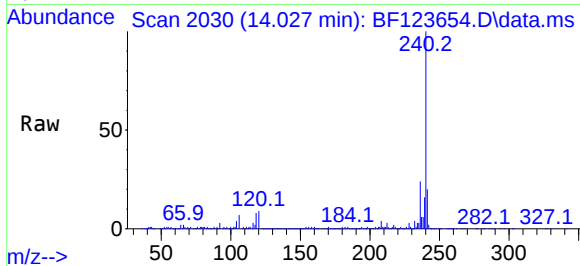


#78
Pyrene
Concen: 5.16 ng
RT: 12.821 min Scan# 1825
Delta R.T. -0.012 min
Lab File: BF123654.D
Acq: 20 Apr 2021 21:22

Tgt Ion:202 Resp: 196766
Ion Ratio Lower Upper
202 100
200 19.9 16.1 24.1
203 17.3 14.8 22.2

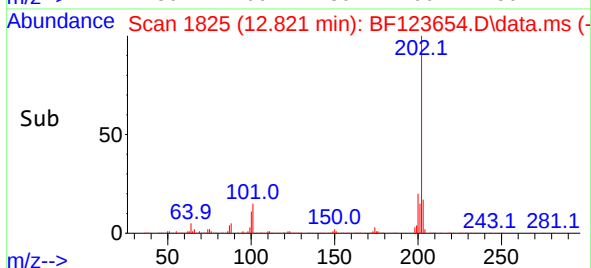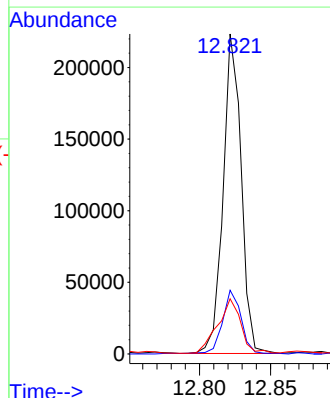
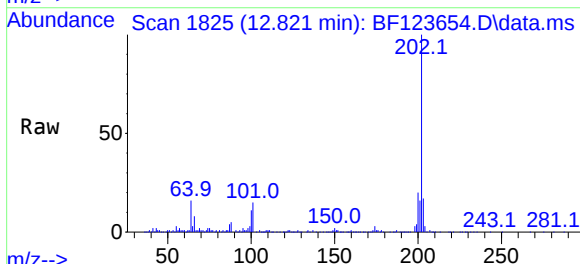




#79
Terphenyl-d14
Concen: 68.48 ng
RT: 12.974 min Scan# 1851
Delta R.T. 0.000 min
Lab File: BF123654.D
Acq: 20 Apr 2021 21:22

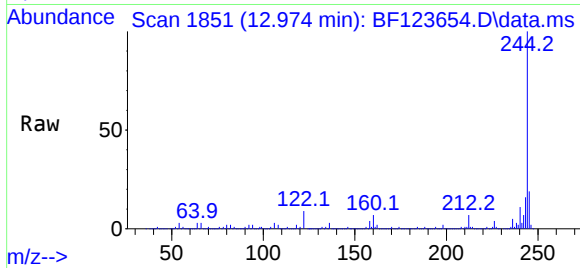


Tgt Ion:244 Resp: 1842178
Ion Ratio Lower Upper
244 100
212 7.0 5.7 8.5
122 9.4 9.7 14.5#

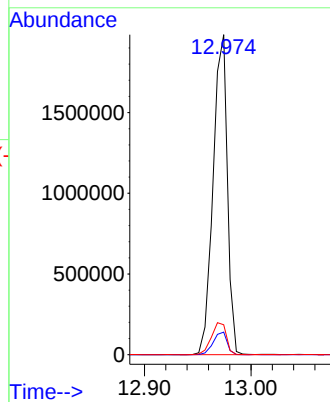


Instrument :
BNA_F
ClientSampleId :
SB-17-14.5-15.0

Manual Integrations
APPROVED



mohammad
4/21/2021 11:25:30 AM




#81
Benzo(a)anthracene
Concen: 3.89 ng
RT: 14.015 min Scan# 2028
Delta R.T. -0.006 min
Lab File: BF123654.D
Acq: 20 Apr 2021 21:22

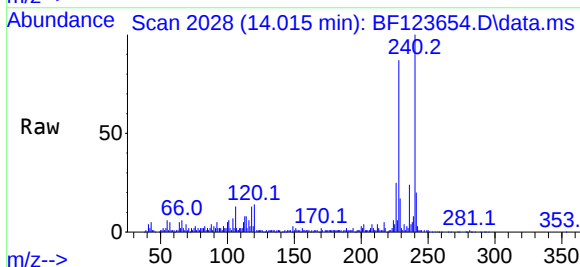

Tgt Ion:228 Resp: 124642
Ion Ratio Lower Upper
228 100
226 28.3 22.4 33.6
229 20.0 16.0 24.0

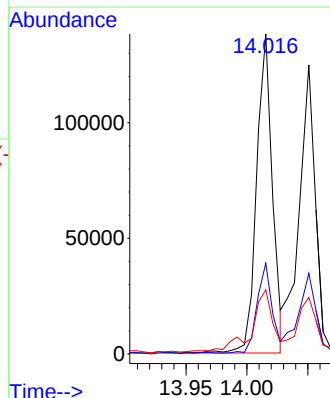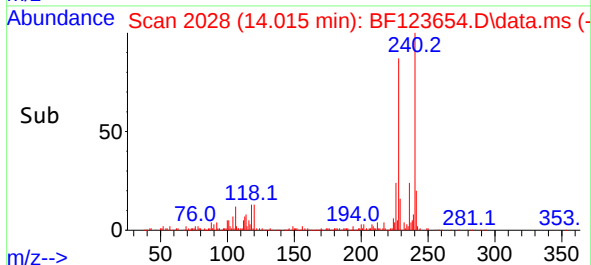







#83
Chrysene
Concen: 3.61 ng m
RT: 14.051 min Scan# 2034
Delta R.T. -0.012 min
Lab File: BF123654.D
Acq: 20 Apr 2021 21:22

Tgt Ion: 228 Resp: 116066
Ion Ratio Lower Upper
228 100
226 27.9 24.3 36.5
229 19.6 16.2 24.2

Instrument :
BNA_F
ClientSampleId :
SB-17-14.5-15.0




Manual Integrations
APPROVED


mohammad
4/21/2021 11:25:30 AM

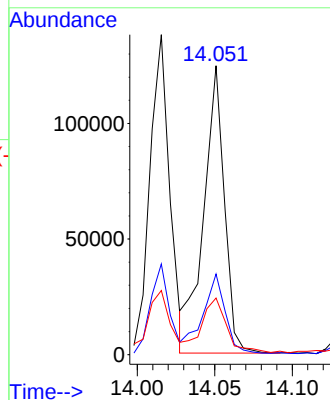

#86
Perylene-d12
Concen: 20.00 ng
RT: 15.504 min Scan# 2281
Delta R.T. 0.000 min
Lab File: BF123654.D
Acq: 20 Apr 2021 21:22

Tgt Ion: 264 Resp: 527962
Ion Ratio Lower Upper
264 100
260 23.7 18.7 28.1
265 21.9 17.8 26.8

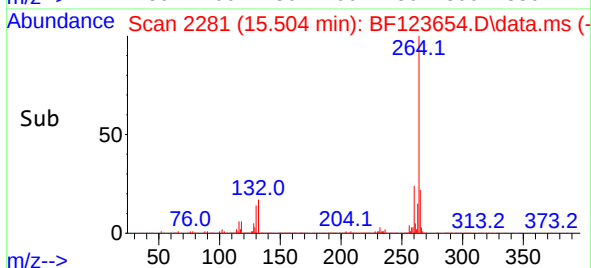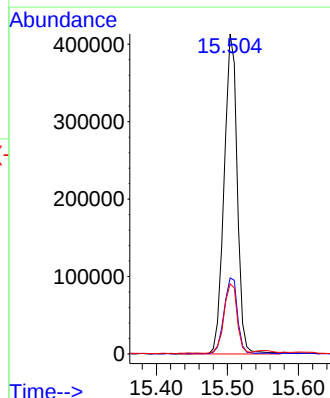







#87
Indeno(1,2,3-cd)pyrene
Concen: 2.04 ng
RT: 16.974 min Scan# 2531
Delta R.T. -0.012 min
Lab File: BF123654.D
Acq: 20 Apr 2021 21:22

Tgt Ion: 276 Resp: 57369
Ion Ratio Lower Upper
276 100
138 28.9 16.2 24.2#
277 24.9 20.1 30.1

Instrument :
BNA_F
ClientSampleId :
SB-17-14.5-15.0




Manual Integrations
APPROVED


mohammad
4/21/2021 11:25:30 AM

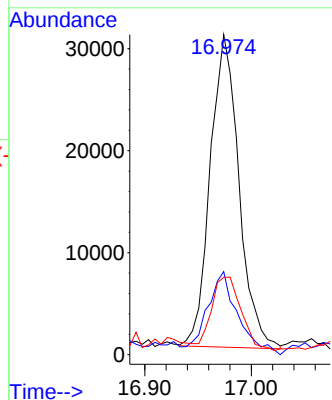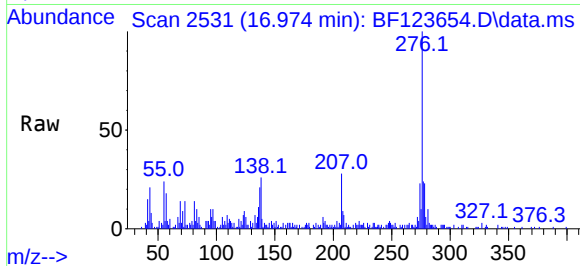

#88
Benzo(b)fluoranthene
Concen: 3.51 ng m
RT: 15.068 min Scan# 2207
Delta R.T. -0.006 min
Lab File: BF123654.D
Acq: 20 Apr 2021 21:22

Tgt Ion: 252 Resp: 130887
Ion Ratio Lower Upper
252 100
253 21.8 18.1 27.1
125 14.7 6.2 9.4#

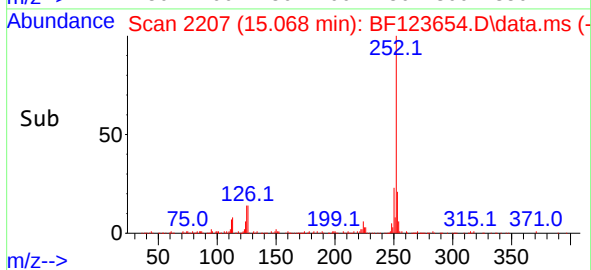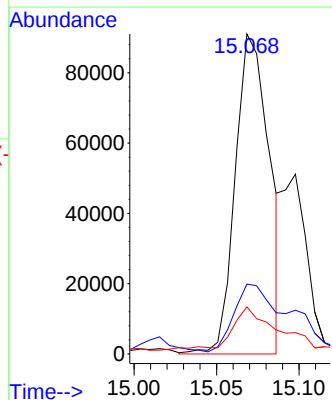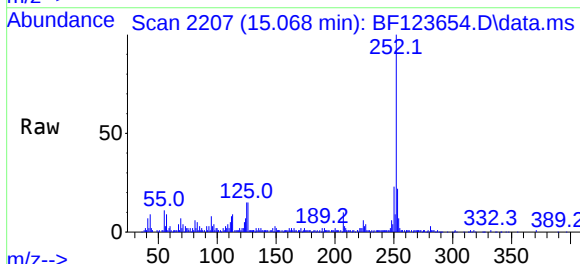

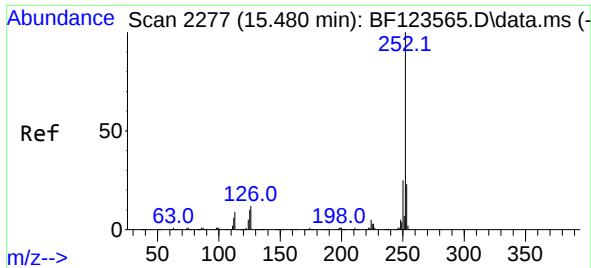

#90
Benzo(a)pyrene
Concen: 3.37 ng
RT: 15.439 min Scan# 2270
Delta R.T. -0.006 min
Lab File: BF123654.D
Acq: 20 Apr 2021 21:22

Tgt Ion:	252	Resp:	99949
Ion Ratio	Lower	Upper	
252	100		
253	20.4	18.4	27.6
125	11.9	8.0	12.0

Instrument :
BNA_F
ClientSampleId :
SB-17-14.5-15.0

Manual Integrations
APPROVED

mohammad
4/21/2021 11:25:30 AM

