
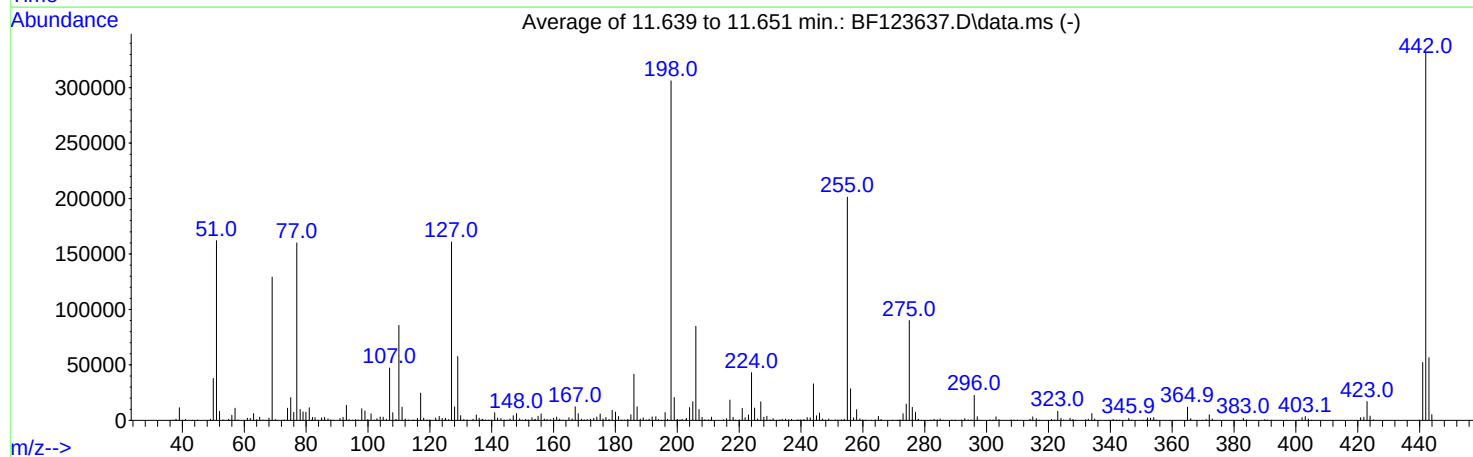


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF042021\
 Data File : BF123637.D
 Acq On : 20 Apr 2021 11:35
 Operator : JU/CG
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF041521.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Tue Apr 20 15:49:40 2021

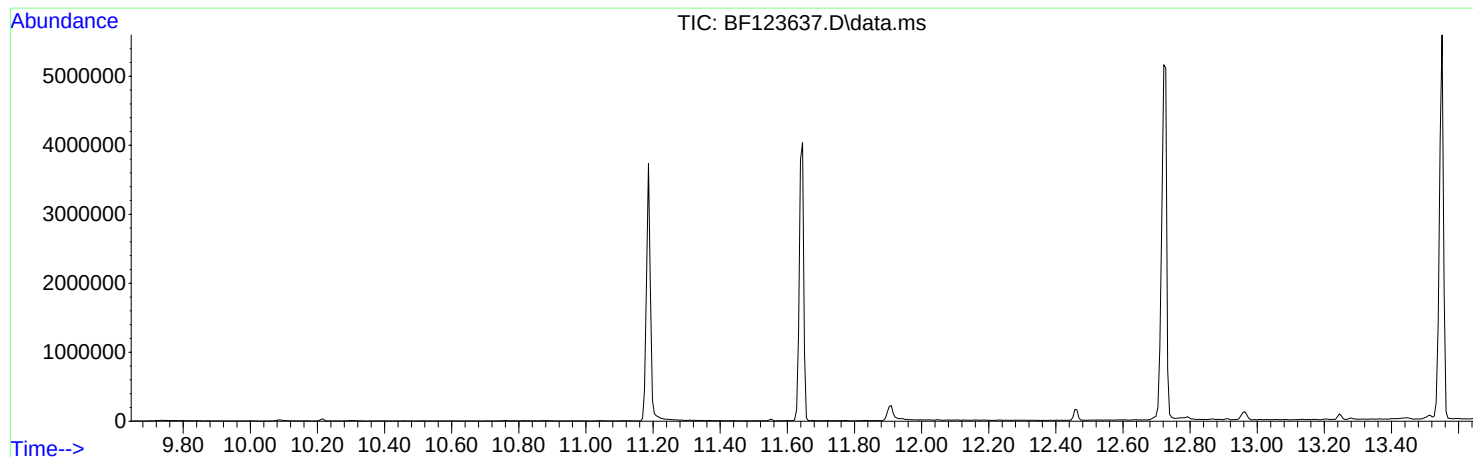




AutoFind: Scans 1624, 1625, 1626; Background Corrected with Scan 1618

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	52.9	162069	PASS
68	69	0.00	2	1.6	2010	PASS
69	198	0.00	100	42.2	129109	PASS
70	69	0.00	2	0.5	670	PASS
127	198	10	80	52.6	160933	PASS
197	198	0.00	2	0.3	833	PASS
198	198	100	100	100.0	306120	PASS
199	198	5	9	6.8	20675	PASS
275	198	10	60	29.4	90085	PASS
365	198	1	100	3.9	11980	PASS
441	198	0.01	100	17.1	52195	PASS
442	442	50	100	100.0	331691	PASS
443	442	15	24	17.1	56632	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF042021\
 Data File : BF123637.D
 Acq On : 20 Apr 2021 11:35
 Operator : JU/CG
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Quant Time: Apr 21 05:59:48 2021
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF041521.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue Apr 20 15:49:40 2021
 Response via : Initial Calibration

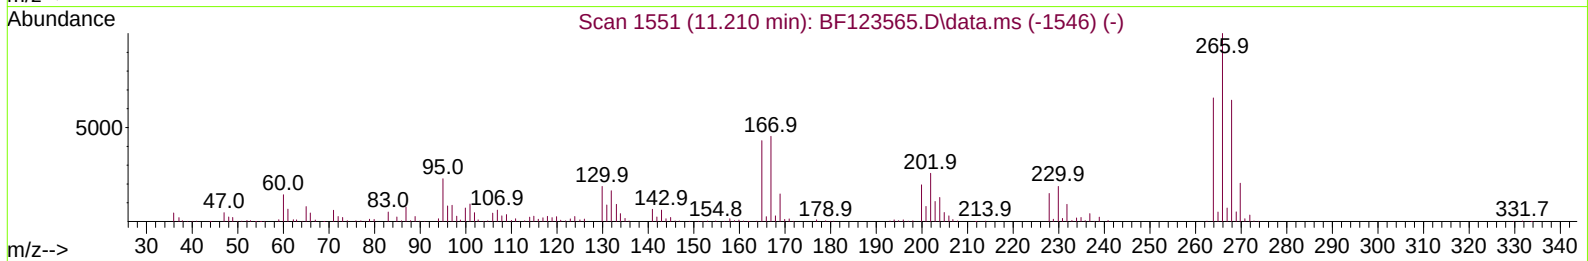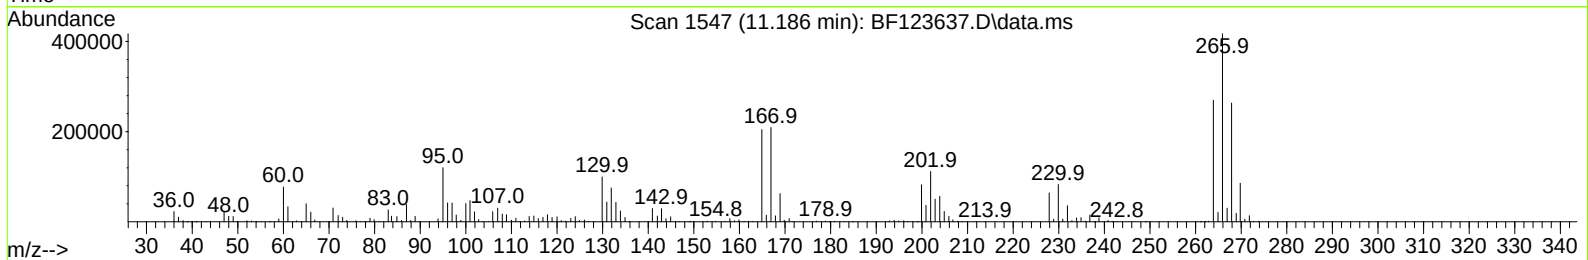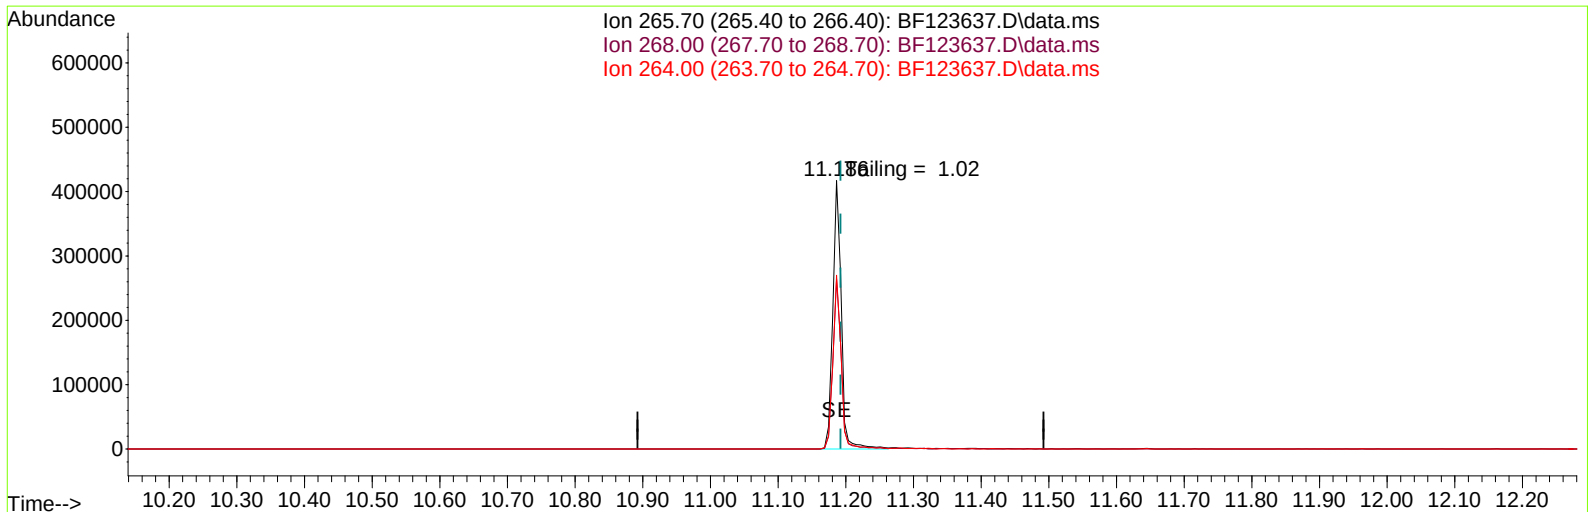

TIC: BF123637.D\data.ms

(70) Pentachlorophenol (C)

11.186min (-0.006) 39857.80 ng




response 363135

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	64.50	63.19
264.00	65.70	64.74
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF042021\
Data File : BF123637.D
Acq On : 20 Apr 2021 11:35
Operator : JU/CG
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Quant Time: Apr 21 05:59:48 2021
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF041521.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Apr 20 15:49:40 2021
Response via : Initial Calibration

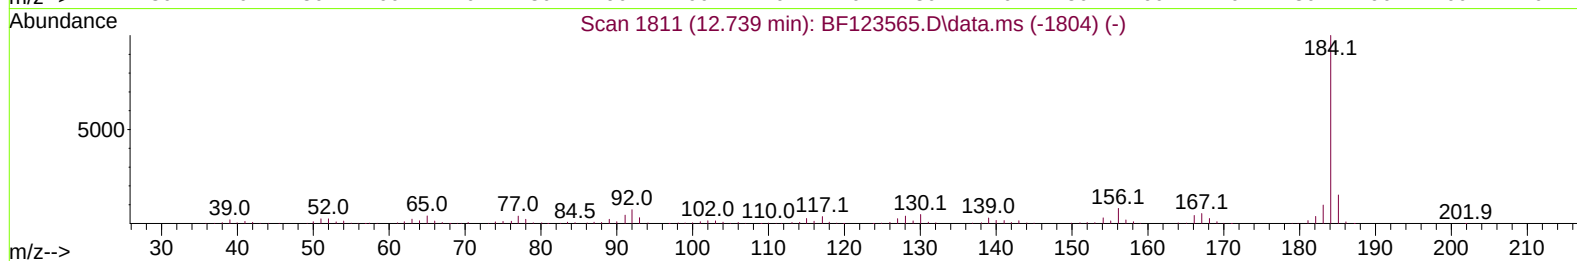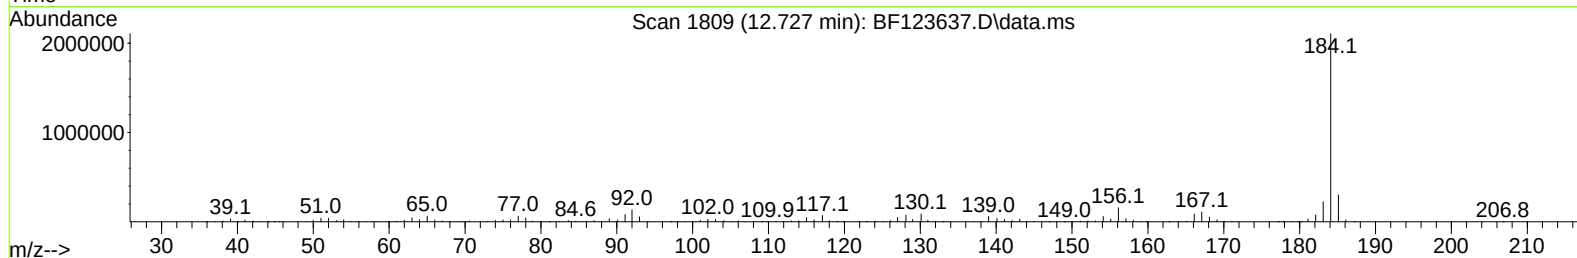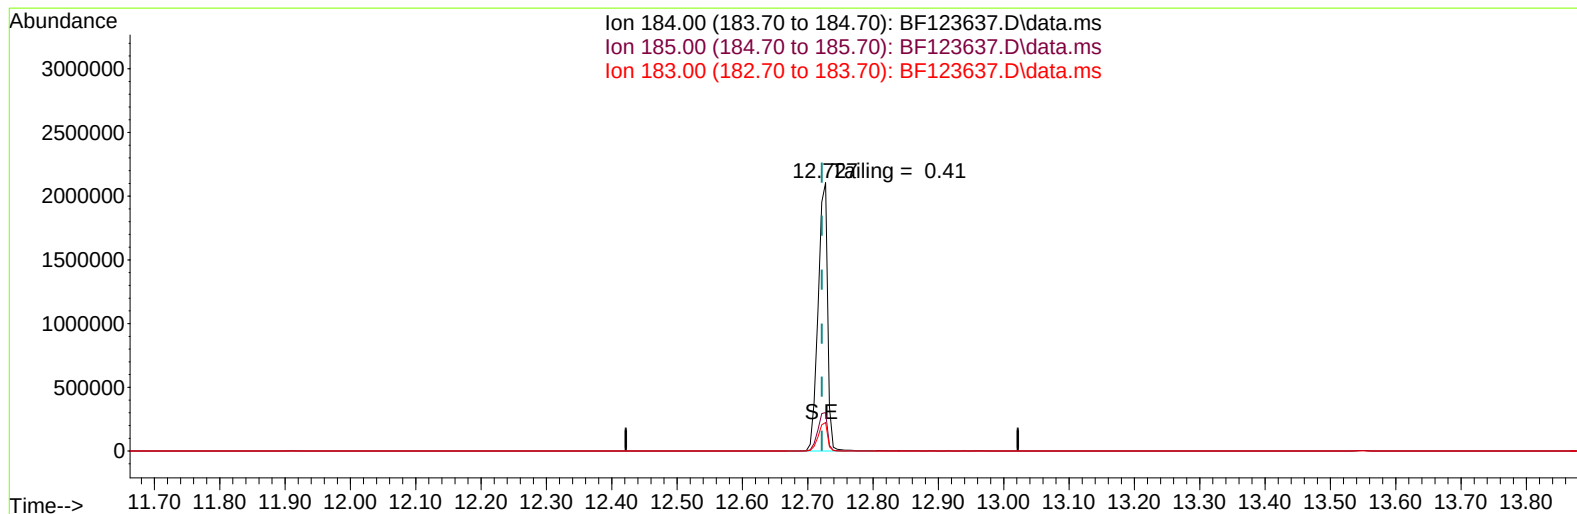

TIC: BF123637.D\data.ms

(77) Benzidine

12.727min (+ 0.006) 0.00 ng

response 2134102

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.10	14.30
183.00	9.80	10.64
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
4/20/2021	BNA_F	<u>BF123637.D</u>
Compound Name	Response	Retention Time
DDT	857527	13.551
DDD	16856	13.245
DDE	1431	12.91
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
18287	875814	2.09