
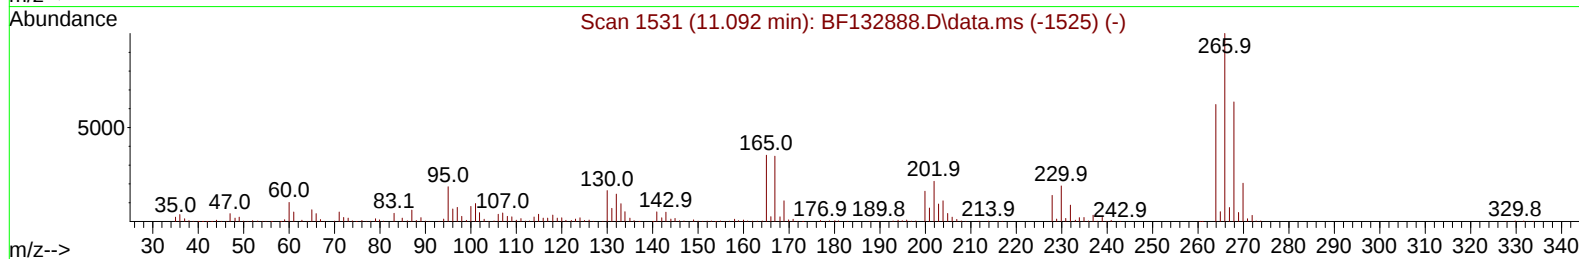
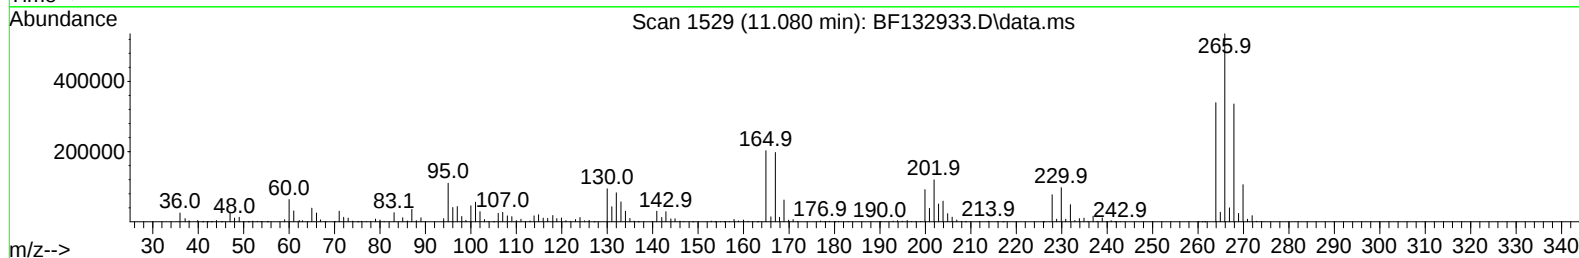


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF042023\
Data File : BF132933.D
Acq On : 20 Apr 2023 10:53
Operator : CG\JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Apr 21 04:20:47 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF041723.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Apr 20 14:15:37 2023
Response via : Initial Calibration

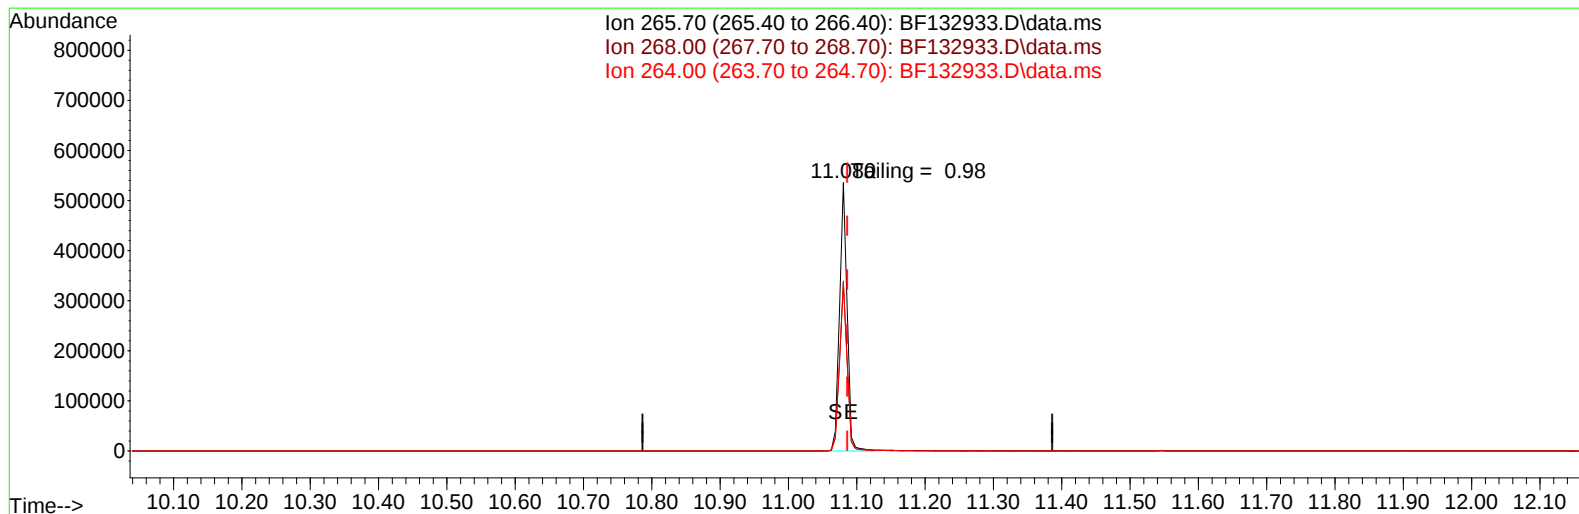

TIC: BF132933.D\data.ms

(70) Pentachlorophenol (C)




11.080min (-0.006) 709692.03 ng

response 417758

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	63.60	62.63
264.00	62.20	63.29
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF042023\
Data File : BF132933.D
Acq On : 20 Apr 2023 10:53
Operator : CG\JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Apr 21 04:20:47 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF041723.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Apr 20 14:15:37 2023
Response via : Initial Calibration

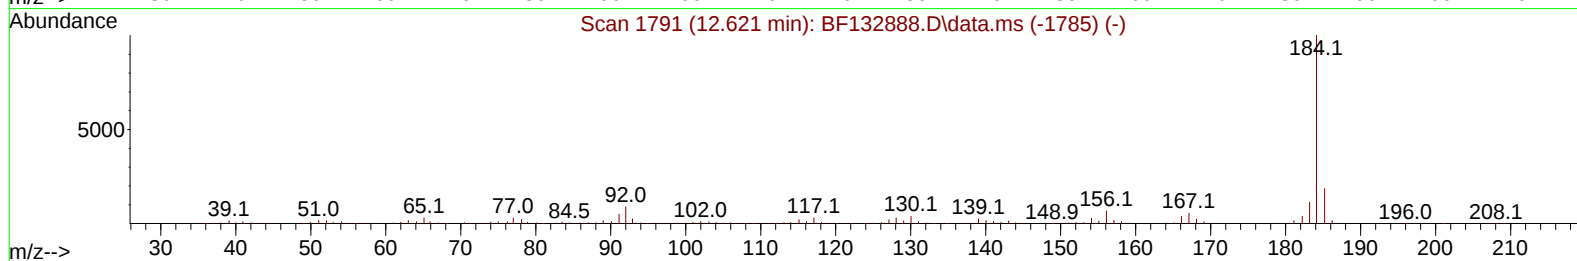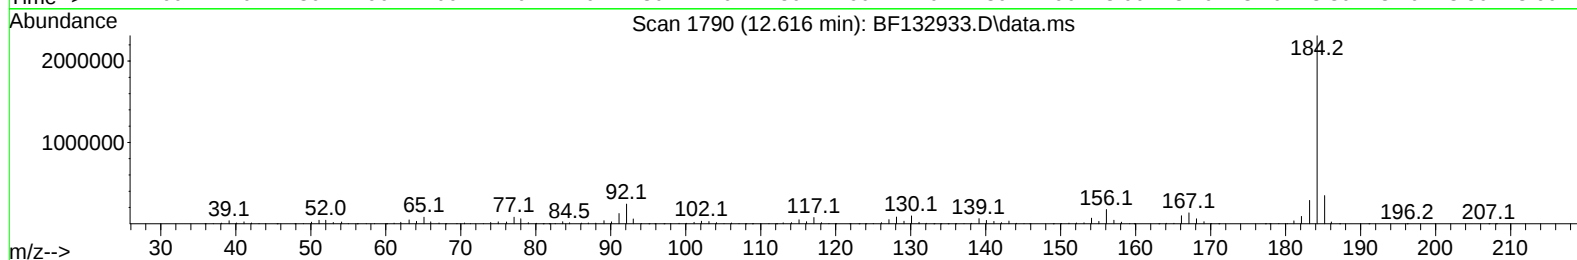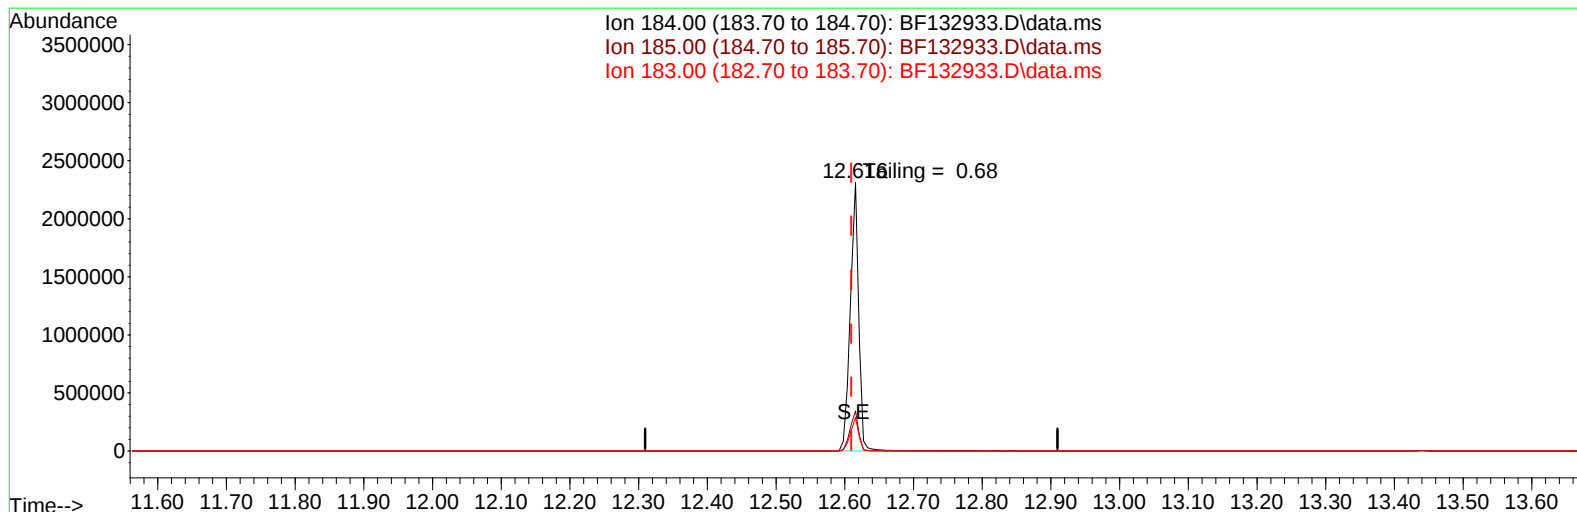

TIC: BF132933.D\data.ms

(77) Benzidine

12.616min (+ 0.006) 10265.13 ng

response 1968443

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	18.60	14.96
183.00	11.30	12.46
0.00	0.00	0.00