
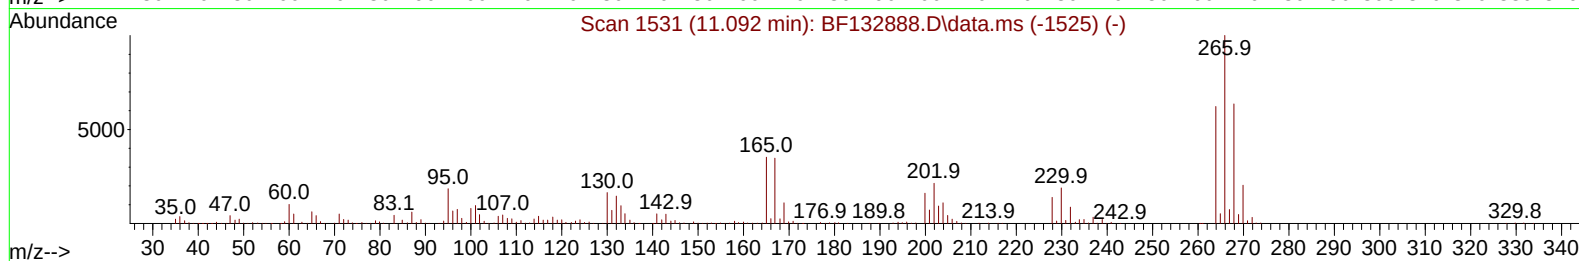
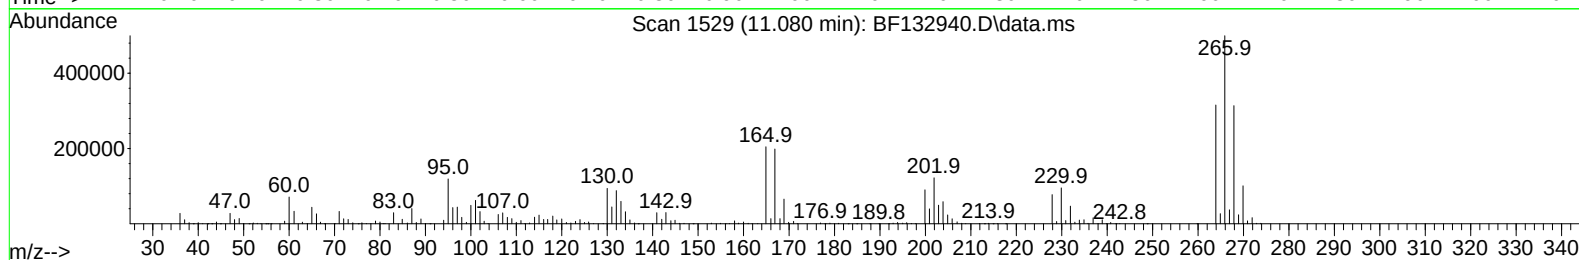


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF042023\
Data File : BF132940.D
Acq On : 20 Apr 2023 16:53
Operator : CG\JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Apr 21 04:22:28 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF041723.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Apr 20 14:15:37 2023
Response via : Initial Calibration

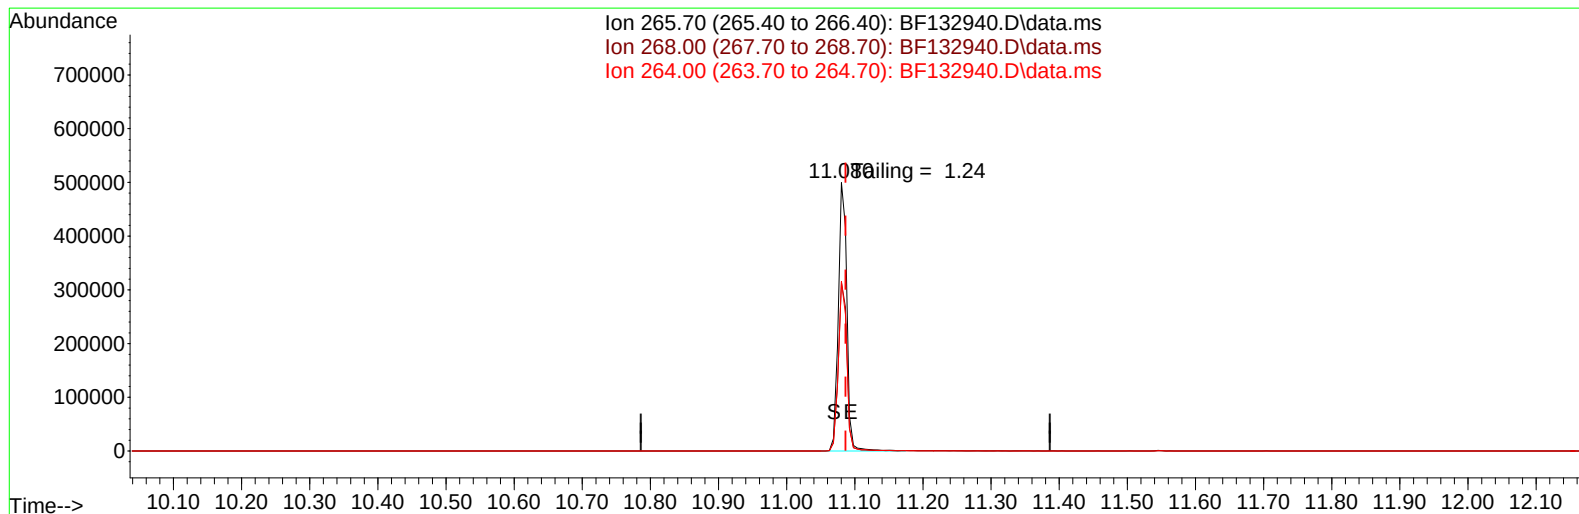

TIC: BF132940.D\data.ms

(70) Pentachlorophenol (C)




11.080min (-0.006) 34169.97 ng

response 435456

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	63.60	62.82
264.00	62.20	63.18
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF042023\
Data File : BF132940.D
Acq On : 20 Apr 2023 16:53
Operator : CG\JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Apr 21 04:22:28 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF041723.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Apr 20 14:15:37 2023
Response via : Initial Calibration

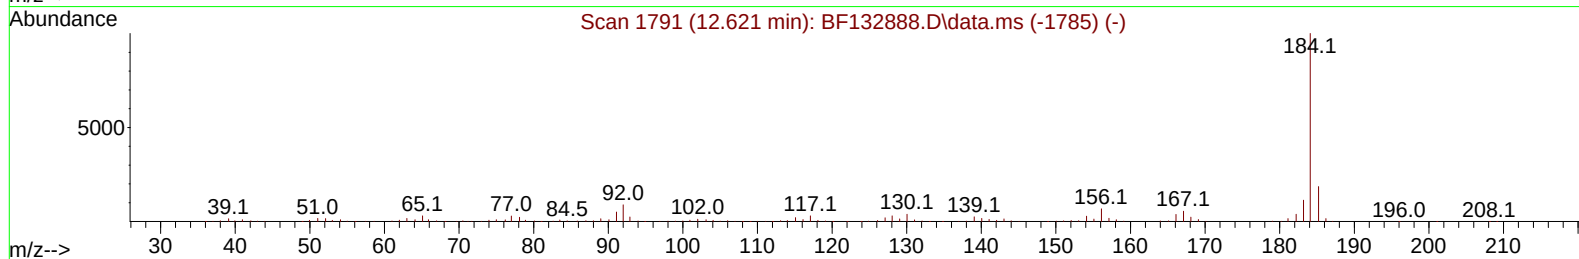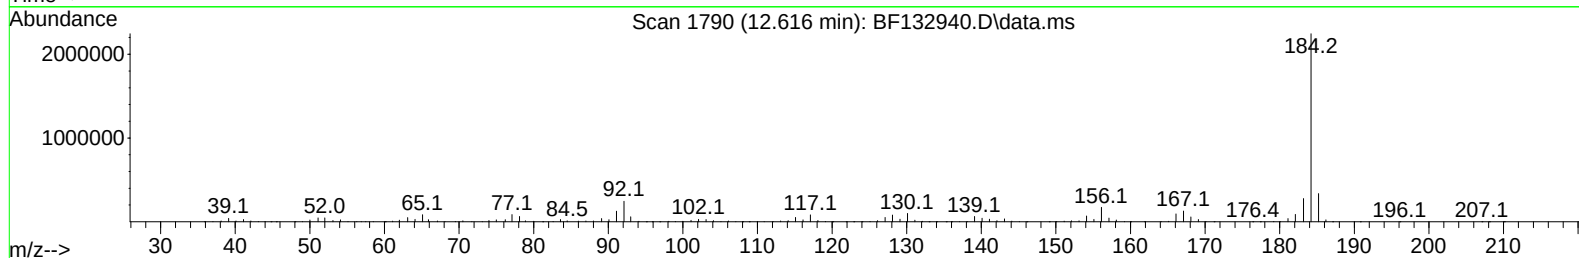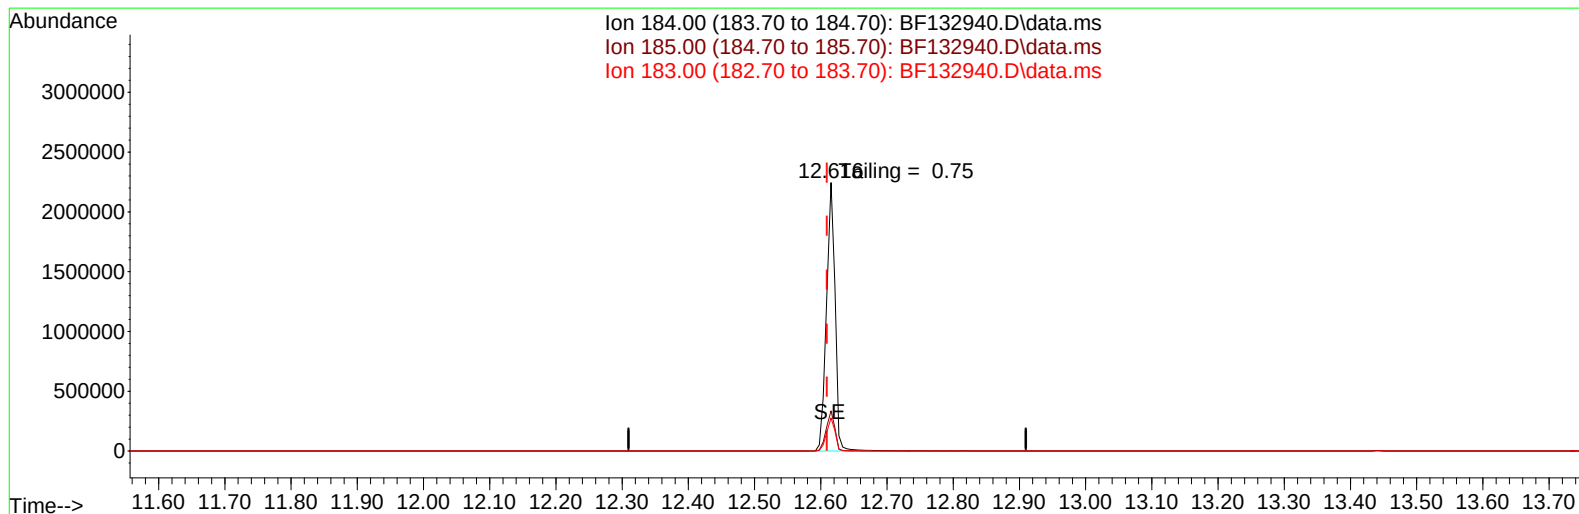

TIC: BF132940.D\data.ms

(77) Benzidine

12.616min (+ 0.006) 2426012.84 ng

response 2040738

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	18.60	15.01
183.00	11.30	12.38
0.00	0.00	0.00