


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF042023\
 Data File : BF132933.D
 Acq On : 20 Apr 2023 10:53
 Operator : CG\JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF041723.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Thu Apr 20 14:15:37 2023

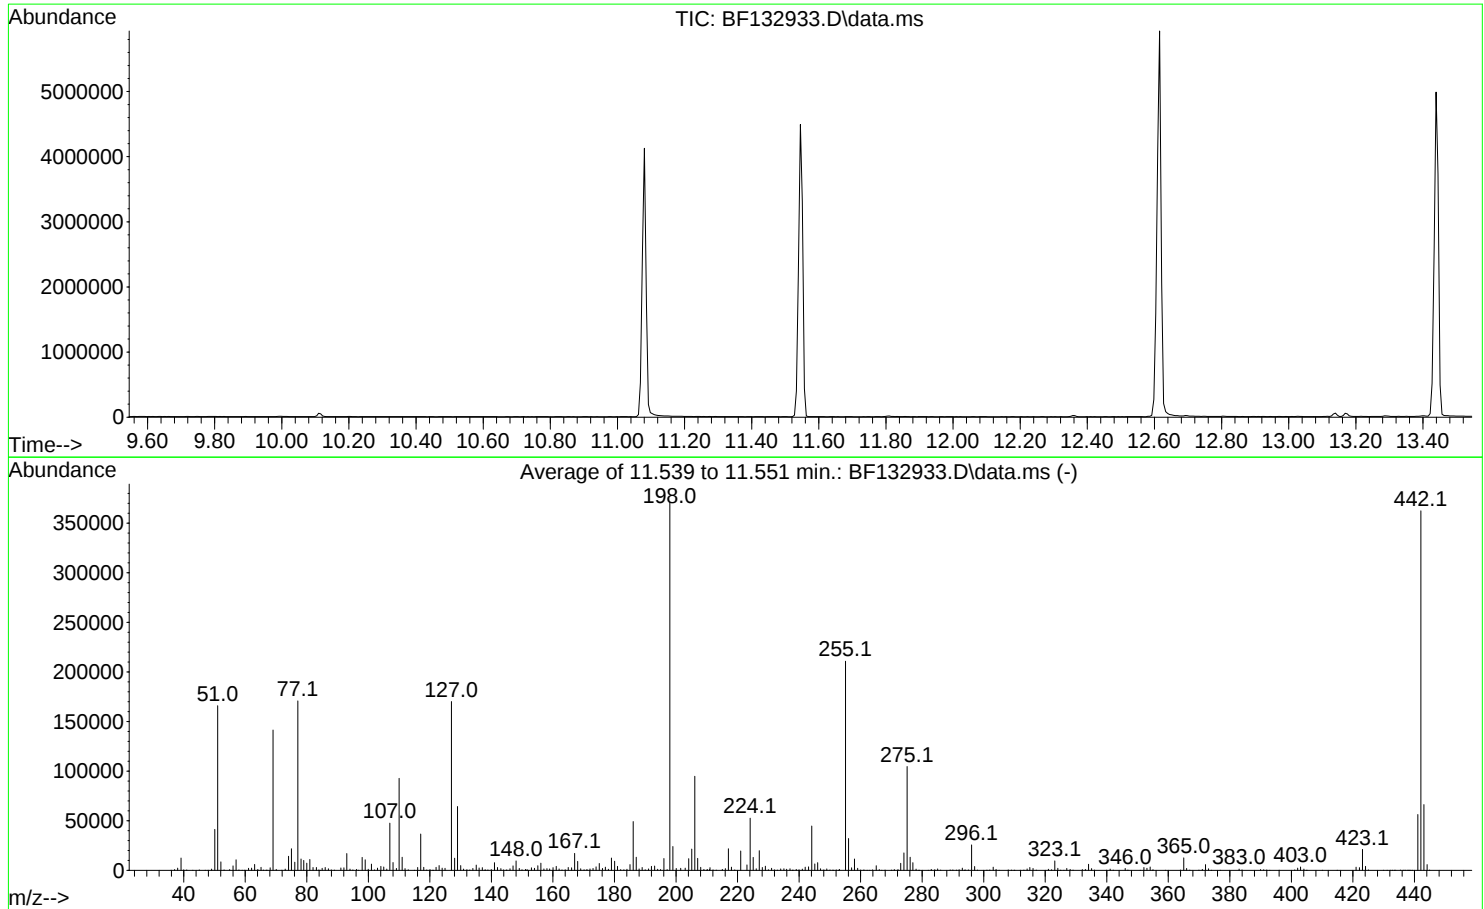




AutoFind: Scans 1607, 1608, 1609; Background Corrected with Scan 1602

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	44.8	166014	PASS
68	69	0.00	2	1.8	2551	PASS
69	198	0.00	100	38.1	141461	PASS
70	69	0.00	2	0.6	832	PASS
127	198	10	80	45.9	170197	PASS
197	198	0.00	2	0.2	750	PASS
198	198	100	100	100.0	370965	PASS
199	198	5	9	6.5	23984	PASS
275	198	10	60	28.2	104603	PASS
365	198	1	100	3.4	12459	PASS
441	198	0.01	100	15.2	56261	PASS
442	442	50	100	100.0	362541	PASS
443	442	15	24	18.3	66325	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF042023\
Data File : BF132933.D
Acq On : 20 Apr 2023 10:53
Operator : CG\JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Quant Time: Apr 21 04:20:47 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF041723.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Apr 20 14:15:37 2023
Response via : Initial Calibration

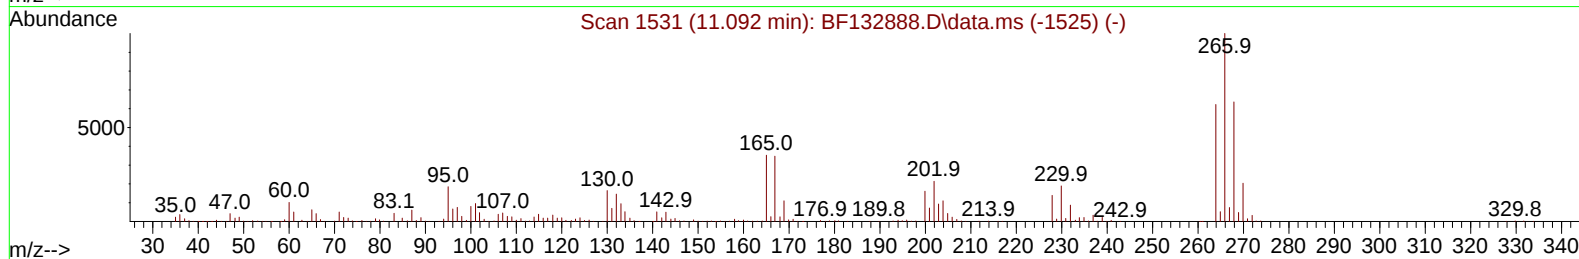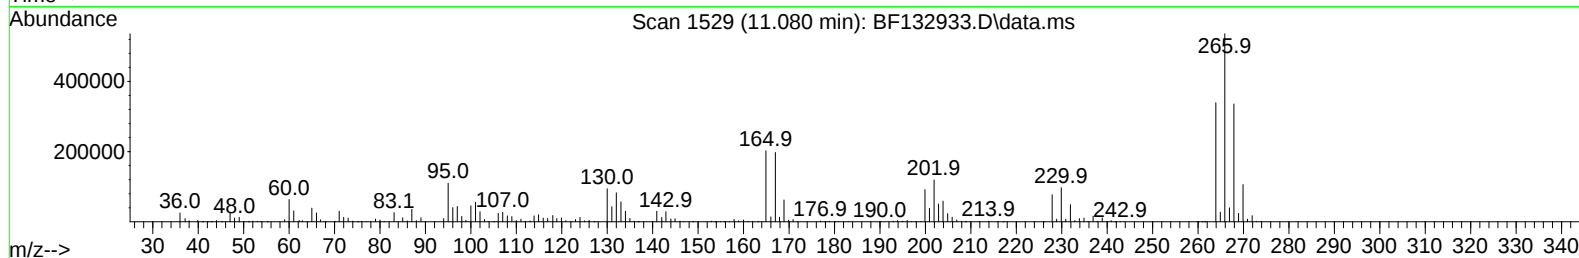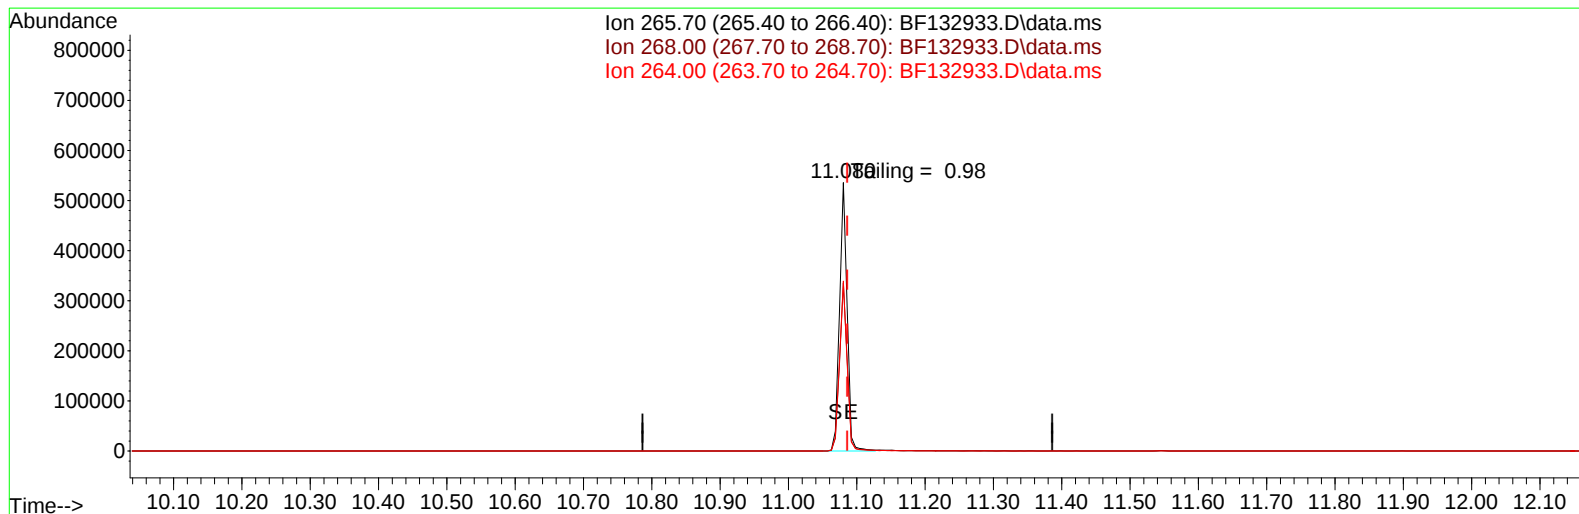

TIC: BF132933.D\data.ms

(70) Pentachlorophenol (C)

11.080min (-0.006) 709692.03 ng




response 417758

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	63.60	62.63
264.00	62.20	63.29
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF042023\
 Data File : BF132933.D
 Acq On : 20 Apr 2023 10:53
 Operator : CG\JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Quant Time: Apr 21 04:20:47 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF041723.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Thu Apr 20 14:15:37 2023
 Response via : Initial Calibration

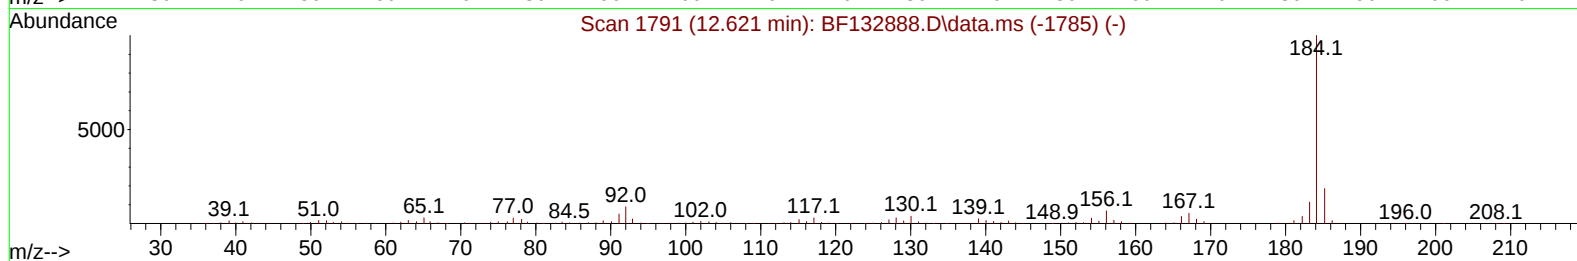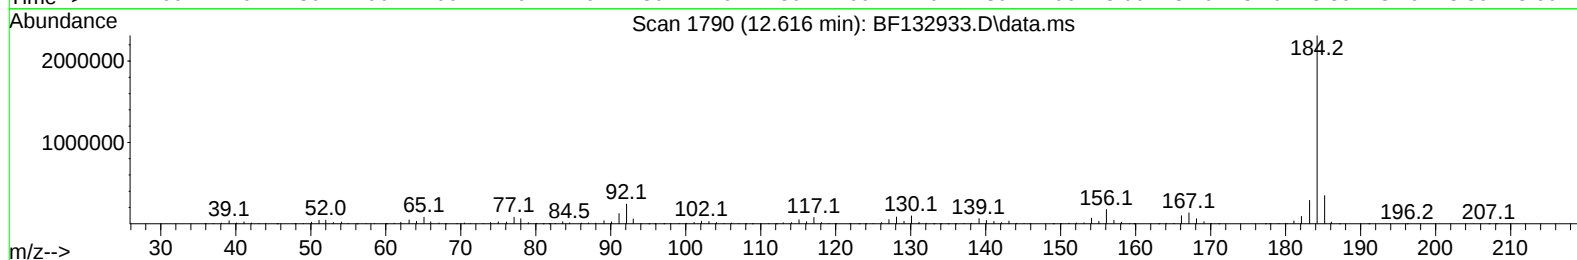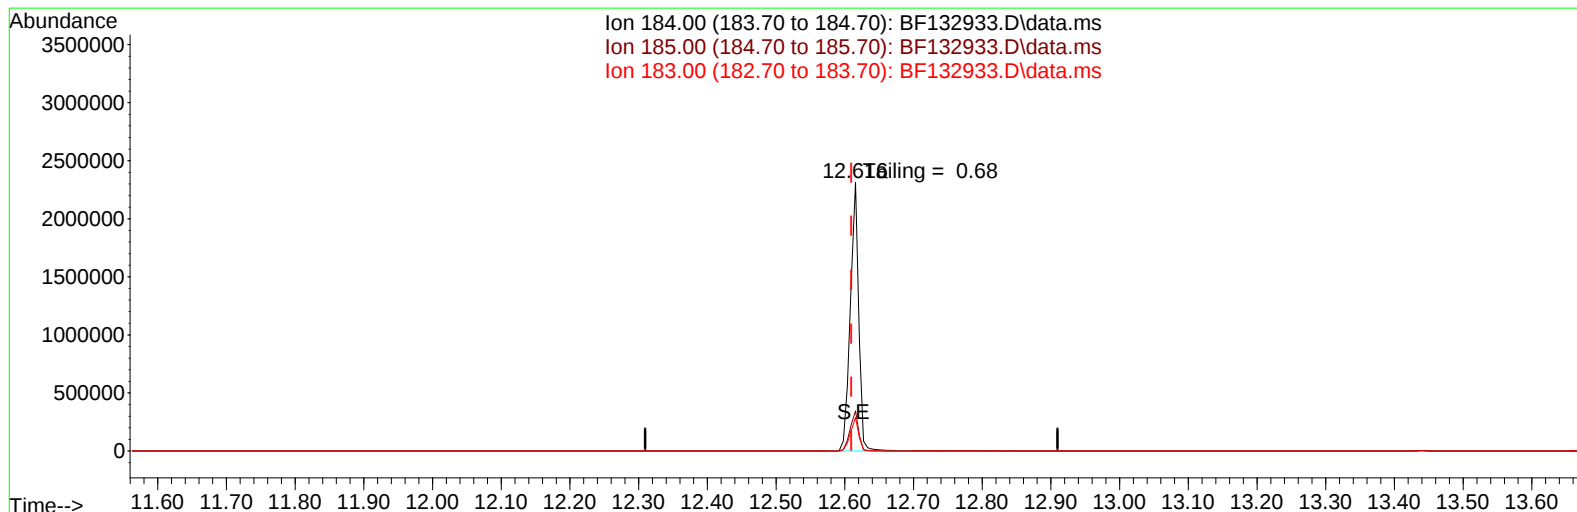

TIC: BF132933.D\data.ms

(77) Benzidine

12.616min (+ 0.006) 10265.13 ng

response 1968443

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	18.60	14.96
183.00	11.30	12.46
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
4/20/2023	BNA_F	<u>BF132933.D</u>
Compound Name	Response	Retention Time
DDT	838856	13.439
DDD	15439	13.139
DDE	454	12.804
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
15893	854749	1.86

Instrument :
BNA_F
ClientSampleId :
DFTPP