


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF042023\
Data File : BF132940.D
Acq On : 20 Apr 2023 16:53
Operator : CG\JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF041723.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Thu Apr 20 14:15:37 2023

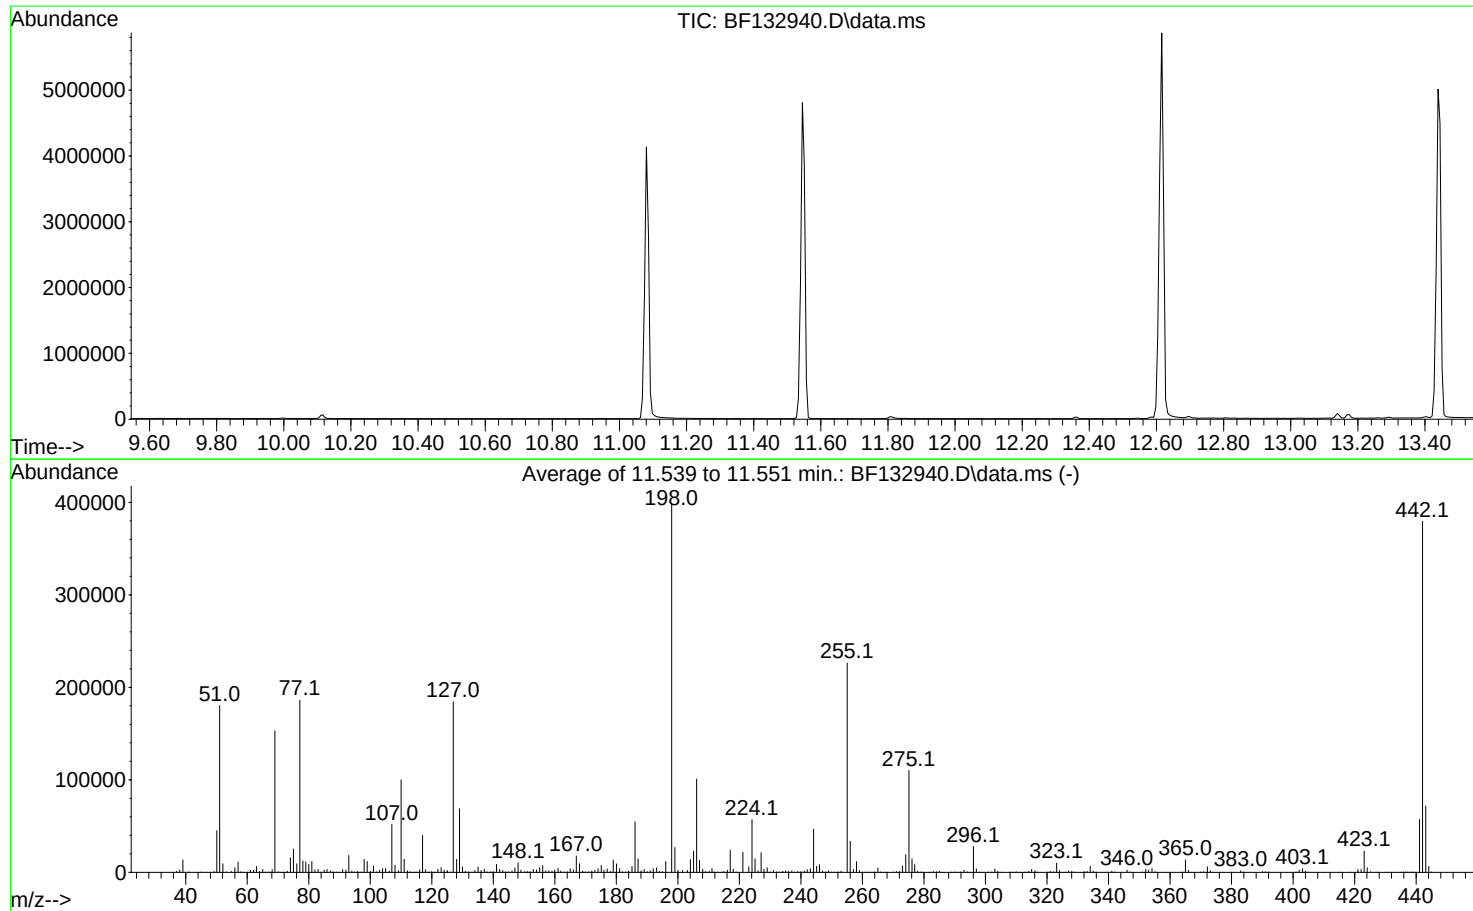




AutoFind: Scans 1607, 1608, 1609; Background Corrected with Scan 1601

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	45.3	180286	PASS
68	69	0.00	2	1.9	2911	PASS
69	198	0.00	100	38.5	153045	PASS
70	69	0.00	2	0.4	684	PASS
127	198	10	80	46.4	184397	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	397781	PASS
199	198	5	9	6.7	26744	PASS
275	198	10	60	27.7	110091	PASS
365	198	1	100	3.4	13427	PASS
441	198	0.01	100	14.4	57201	PASS
442	442	50	100	100.0	379565	PASS
443	442	15	24	18.9	71749	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF042023\
Data File : BF132940.D
Acq On : 20 Apr 2023 16:53
Operator : CG\JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Quant Time: Apr 21 04:22:28 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF041723.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Apr 20 14:15:37 2023
Response via : Initial Calibration

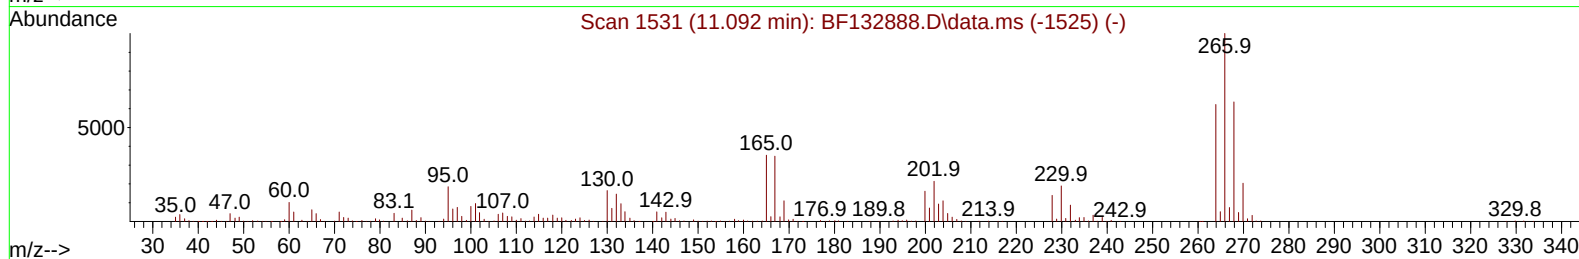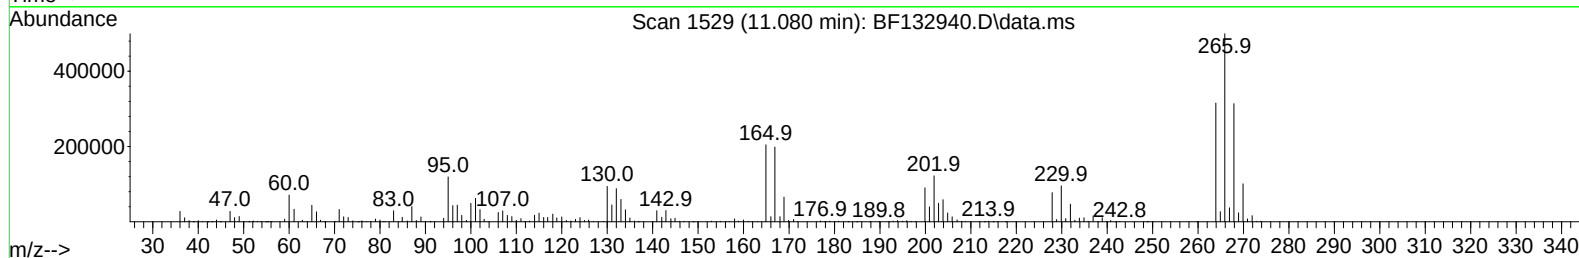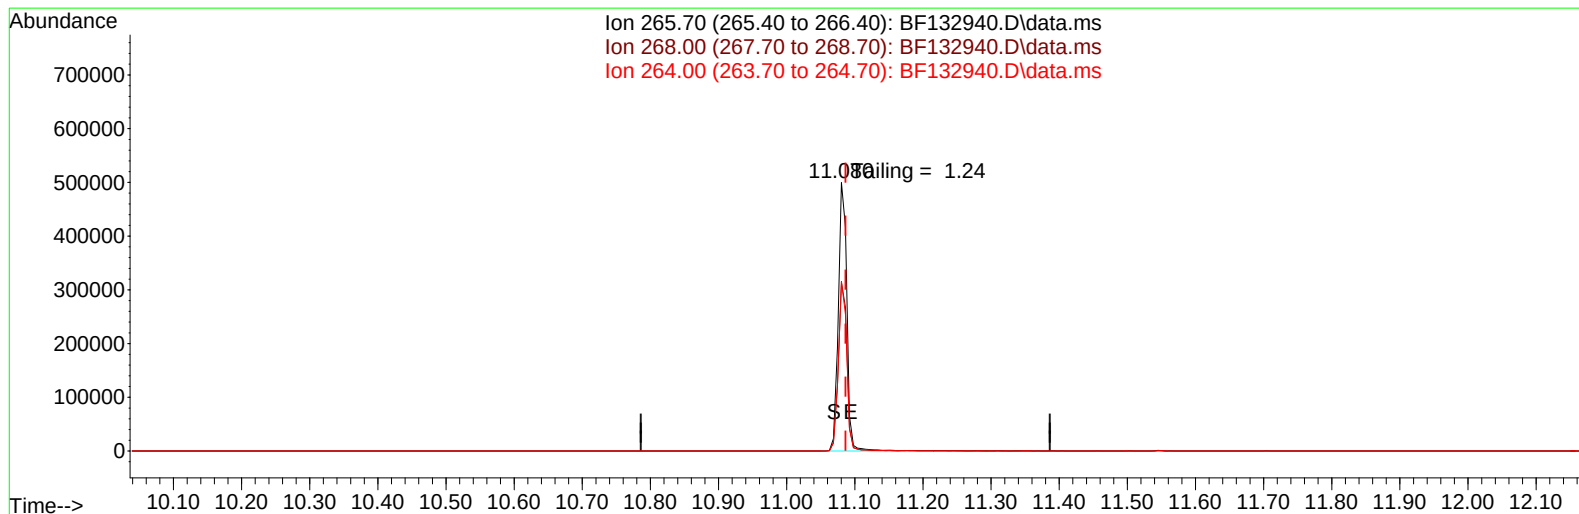

TIC: BF132940.D\data.ms

(70) Pentachlorophenol (C)

11.080min (-0.006) 34169.97 ng




response 435456

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	63.60	62.82
264.00	62.20	63.18
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF042023\
Data File : BF132940.D
Acq On : 20 Apr 2023 16:53
Operator : CG\JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Quant Time: Apr 21 04:22:28 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF041723.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Apr 20 14:15:37 2023
Response via : Initial Calibration

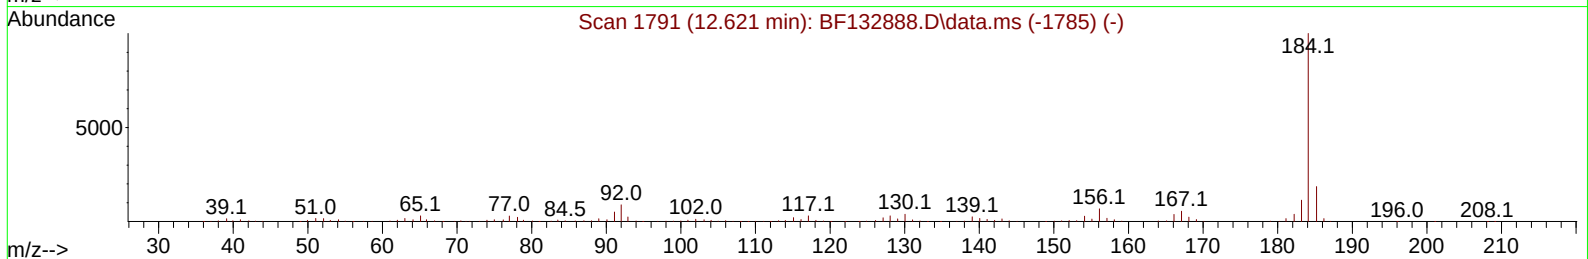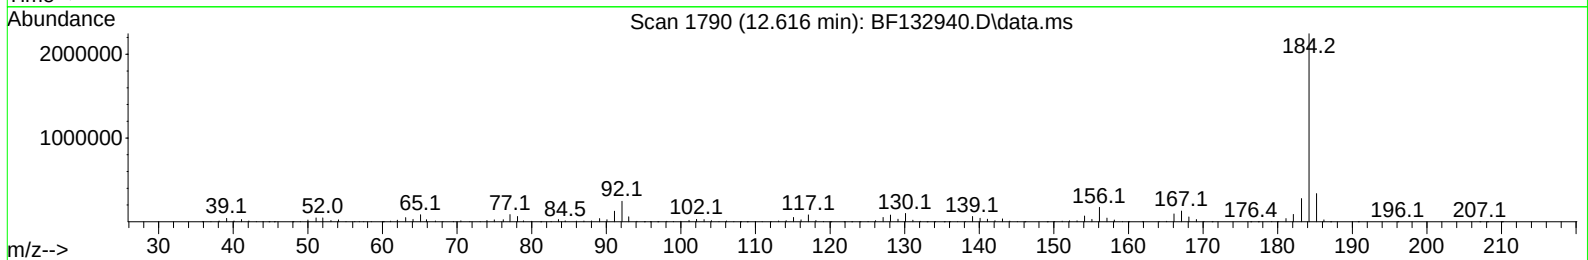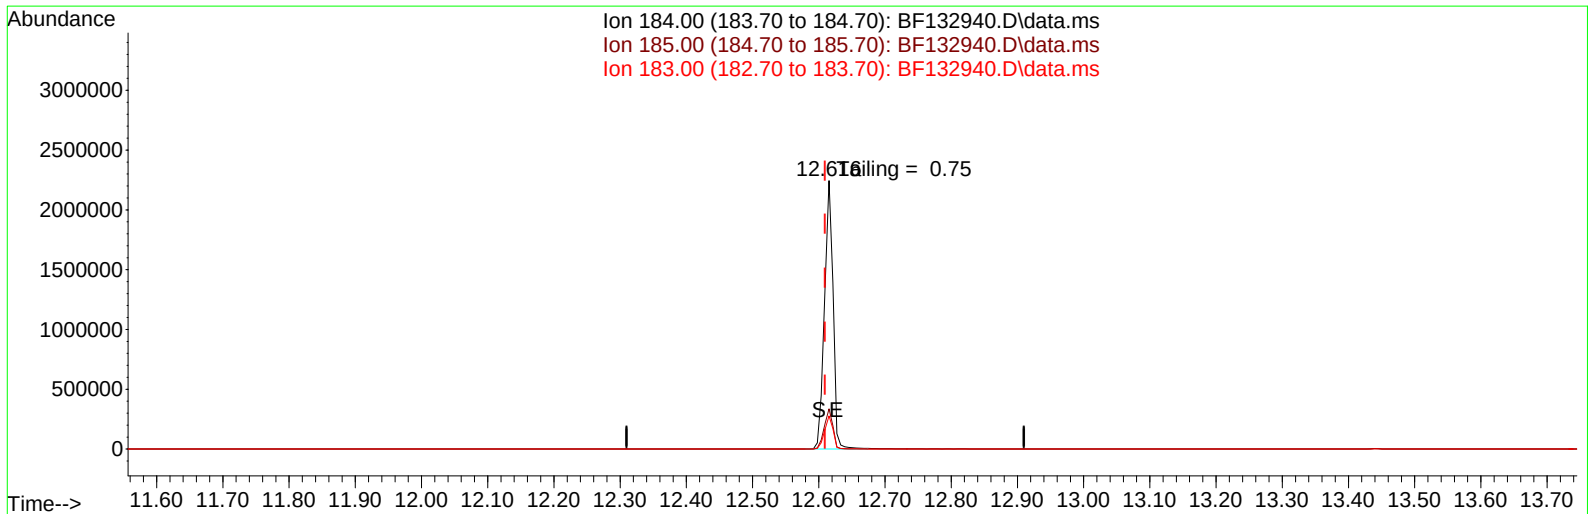

TIC: BF132940.D\data.ms

(77) Benzidine

12.616min (+ 0.006) 2426012.84 ng

response 2040738

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	18.60	15.01
183.00	11.30	12.38
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
4/20/2023	BNA_F	<u>BF132940.D</u>
Compound Name	Response	Retention Time
DDT	896129	13.439
DDD	19557	13.139
DDE	760	12.804
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
20317	916446	2.22

Instrument :
BNA_F
ClientSampleId :
DFTPP