
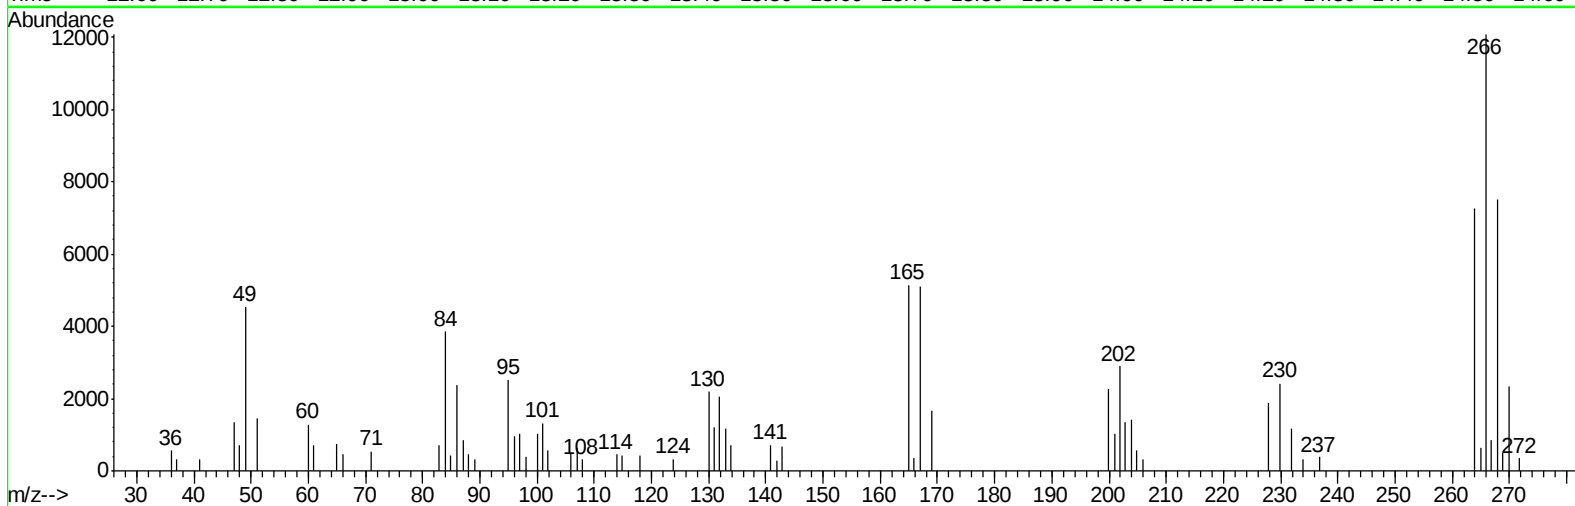


Data Path : Z:\HPCHEM1\BNA_F\DATA\BF042115\
Data File : BF078683.D
Acq On : 21 Apr 2015 14:35
Operator : TP/IZ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Apr 22 07:21:48 2015
Quant Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF040115.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Apr 22 05:03:12 2015
Response via : Initial Calibration

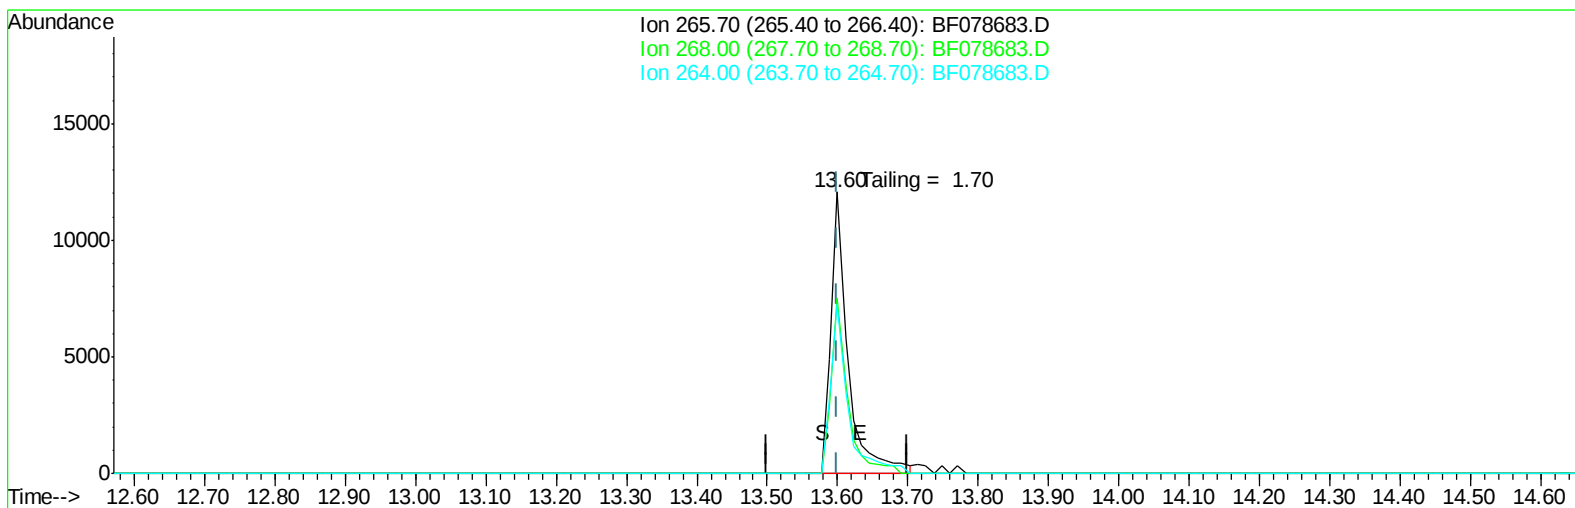

TIC: BF078683.D

(69) Pentachlorophenol (C)



13.600min (+0.000) 0.00ng

response 18975

Ion	Exp%	Act%
265.70	100	100
268.00	62.60	62.09
264.00	62.50	60.12
0.00	0.00	0.00

Data Path : Z:\HPCHEM1\BNA_F\DATA\BF042115\
Data File : BF078683.D
Acq On : 21 Apr 2015 14:35
Operator : TP/IZ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Apr 22 07:21:48 2015
Quant Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF040115.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Apr 22 05:03:12 2015
Response via : Initial Calibration

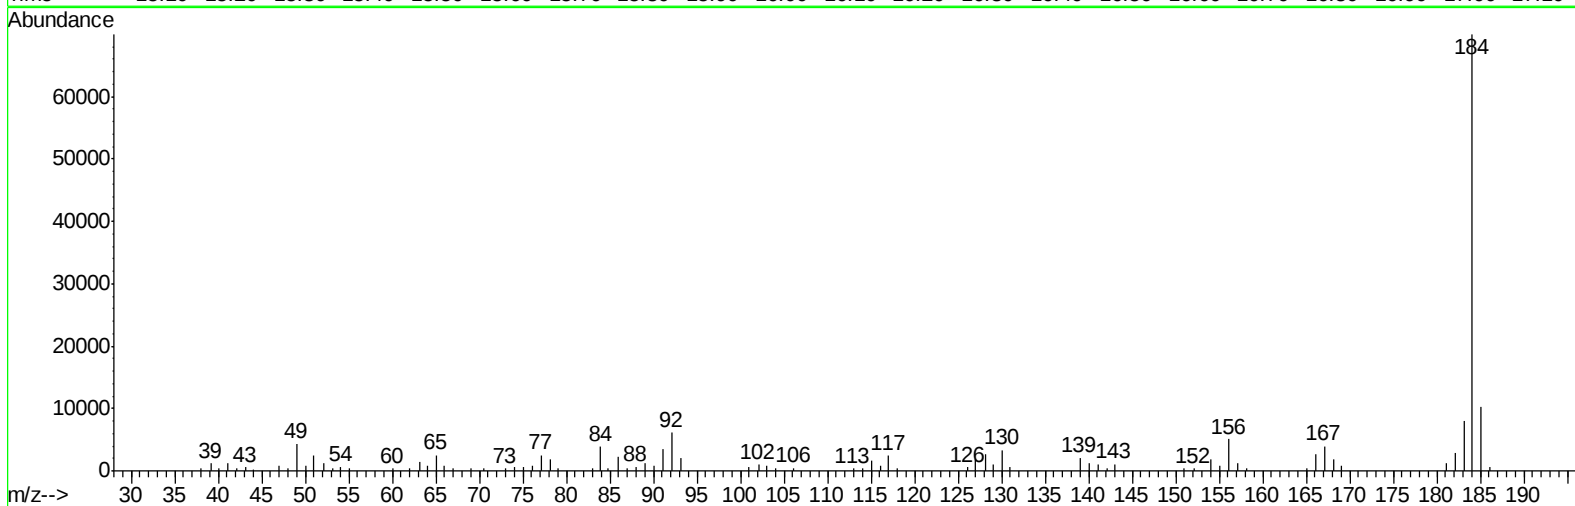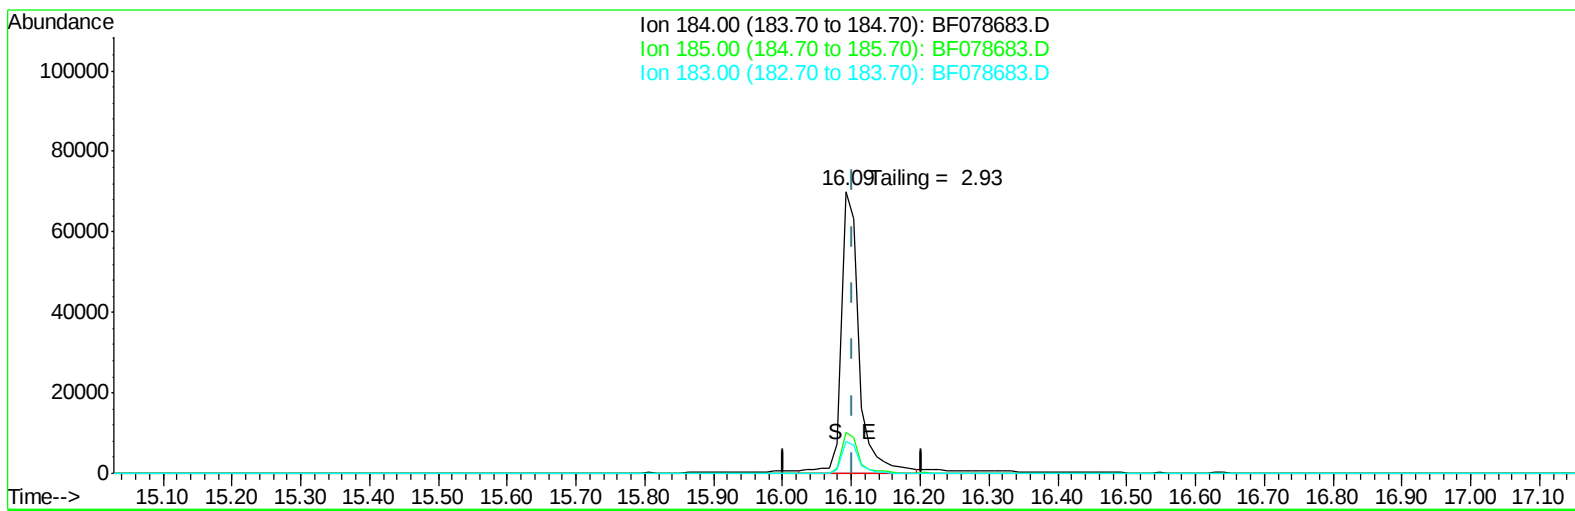

TIC: BF078683.D

(76) Benzidine

16.091min (-0.011) 0.00ng

response 116007

Ion	Exp%	Act%
184.00	100	100
185.00	15.20	14.58
183.00	11.90	11.31
0.00	0.00	0.00