

Data Path : Z:\HPCHEM1\BNA_F\DATA\BF042115\
 Data File : BF078698.D
 Acq On : 21 Apr 2015 22:40
 Operator : TP/IZ
 Sample : G1938-01 5X
 Misc :
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 SB-68AS

Integration Parameters: rteint.p
 Integrator: RTE
 Smoothing : ON Filtering: 5
 Sampling : 1 Min Area: 3 % of largest Peak
 Start Thrs: 0.2 Max Peaks: 100
 Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF040115.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.427	19	21	26	rVV	20229	45317	1.75%	0.766%
2	1.507	26	28	63	rVB	1304582	2589478	100.00%	43.786%
3	3.839	230	232	238	rVB	69503	91325	3.53%	1.544%
4	5.324	360	362	368	rBV	75382	96397	3.72%	1.630%
5	5.462	371	374	378	rVB	77903	108483	4.19%	1.834%
6	5.816	402	405	408	rBV	169027	196094	7.57%	3.316%
7	6.056	423	426	429	rBV	69195	80074	3.09%	1.354%
8	6.753	485	487	493	rVB	47376	59520	2.30%	1.006%
9	7.976	591	594	597	rBV	219838	278626	10.76%	4.711%
10	9.988	768	770	773	rBV	117360	136794	5.28%	2.313%
11	11.165	870	873	876	rBB	262638	340134	13.14%	5.751%
12	12.639	999	1002	1005	rBB	50661	68687	2.65%	1.161%
13	13.897	1109	1112	1115	rBV	265319	350698	13.54%	5.930%
14	15.828	1279	1281	1285	rVB2	49245	92026	3.55%	1.556%
15	16.137	1306	1308	1311	rBV2	45348	57246	2.21%	0.968%
16	16.434	1331	1334	1336	rVB	117523	167300	6.46%	2.829%
17	17.771	1445	1451	1453	rBV	323467	524643	20.26%	8.871%
18	19.040	1559	1562	1567	rBV	40854	102590	3.96%	1.735%
19	19.394	1591	1593	1596	rBV	35418	41167	1.59%	0.696%
20	19.463	1596	1599	1601	rBV	332064	452826	17.49%	7.657%
21	20.606	1697	1699	1704	rVB2	18629	34571	1.34%	0.585%




Sum of corrected areas: 5913996

Data Path : Z:\HPCHEM1\BNA_F\DATA\BF042115\
Data File : BF078698.D
Acq On : 21 Apr 2015 22:40
Operator : TP/IZ
Sample : G1938-01 5X
Misc :
ALS Vial : 16 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
SB-68AS

Quant Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF040115.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST02.L
TIC Integration Parameters: LSCINT.P

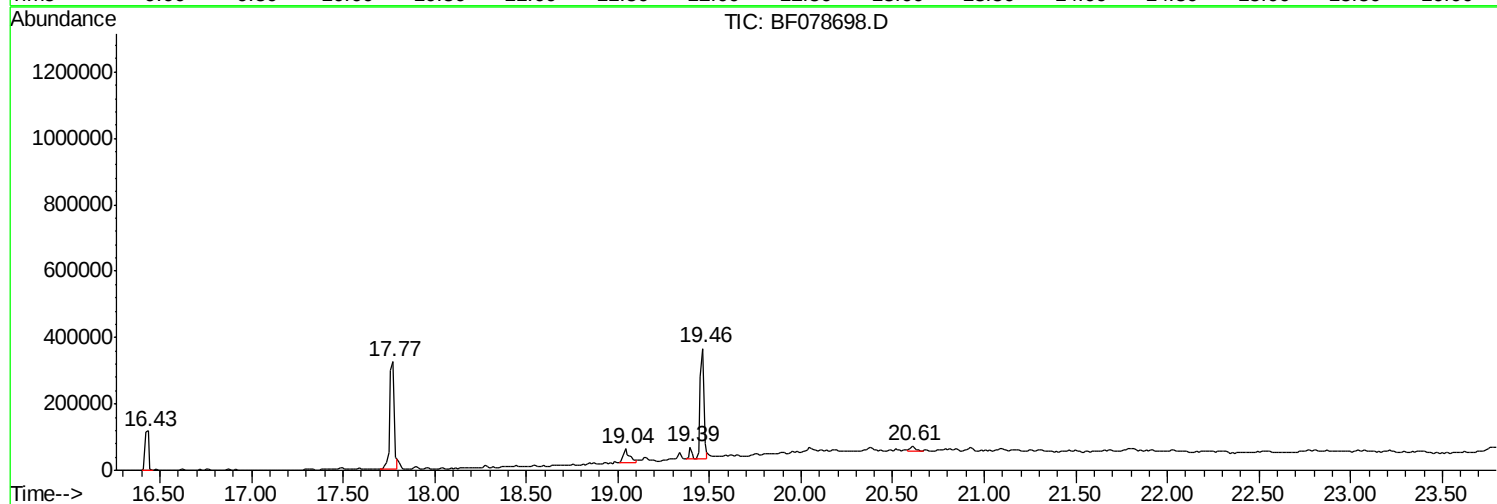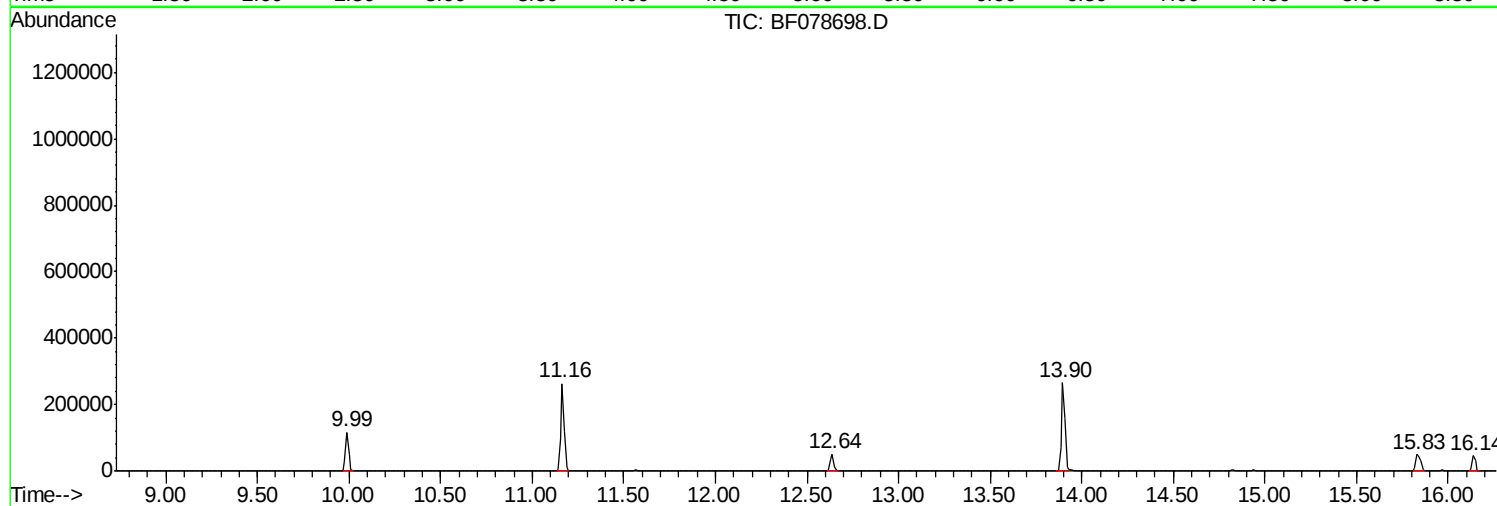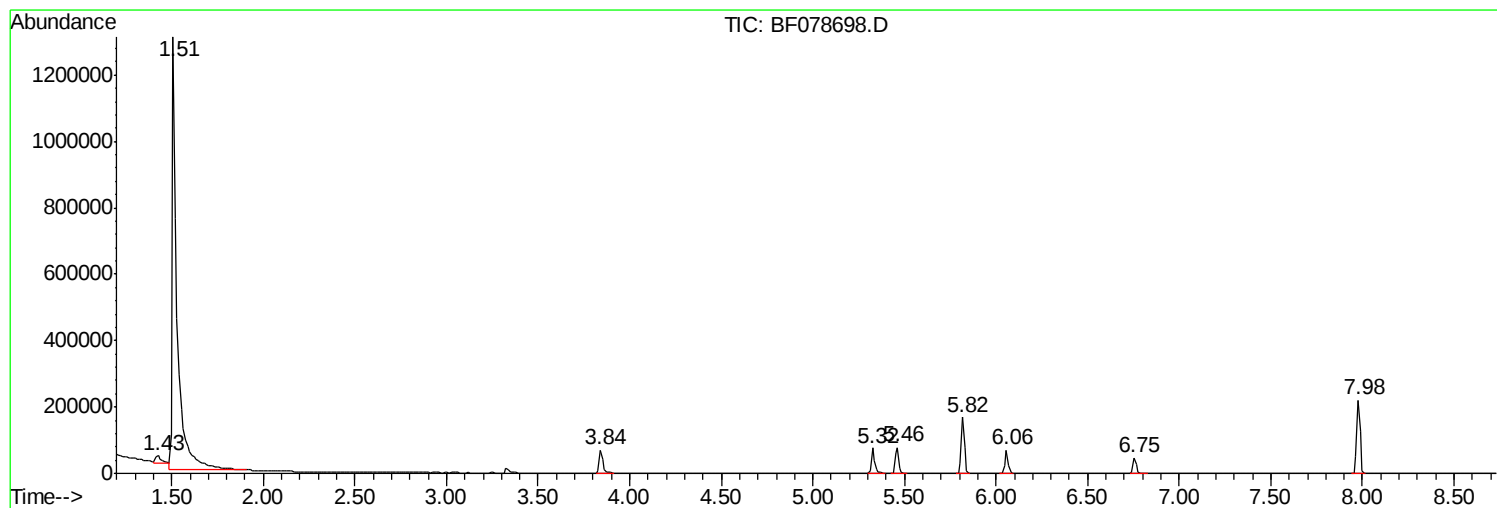

Data Path : Z:\HPCHEM1\BNA F\DATA\BF042115\
Data File : BF078698.D
Acq On : 21 Apr 2015 22:40
Operator : TP/IZ
Sample : G1938-01 5X
Misc :
ALS Vial : 16 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
SB-68AS










Quant Method : Z:\HPCHEM1\BNA F\METHODS\8270-BF040115.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST02.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 unknown1.43 Concentration Rank 4

R.T.	EstConc	Area	Relative to ISTD	R.T.
1.43	4.62 ng	45317	1,4-Dichlorobenzene-d4	5.82

Hit#	of	5	Tentative ID	MW	MolForm	CAS#	Qual
1			Manganese(II) acetate	173	C4H6MnO4	006156-78-1	40
2			Acetone	58	C3H6O	000067-64-1	9
3			Formic acid, chloro-, (3,4,4-tri...	194	C7H11ClO4	107323-92-2	4
4			1,4-Butanediamine	88	C4H12N2	000110-60-1	4
5			Oxirane, (propoxymethyl)-	116	C6H12O2	003126-95-2	4

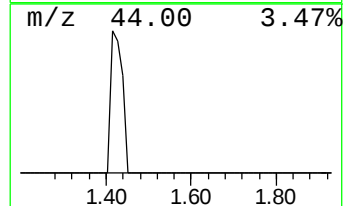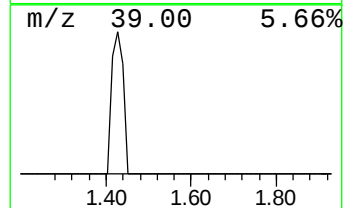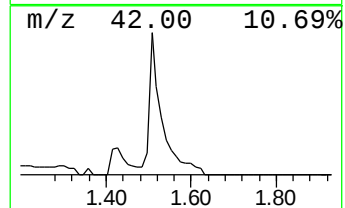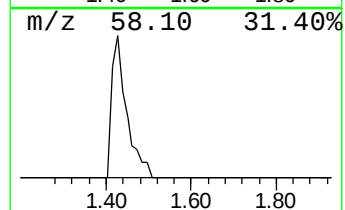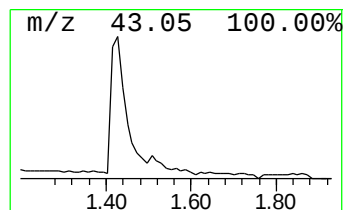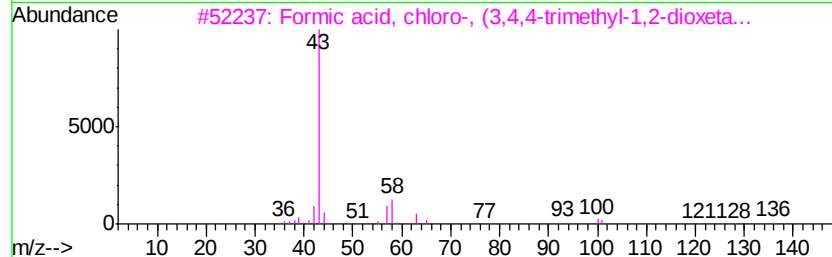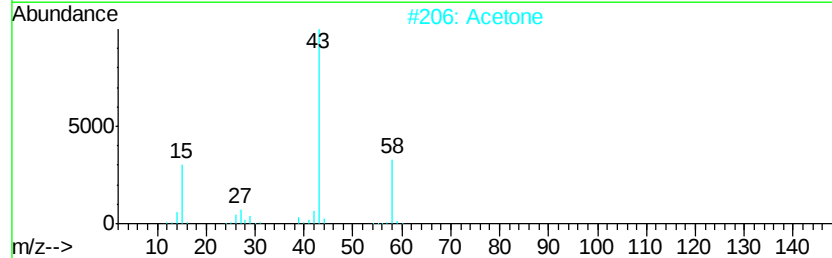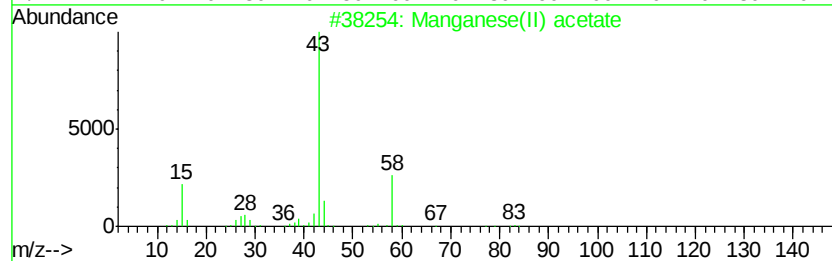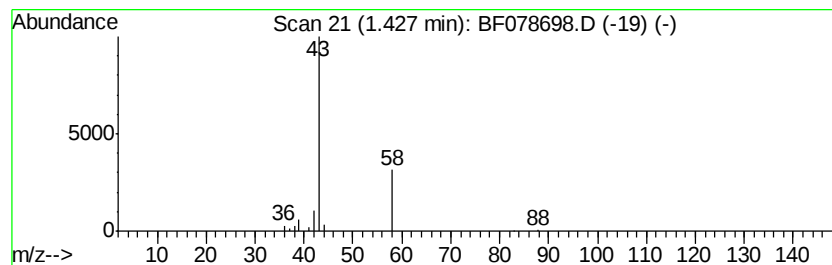

Data Path : Z:\HPCHEM1\BNA_F\DATA\BF042115\
Data File : BF078698.D
Acq On : 21 Apr 2015 22:40
Operator : TP/IZ
Sample : G1938-01 5X
Misc :
ALS Vial : 16 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
SB-68AS










Quant Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF040115.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST02.L
TIC Integration Parameters: LSCINT.P

Peak Number 3 unknown5.46 Concentration Rank 2

R.T.	EstConc	Area	Relative to ISTD	R.T.
5.46	11.06 ng	108483	1,4-Dichlorobenzene-d4	5.82

Hit#	of	Tentative ID	MW	MolForm	CAS#	Qual
1	5	3-Chloro-6-fluoro-pyrazine	132	C4H2ClFN2	1000146-10-7	25
2		Amphetaminil	250	C17H18N2	017590-01-1	12
3		(E)-3-Chloro-2-methyl-2-pentenal	132	C6H9ClO	031357-76-3	12
4		5-Aminoindole	132	C8H8N2	005192-03-0	10
5		4-Chloro-2-fluoro-pyrimidine	132	C4H2ClFN2	051422-00-5	9

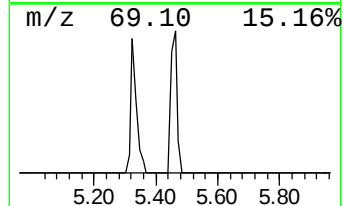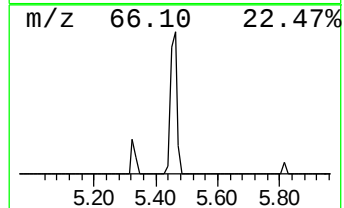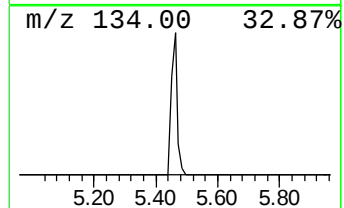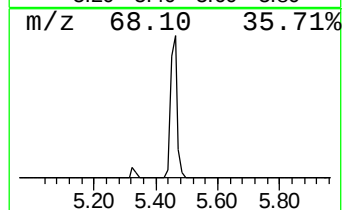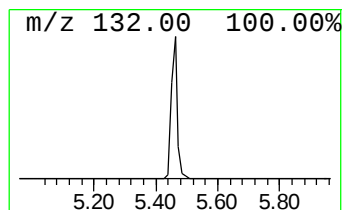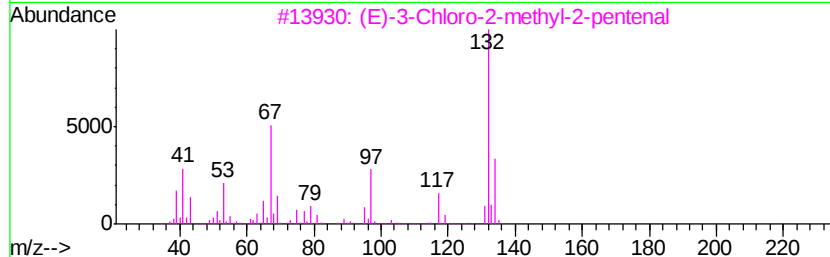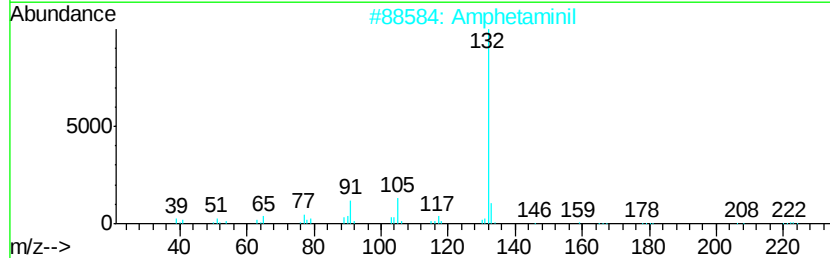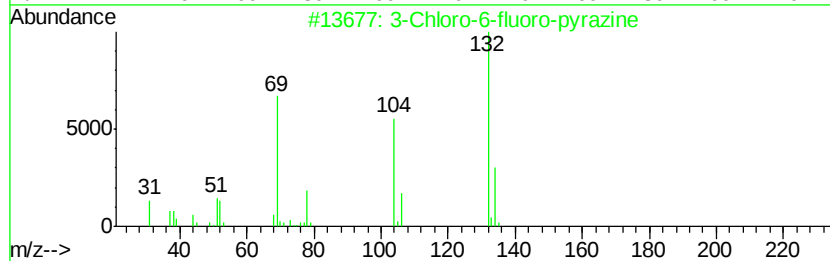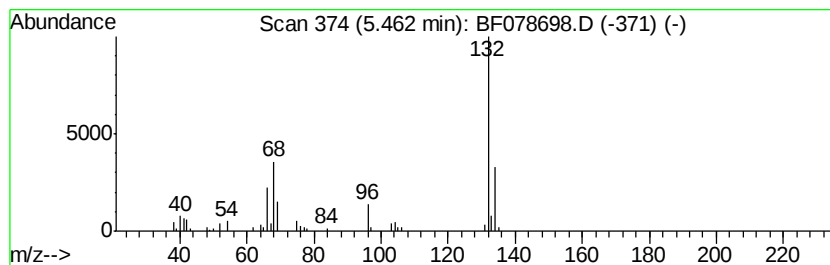

Data Path : Z:\HPCHEM1\BNA_F\DATA\BF042115\
Data File : BF078698.D
Acq On : 21 Apr 2015 22:40
Operator : TP/IZ
Sample : G1938-01 5X
Misc :
ALS Vial : 16 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
SB-68AS

Quant Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF040115.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST02.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
unknown1.43	1.43	4.6	ng	45317	1	5.82	196094	20.0
unknown5.46	5.46	11.1	ng	108483	1	5.82	196094	20.0