
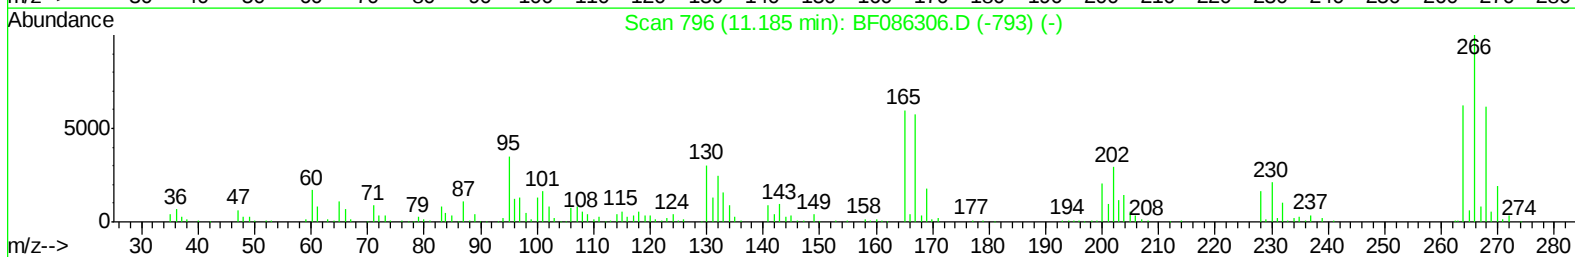
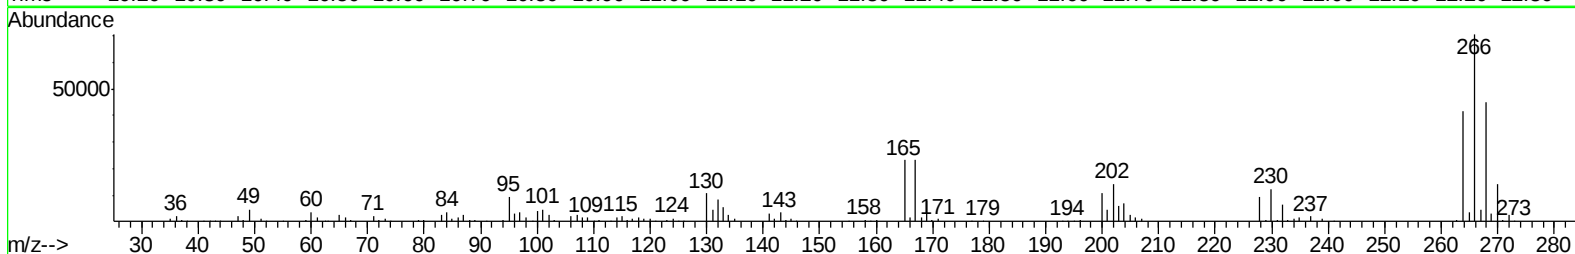


Data Path : Z:\HPCHEM1\BNA_F\DATA\BF042116\
Data File : BF086345.D
Acq On : 21 Apr 2016 14:26
Operator : UM/SJ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Apr 22 01:19:01 2016
Quant Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF042016.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Apr 20 15:45:26 2016
Response via : Initial Calibration

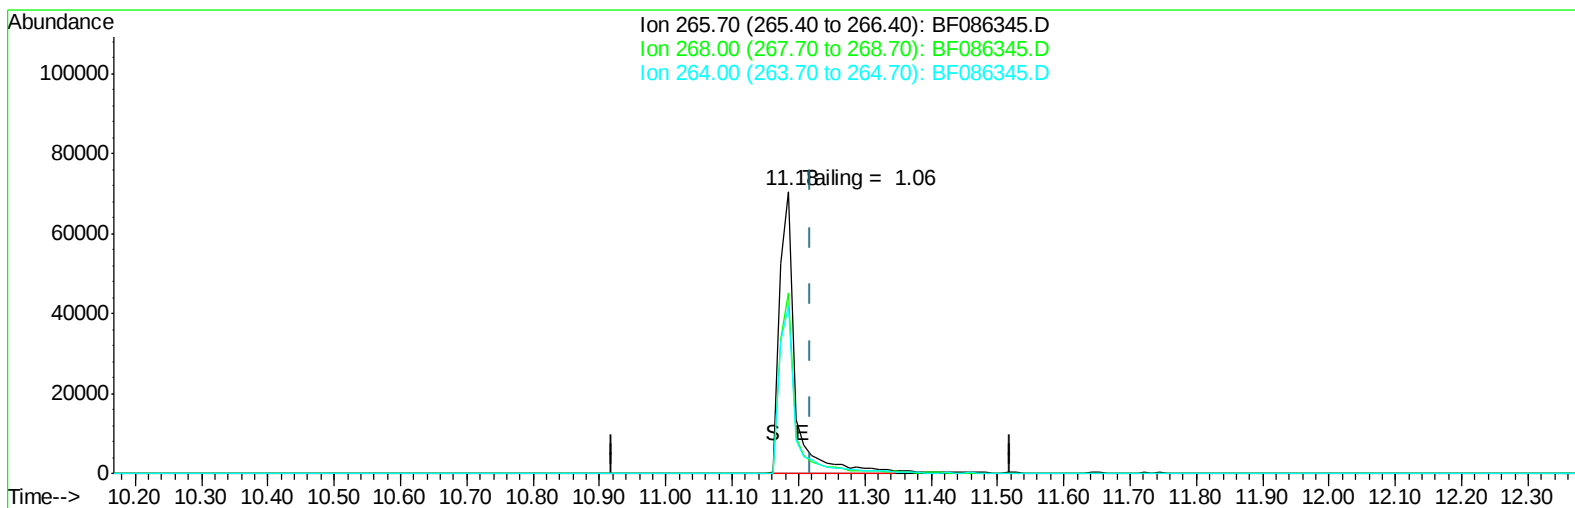

TIC: BF086345.D

(69) Pentachlorophenol (C)




11.185min (-0.034) 25287.30ng

response 110140

Ion	Exp%	Act%
265.70	100	100
268.00	66.20	63.91
264.00	64.10	59.40
0.00	0.00	0.00

Data Path : Z:\HPCHEM1\BNA_F\DATA\BF042116\
Data File : BF086345.D
Acq On : 21 Apr 2016 14:26
Operator : UM/SJ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Apr 22 01:19:01 2016
Quant Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF042016.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Apr 20 15:45:26 2016
Response via : Initial Calibration

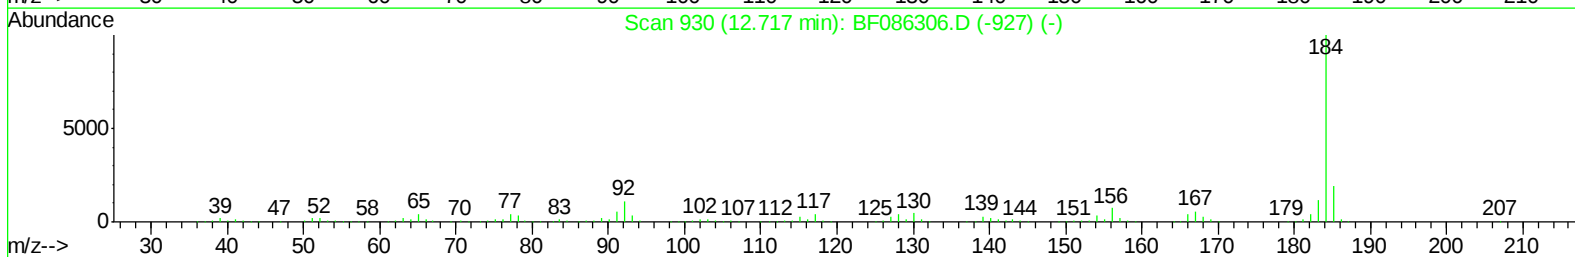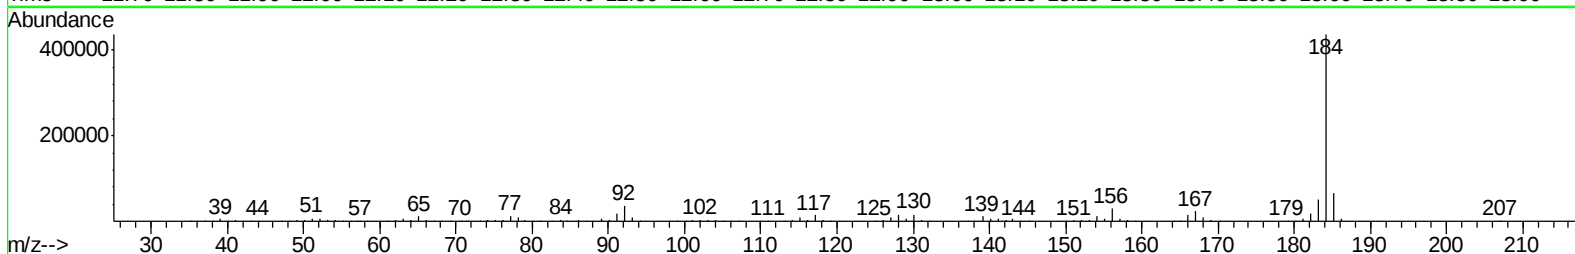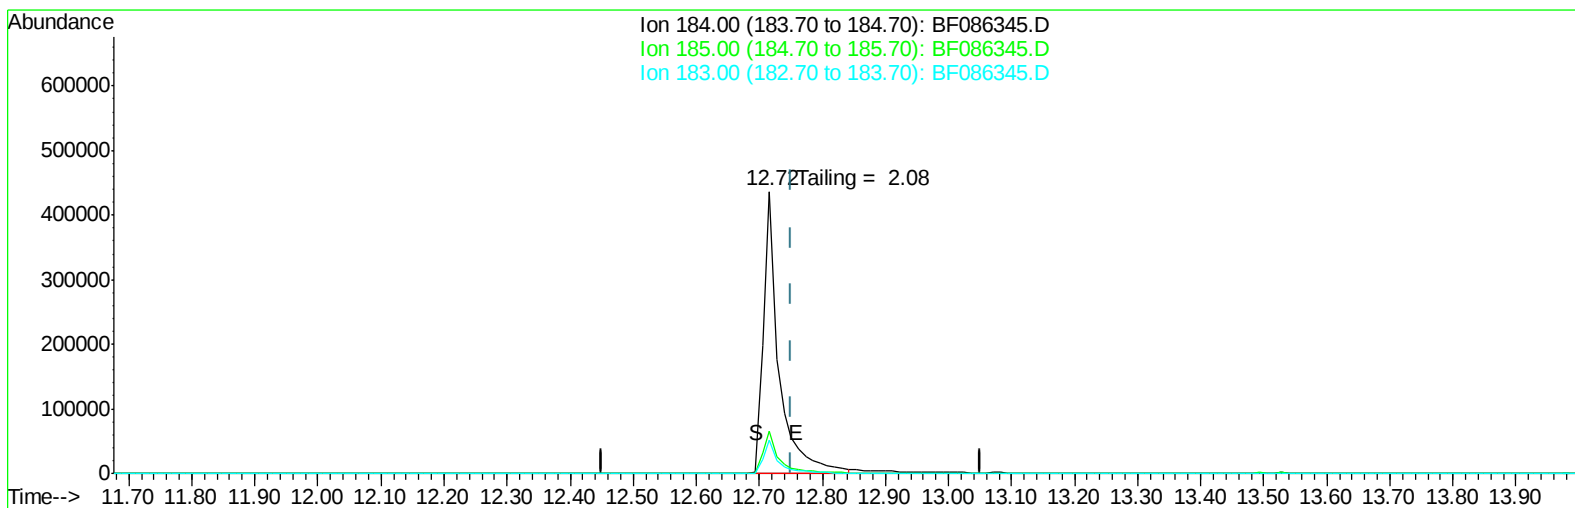

TIC: BF086345.D

(76) Benzidine

12.717min (-0.034) 0.00ng

response 778139

Ion	Exp%	Act%
184.00	100	100
185.00	17.70	14.98
183.00	12.20	11.74
0.00	0.00	0.00