

Data Path : Z:\HPCHEM1\BNA F\DATA\BF042117\
 Data File : BF094573.D
 Acq On : 21 Apr 2017 20:09
 Operator : SJ/MA
 Sample : I2786-04
 Misc :
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :

Quant Time: Apr 21 23:37:29 2017
 Quant Method : Z:\HPCHEM1\BNA F\METHODS\8270-BF041717.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Mon Apr 17 14:59:23 2017
 Response via : Initial Calibration


Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	5.76	152	104814	20.00	ng	0.00
21) Naphthalene-d8	7.25	136	417576	20.00	ng	0.00
38) Acenaphthene-d10	9.39	164	187044	20.00	ng	0.00
63) Phenanthrene-d10	11.21	188	318902	20.00	ng	-0.01
75) Chrysene-d12	14.45	240	267347	20.00	ng	-0.01
86) Perylene-d12	16.08	264	266627	20.00	ng	0.00
System Monitoring Compounds						
5) 2-Fluorophenol	4.31	112	694084	109.86	ng	0.00
7) Phenol-d6	5.39	99	853340	114.57	ng	0.00
23) Nitrobenzene-d5	6.41	82	520246	76.93	ng	0.00
41) 2,4,6-Tribromophenol	10.37	330	168548	115.20	ng	0.00
44) 2-Fluorobiphenyl	8.58	172	1018041	80.08	ng	0.00
78) Terphenyl-d14	13.18	244	760461	76.03	ng	-0.01
Target Compounds						
9) Benzaldehyde	5.51	77	14719	2.60	ng	Qvalue 83
10) Phenol	5.40	94	46793	5.11	ng	89
19) n-Nitroso-di-n-propylamine	6.41	70	70236	14.23	ng	# 75
49) Dimethylphthalate	9.08	163	224349	16.09	ng	98
56) 2,4-Dinitrotoluene	9.39	165	23616	6.15	ng	# 31

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\HPCHEM1\BNA F\DATA\BF042117\
Data File : BF094573.D
Acq On : 21 Apr 2017 20:09
Operator : SJ/MA
Sample : I2786-04
Misc :
ALS Vial : 16 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :

Quant Time: Apr 21 23:37:29 2017
Quant Method : Z:\HPCHEM1\BNA F\METHODS\8270-BF041717.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Apr 17 14:59:23 2017
Response via : Initial Calibration

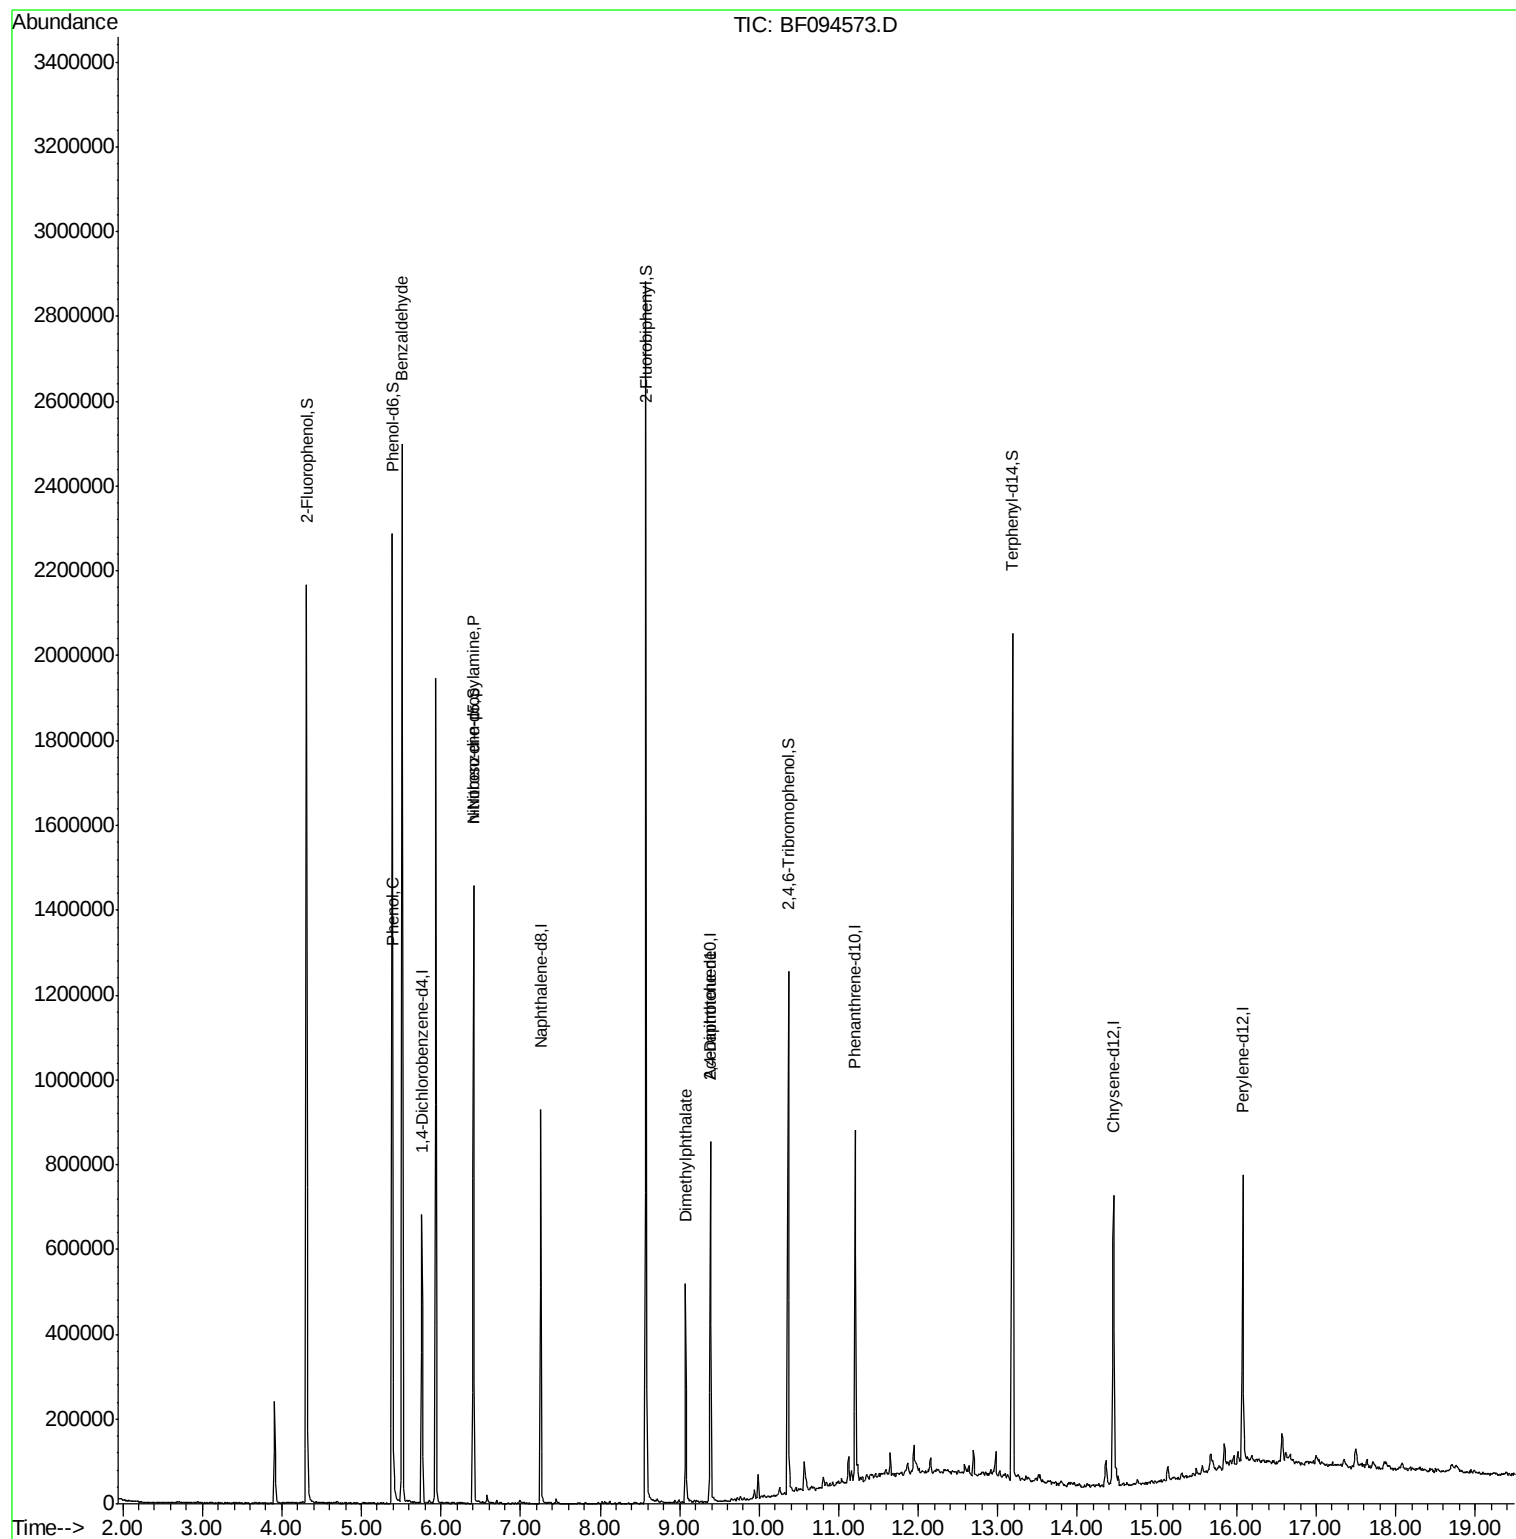




#1




1,4-Dichlorobenzene-d4
 Concen: 20.00 ng
 RT: 5.76 min Scan# 650
 Delta R.T. -0.00 min
 Lab File: BF094573.D
 Acq: 21 Apr 2017 20:09

Instrument :
 BNA_F
 ClientSampleId :

Tot Ion:152 Resp: 104814
 Ion Ratio Lower Upper
 152 100
 150 160.4 126.2 189.2
 115 62.5 52.2 78.2

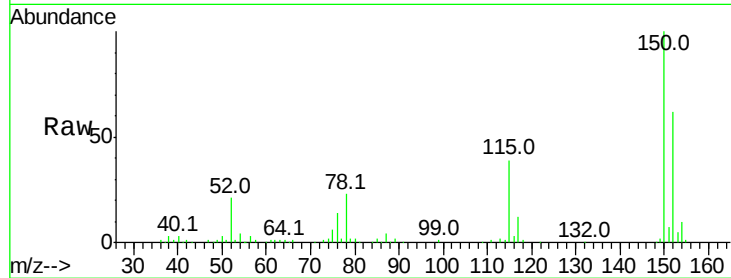


Abundance Ion 152.00 (151.70 to 152.70): E
 Ion 150.00 (149.70 to 150.70): E
 Ion 115.00 (114.70 to 115.70): E

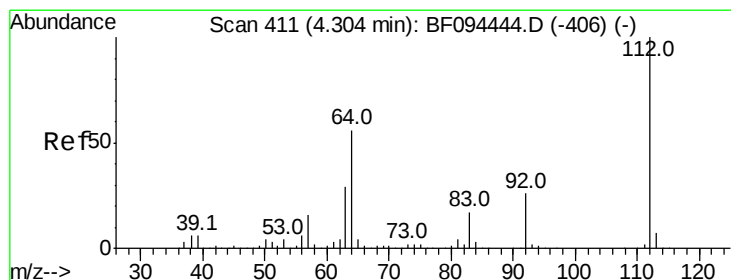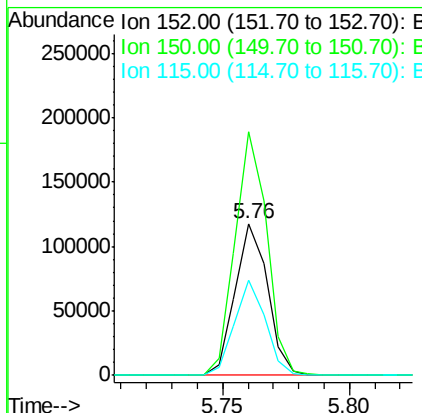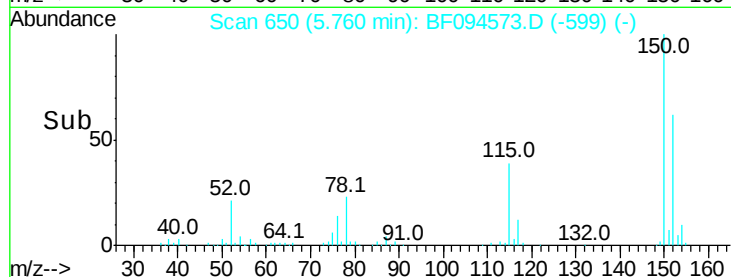



#5


2-Fluorophenol
 Concen: 109.86 ng
 RT: 4.31 min Scan# 404
 Delta R.T. 0.01 min
 Lab File: BF094573.D
 Acq: 21 Apr 2017 20:09

Tgt Ion:112 Resp: 694084
 Ion Ratio Lower Upper
 112 100
 64 54.4 46.0 69.0
 63 26.3 23.4 35.0

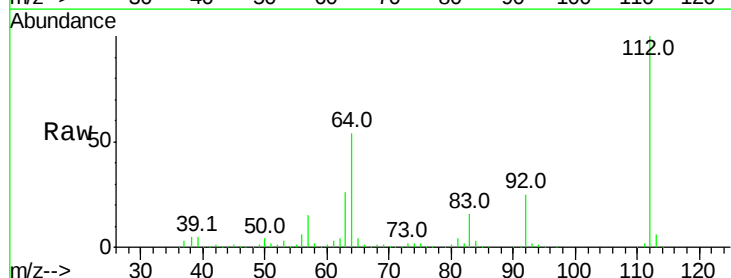

Abundance Ion 112.00 (111.70 to 112.70): E
 Ion 64.00 (63.70 to 64.70): BF0
 Ion 63.00 (62.70 to 63.70): BF0

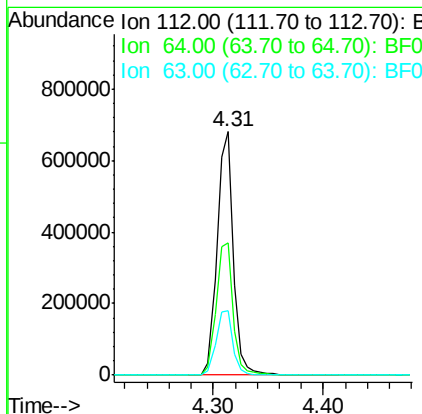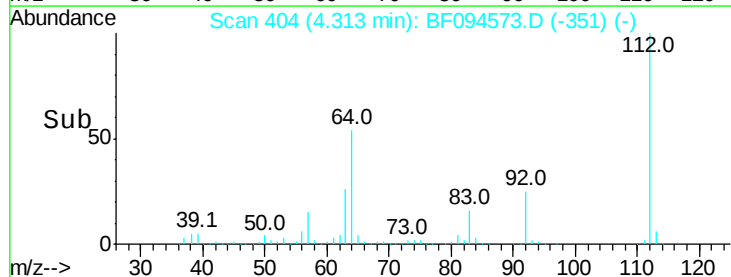

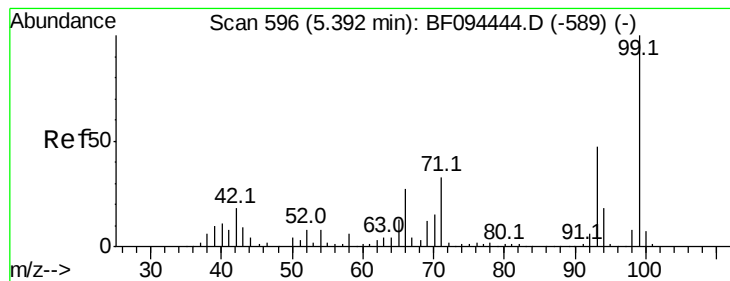

#7

Phenol-d6

Concen: 114.57 ng

RT: 5.39 min Scan# 587

Delta R.T. -0.00 min

Lab File: BF094573.D

Acq: 21 Apr 2017 20:09

Instrument :

BNA_F

ClientSampleId :


Tot Ion: 99 Resp: 853340

Ion Ratio Lower Upper




99 100

42 17.4 13.5 20.3

71 32.7 24.5 36.7

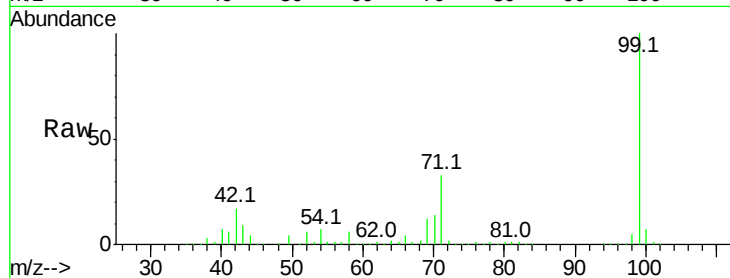

Abundance Ion 99.00 (98.70 to 99.70): BF0
Ion 42.00 (41.70 to 42.70): BF0
Ion 71.00 (70.70 to 71.70): BF0

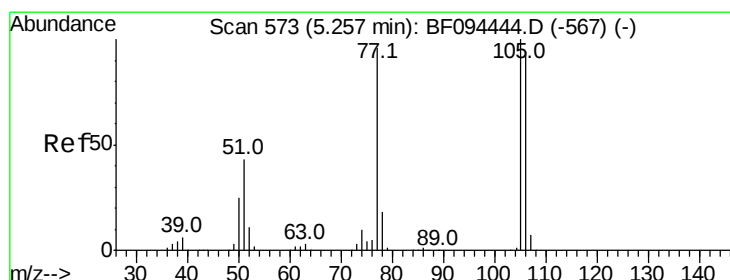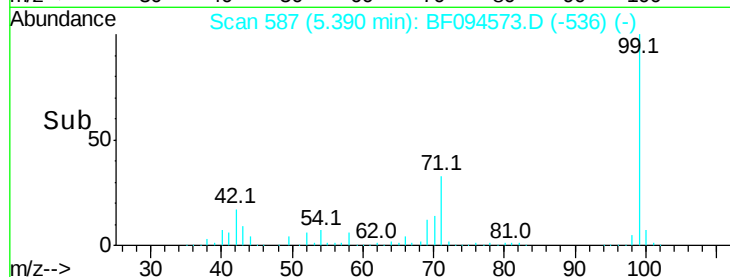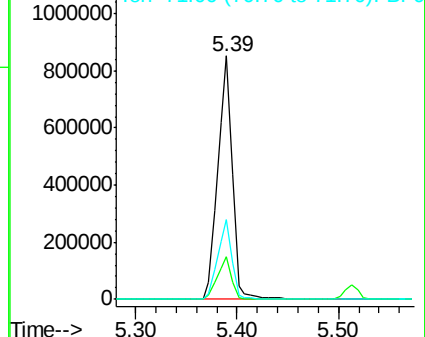

#9

Benzaldehyde

Concen: 2.60 ng

RT: 5.51 min Scan# 608

Delta R.T. 0.26 min

Lab File: BF094573.D

Acq: 21 Apr 2017 20:09


Tgt Ion: 77 Resp: 14719

Ion Ratio Lower Upper



77 100


105 85.2 83.8 123.8

106 84.3 79.1 119.1

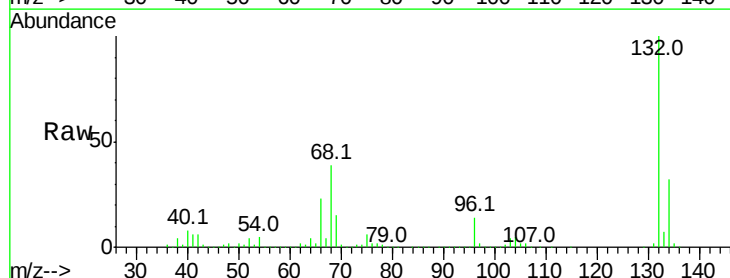

Abundance Ion 77.00 (76.70 to 77.70): BF0
Ion 105.00 (104.70 to 105.70): E
Ion 106.00 (105.70 to 106.70): E

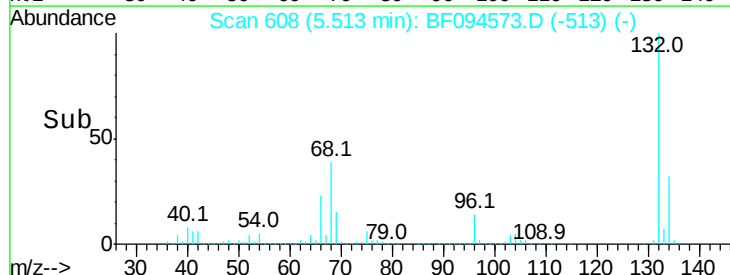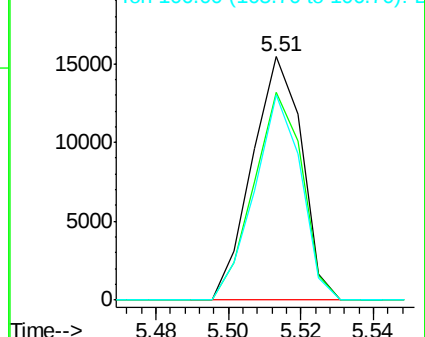

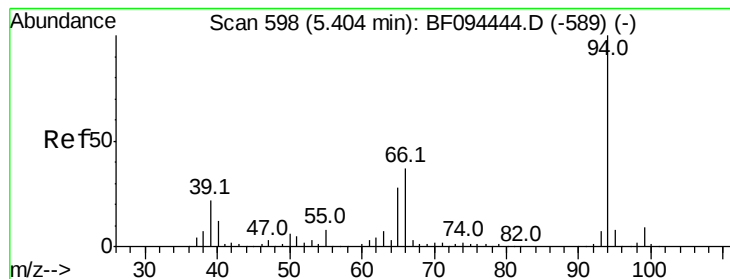

#10

Phenol

Concen: 5.11 ng

RT: 5.40 min Scan# 589

Delta R.T. -0.00 min

Lab File: BF094573.D

Acq: 21 Apr 2017 20:09

Instrument :

BNA_F

ClientSampled :


Tot Ion: 94 Resp: 46793

Ion Ratio Lower Upper

94 100

65 26.9 9.9 49.9




66 34.1 23.1 63.1

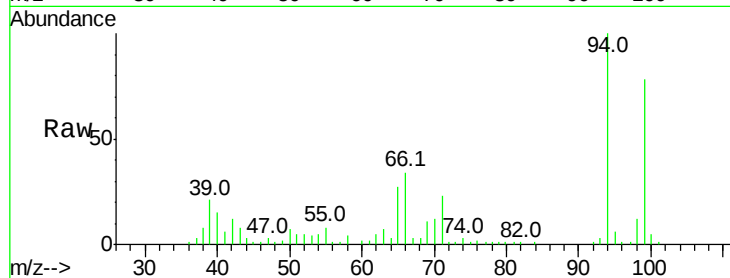

Abundance Ion 94.00 (93.70 to 94.70): BF0

Ion 65.00 (64.70 to 65.70): BF0

Ion 66.00 (65.70 to 66.70): BF0

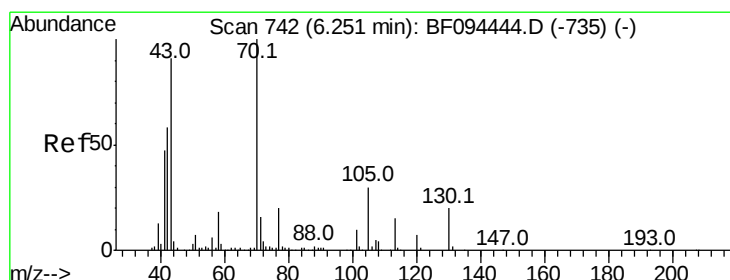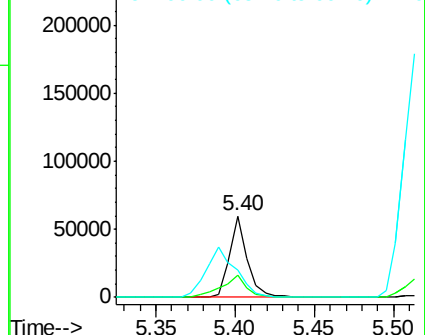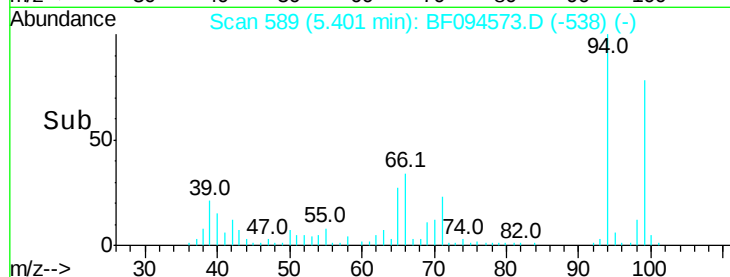

#19

n-Nitroso-di-n-propylamine

Concen: 14.23 ng

RT: 6.41 min Scan# 761

Delta R.T. 0.16 min

Lab File: BF094573.D

Acq: 21 Apr 2017 20:09

Tgt Ion: 70 Resp: 70236


Ion Ratio Lower Upper

70 100

42 43.3 47.2 70.8#

101 0.0 7.2 10.8#

130 2.2 15.9 23.9#


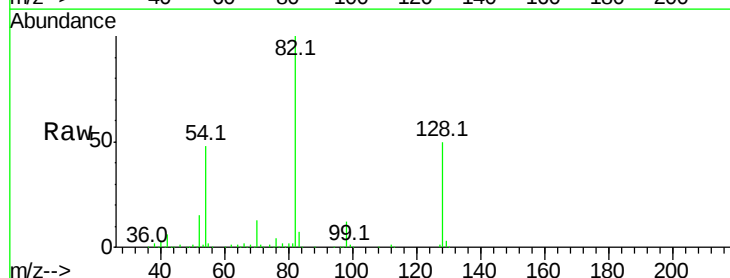



Abundance Ion 70.00 (69.70 to 70.70): BF0

Ion 42.00 (41.70 to 42.70): BF0

Ion 101.00 (100.70 to 101.70): BF0

Ion 130.00 (129.70 to 130.70): BF0

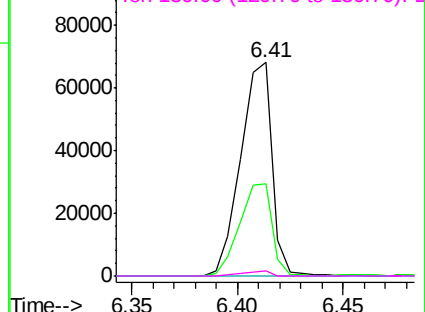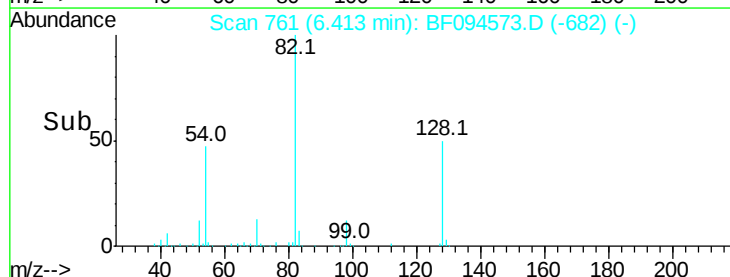

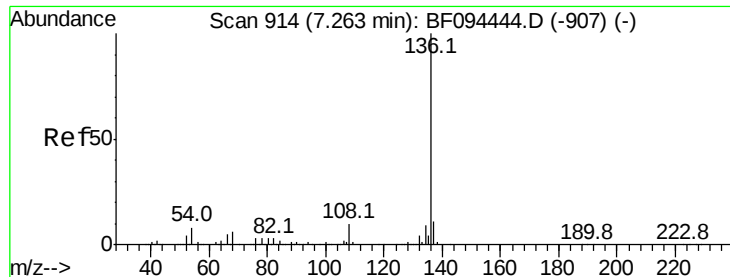

#21

Naphthalene-d8

Concen: 20.00 ng

RT: 7.25 min Scan# 904

Delta R.T. -0.01 min

Lab File: BF094573.D

Acq: 21 Apr 2017 20:09

Instrument :

BNA_F

ClientSampleId :

Tot Ion:136 Resp: 417576


Ion Ratio Lower Upper

136 100

137 11.4 8.5 12.7

54 7.4 4.9 7.3#

68 5.6 4.1 6.1



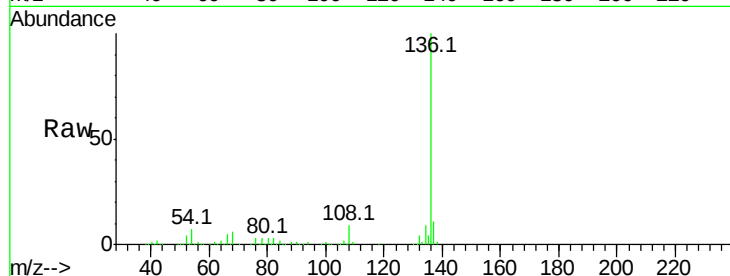


Abundance Ion 136.00 (135.70 to 136.70): E

Ion 137.00 (136.70 to 137.70): E

Ion 54.00 (53.70 to 54.70): BF0

Ion 68.00 (67.70 to 68.70): BF0

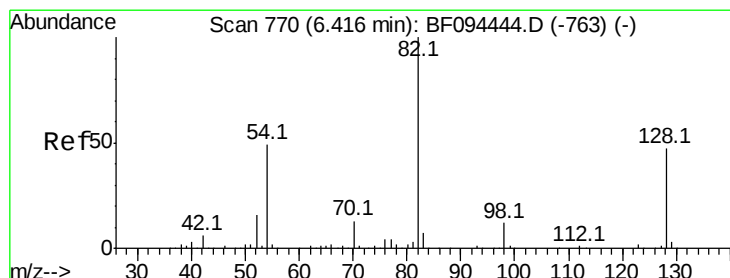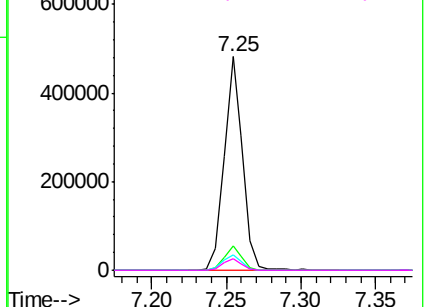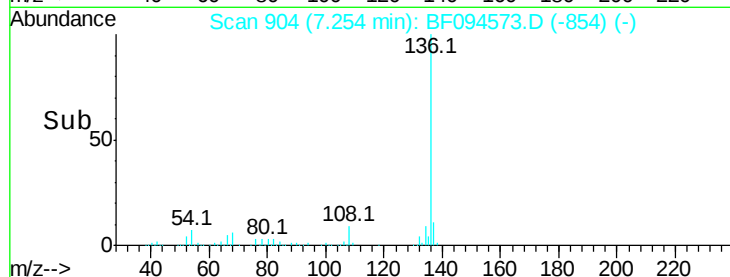

#23

Nitrobenzene-d5

Concen: 76.93 ng

RT: 6.41 min Scan# 761

Delta R.T. -0.00 min

Lab File: BF094573.D

Acq: 21 Apr 2017 20:09


Tgt Ion: 82 Resp: 520246

Ion Ratio Lower Upper

82 100

128 50.0 34.0 51.0



54 48.2 42.2 63.2

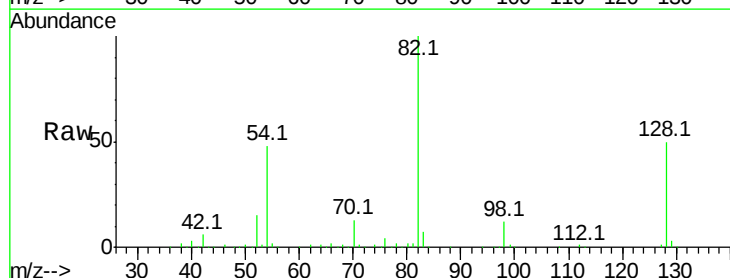


Abundance Ion 82.00 (81.70 to 82.70): BF0

Ion 128.00 (127.70 to 128.70): E

Ion 54.00 (53.70 to 54.70): BF0

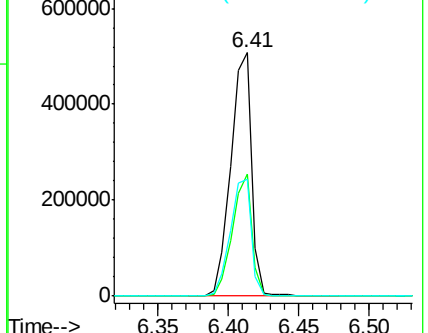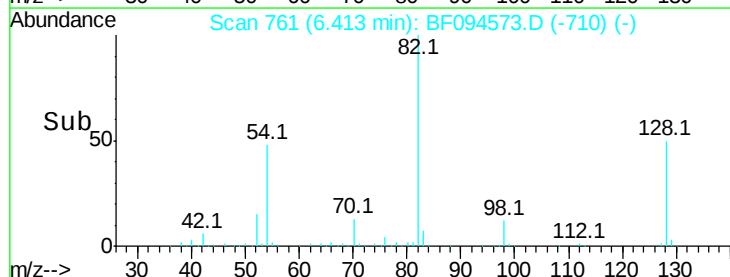


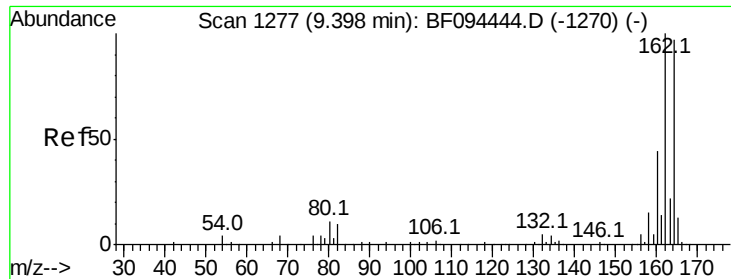




#38
Acenaphthene-d10
Concen: 20.00 ng
RT: 9.39 min Scan# 1267
Delta R.T. -0.01 min
Lab File: BF094573.D
Acq: 21 Apr 2017 20:09

Instrument :
BNA_F
ClientSampled :

Tot Ion:164 Resp: 187044
Ion Ratio Lower Upper
164 100
162 102.8 82.6 123.8
160 46.6 36.2 54.2

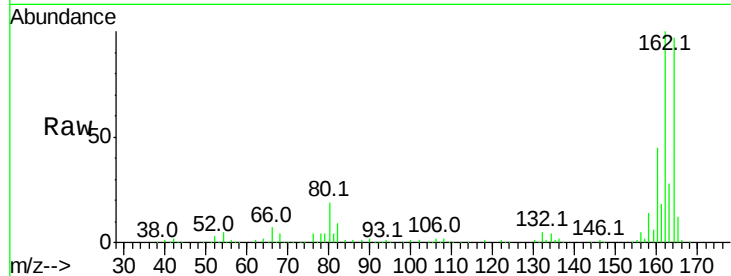


Abundance Ion 164.00 (163.70 to 164.70): E
Ion 162.00 (161.70 to 162.70): E
Ion 160.00 (159.70 to 160.70): E

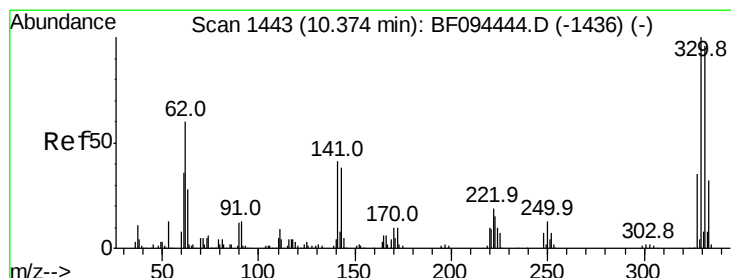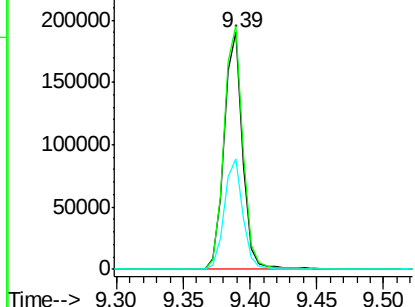
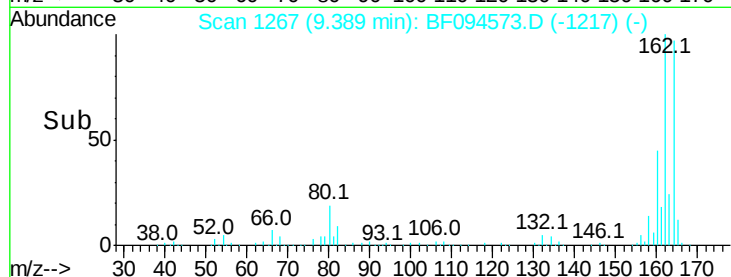



#41
2,4,6-Tribromophenol
Concen: 115.20 ng
RT: 10.37 min Scan# 1433
Delta R.T. -0.01 min
Lab File: BF094573.D
Acq: 21 Apr 2017 20:09

Tgt Ion:330 Resp: 168548
Ion Ratio Lower Upper
330 100
332 95.4 76.6 115.0
141 40.1 31.4 47.2

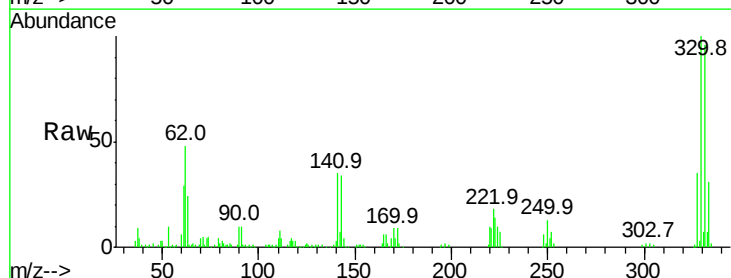

Abundance Ion 329.80 (329.50 to 330.50): E
Ion 331.80 (331.50 to 332.50): E
Ion 141.00 (140.70 to 141.70): E

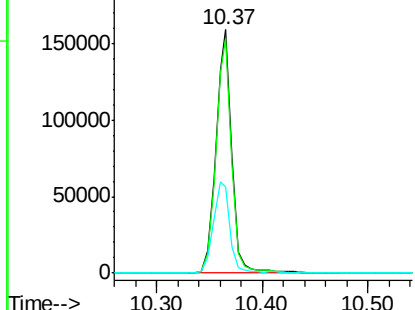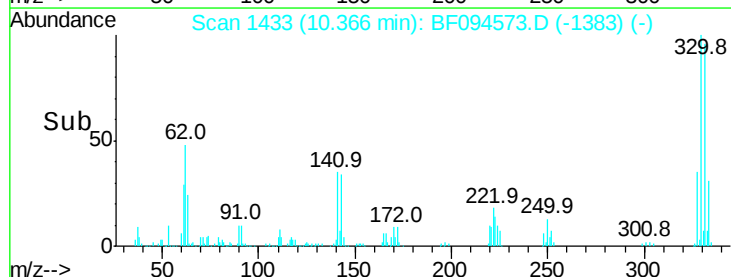


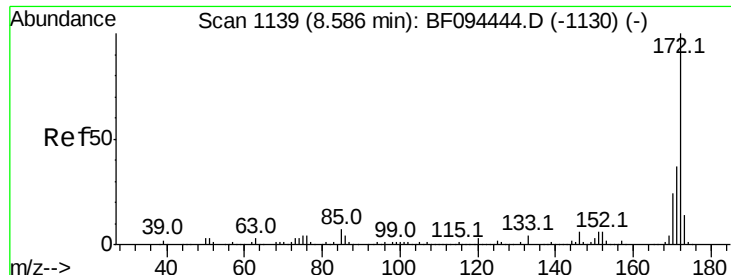




#44
2-Fluorobiphenyl
Concen: 80.08 ng
RT: 8.58 min Scan# 1129
Delta R.T. -0.01 min
Lab File: BF094573.D
Acq: 21 Apr 2017 20:09

Instrument :
BNA_F
ClientSampleId :

Tot Ion:172 Resp: 1018041
Ion Ratio Lower Upper
172 100
171 35.8 29.6 44.4
170 24.2 19.8 29.8

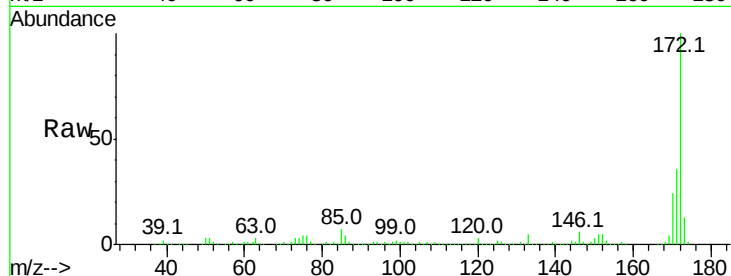


Abundance Ion 172.00 (171.70 to 172.70): E
Ion 171.00 (170.70 to 171.70): E
Ion 170.00 (169.70 to 170.70): E

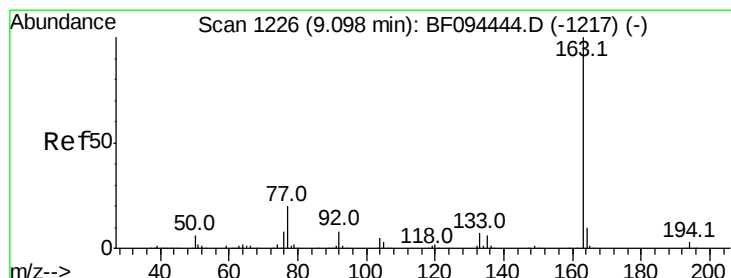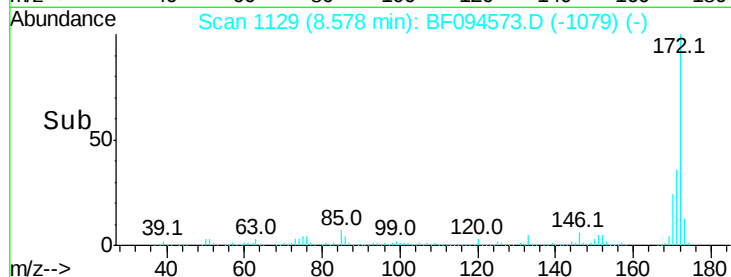
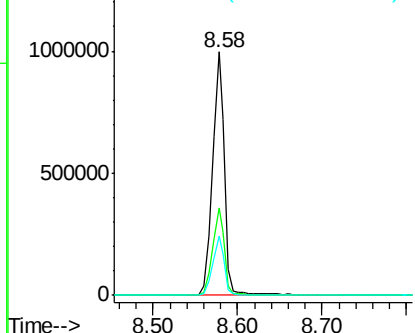



#49
Dimethylphthalate
Concen: 16.09 ng
RT: 9.08 min Scan# 1214
Delta R.T. -0.02 min
Lab File: BF094573.D
Acq: 21 Apr 2017 20:09

Tgt Ion:163 Resp: 224349
Ion Ratio Lower Upper
163 100
194 3.5 2.6 4.0
164 9.7 8.4 12.6

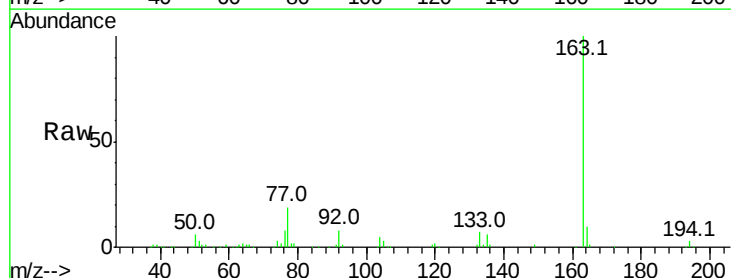

Abundance Ion 163.00 (162.70 to 163.70): E
Ion 194.00 (193.70 to 194.70): E
Ion 164.00 (163.70 to 164.70): E

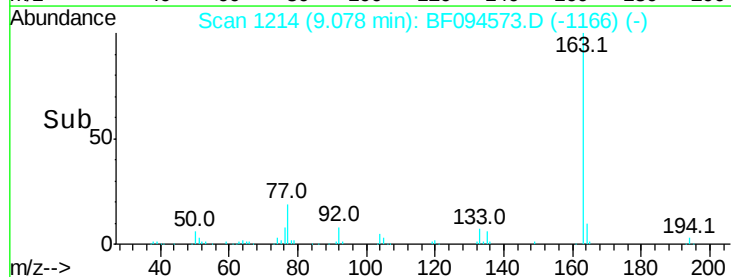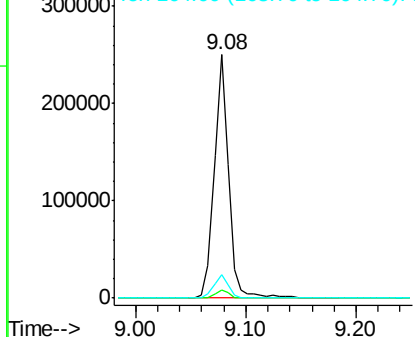


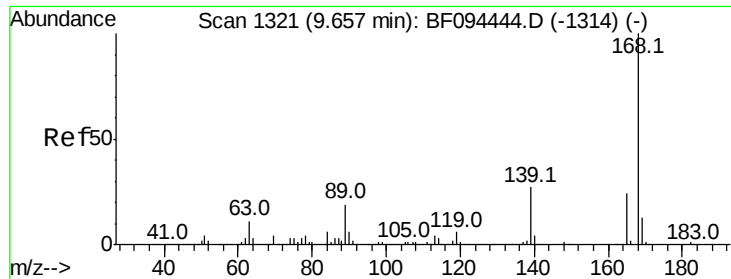




#56
 2,4-Dinitrotoluene
 Concen: 6.15 ng
 RT: 9.39 min Scan# 1267
 Delta R.T. -0.27 min
 Lab File: BF094573.D
 Acq: 21 Apr 2017 20:09

Instrument :
 BNA_F
 ClientSampleId :

Tot Ion:165 Resp: 23616
 Ion Ratio Lower Upper
 165 100
 63 0.0 25.4 38.0#
 89 0.0 46.4 69.6#
 182 0.0 1.8 2.6#

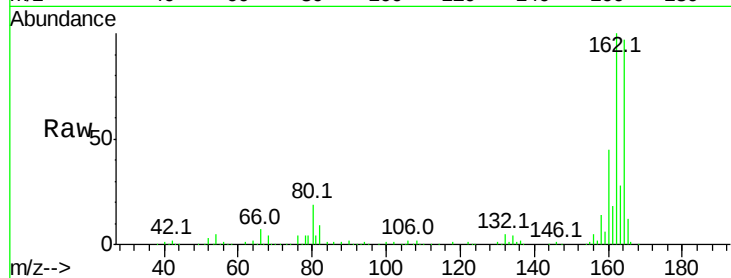


Abundance Ion 165.00 (164.70 to 165.70): E

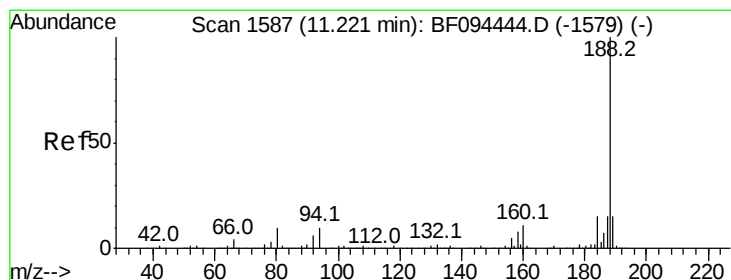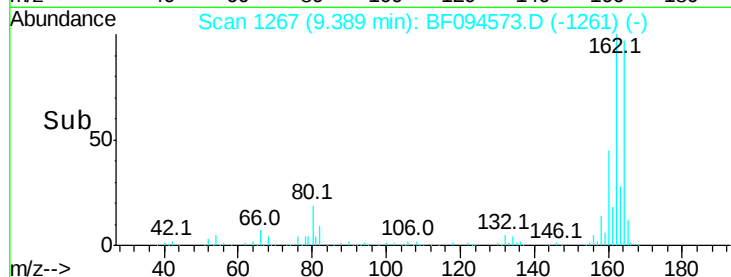
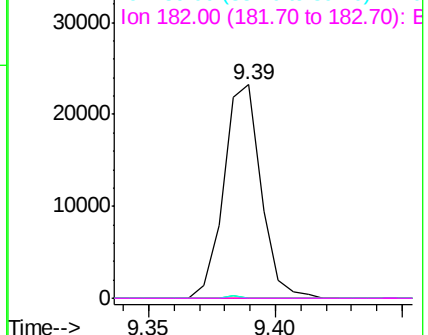



#63
 Phenanthrene-d10
 Concen: 20.00 ng
 RT: 11.21 min Scan# 1576
 Delta R.T. -0.01 min
 Lab File: BF094573.D
 Acq: 21 Apr 2017 20:09

Tgt Ion:188 Resp: 318902
 Ion Ratio Lower Upper
 188 100
 94 10.6 9.4 14.2
 80 11.8 10.2 15.2

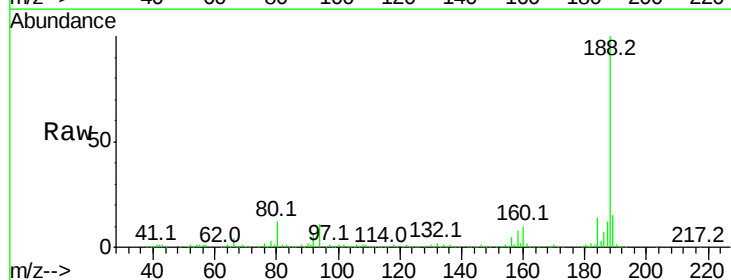

Abundance Ion 188.00 (187.70 to 188.70): E

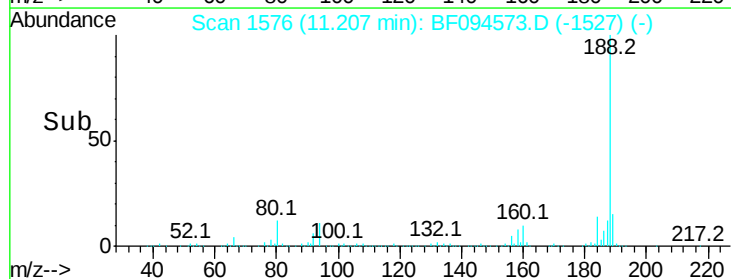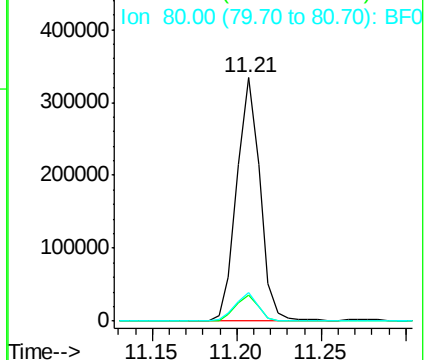

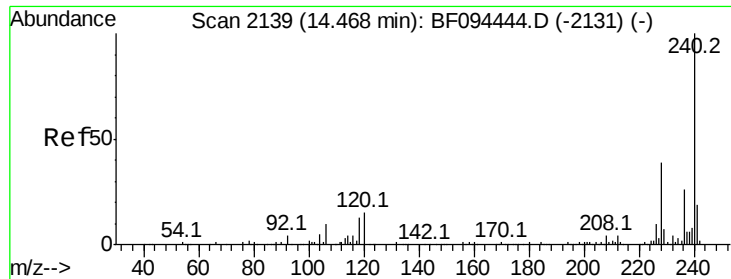

#75

Chrysene-d12

Concen: 20.00 ng

RT: 14.45 min Scan# 2128

Delta R.T. -0.01 min

Lab File: BF094573.D

Acq: 21 Apr 2017 20:09

Instrument :

BNA_F

ClientSampleId :


Tot Ion:240 Resp: 267347

Ion Ratio Lower Upper

240 100

120 13.7 5.8 8.8#




236 26.1 20.5 30.7

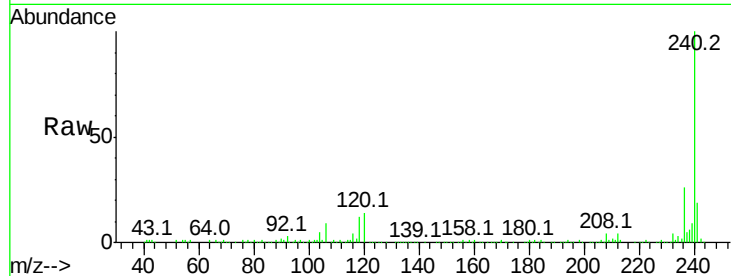

Abundance Ion 240.00 (239.70 to 240.70): E

Ion 120.00 (119.70 to 120.70): E

Ion 236.00 (235.70 to 236.70): E

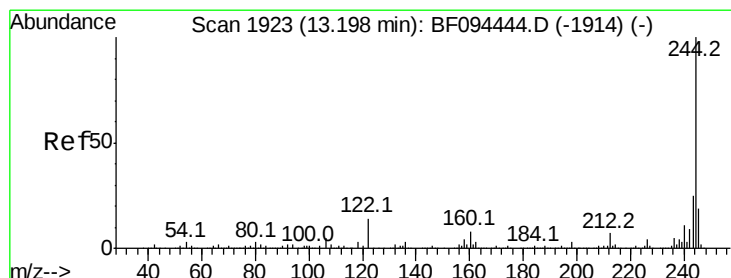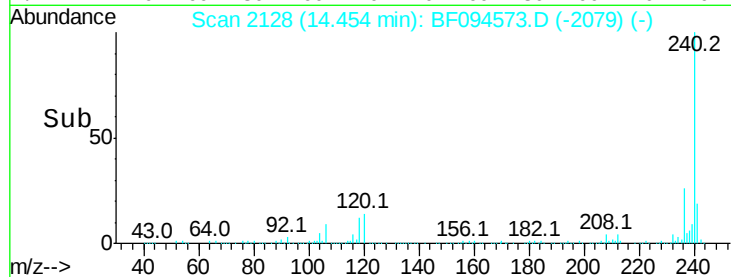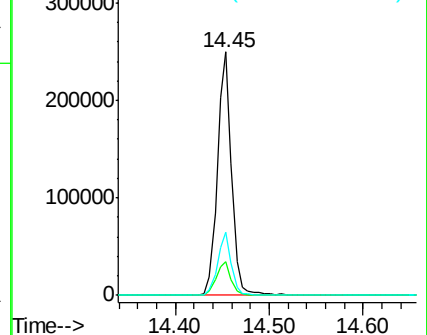

#78

Terphenyl-d14

Concen: 76.03 ng

RT: 13.18 min Scan# 1912

Delta R.T. -0.01 min

Lab File: BF094573.D

Acq: 21 Apr 2017 20:09


Tgt Ion:244 Resp: 760461

Ion Ratio Lower Upper

244 100

212 7.0 6.0 9.0



122 15.0 10.3 15.5

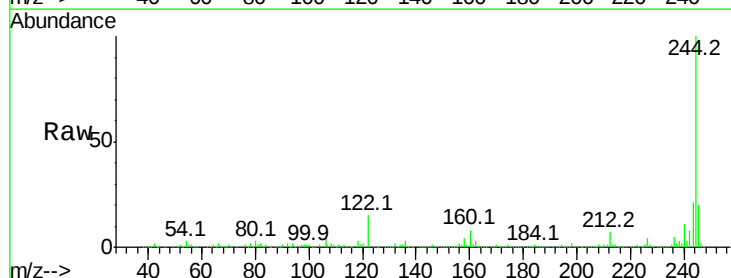


Abundance Ion 244.00 (243.70 to 244.70): E

Ion 212.00 (211.70 to 212.70): E

Ion 122.00 (121.70 to 122.70): E

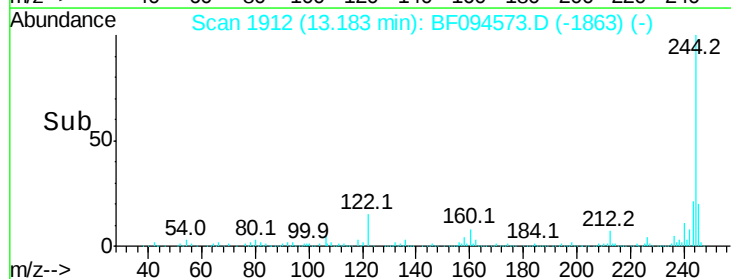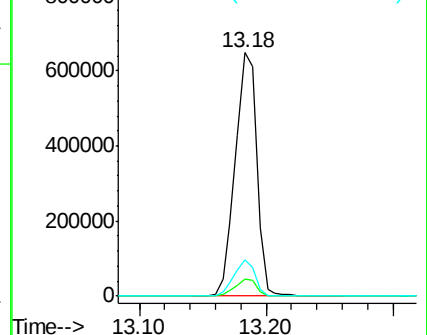


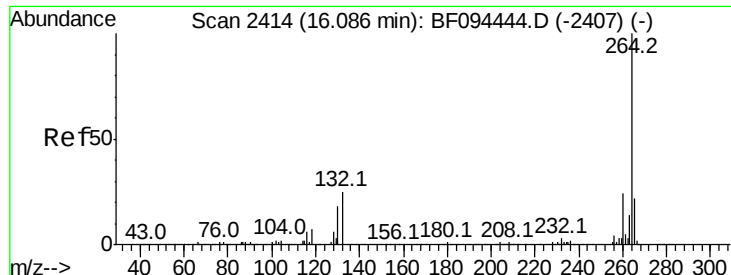

#86
Pervlene-d12
Concen: 20.00 ng
RT: 16.08 min Scan# 2404
Delta R.T. -0.01 min
Lab File: BF094573.D
Acq: 21 Apr 2017 20:09

Instrument :
BNA_F
ClientSampleId :

Tot Ion	Ratio	Lower	Upper
264	100		
260	24.0	19.5	29.3
265	21.8	17.2	25.8

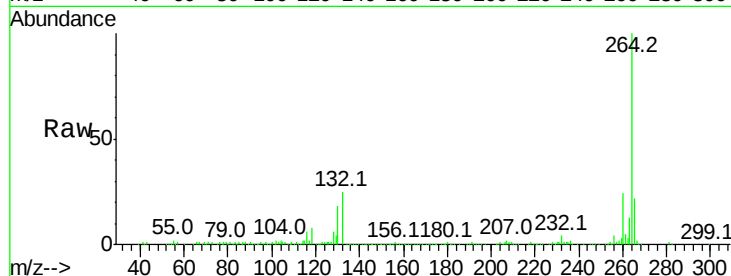

Abundance Ion 264.00 (263.70 to 264.70): E
Ion 260.00 (259.70 to 260.70): E
Ion 265.00 (264.70 to 265.70): E

